

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019147.D
 Acq On : 29 Dec 2023 04:27
 Operator : MA/JU
 Sample : 05986-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	30	rVB	35494	40143	0.74%	0.099%
2	3.658	94	97	105	rBV	130804	187365	3.45%	0.463%
3	3.881	132	135	139	rVB4	6541	8096	0.15%	0.020%
4	3.976	147	151	155	rBV3	12192	16910	0.31%	0.042%
5	4.899	305	308	312	rBV4	4398	6367	0.12%	0.016%
6	6.981	656	662	673	rVB	116360	194084	3.58%	0.480%
7	7.140	683	689	701	rBV	520865	803865	14.81%	1.988%
8	7.334	715	722	733	rBV	474033	739175	13.62%	1.828%
9	7.805	795	802	812	rBV	600027	960155	17.69%	2.375%
10	8.522	916	924	934	rBV	348149	573737	10.57%	1.419%
11	8.969	990	1000	1011	rBV	561836	935273	17.23%	2.313%
12	9.375	1063	1069	1074	rVB5	9169	17078	0.31%	0.042%
13	9.687	1113	1122	1136	rBV	431301	704814	12.99%	1.743%
14	10.222	1206	1213	1230	rBV	649573	1125523	20.74%	2.784%
15	10.599	1269	1277	1287	rBV	791094	1293174	23.83%	3.199%
16	10.746	1295	1302	1317	rBV	450929	796367	14.67%	1.970%
17	11.410	1406	1415	1417	rBV10	3848	9303	0.17%	0.023%
18	11.863	1487	1492	1499	rVB7	6051	12518	0.23%	0.031%
19	12.199	1542	1549	1558	rBV3	11112	24131	0.44%	0.060%
20	12.722	1633	1638	1640	rBV6	3642	5522	0.10%	0.014%
21	12.810	1648	1653	1655	rBV6	4375	6743	0.12%	0.017%
22	13.057	1688	1695	1700	rBV6	3397	6967	0.13%	0.017%
23	13.346	1739	1744	1749	rBV4	13790	21573	0.40%	0.053%
24	13.863	1826	1832	1844	rBV	1444144	1923222	35.44%	4.757%
25	14.140	1870	1879	1893	rBV	1474039	2160915	39.82%	5.345%
26	14.446	1923	1931	1941	rBV	1193009	1746050	32.17%	4.319%
27	14.669	1964	1969	1981	rBV	70169	147936	2.73%	0.366%
28	14.869	1997	2003	2005	rBV7	4717	7621	0.14%	0.019%
29	15.440	2091	2100	2108	rBV	2041836	3000340	55.29%	7.422%
30	15.569	2115	2122	2137	rBV	620382	847987	15.63%	2.098%
31	15.687	2137	2142	2148	rVB5	9479	17589	0.32%	0.044%
32	15.816	2159	2164	2168	rBV	64616	84960	1.57%	0.210%
33	16.010	2194	2197	2203	rVB8	3977	5851	0.11%	0.014%
34	16.181	2219	2226	2231	rBV4	16990	32968	0.61%	0.082%
35	16.228	2231	2234	2240	rVB6	10544	15089	0.28%	0.037%
36	16.293	2241	2245	2248	rBV3	10859	14862	0.27%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019147.D
 Acq On : 29 Dec 2023 04:27
 Operator : MA/JU
 Sample : 05986-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	16.375	2256	2259	2263	rVB5	3276	5804	0.11%	0.014%
38	16.869	2338	2343	2344	rBV5	5920	7952	0.15%	0.020%
39	17.016	2365	2368	2371	rBV6	3356	5861	0.11%	0.014%
40	17.081	2376	2379	2383	rBV6	6748	9668	0.18%	0.024%
41	17.204	2393	2400	2407	rBV	1572575	2181226	40.19%	5.395%
42	17.304	2410	2417	2427	rVV	2436070	3556048	65.53%	8.796%
43	17.869	2511	2513	2518	rVB6	6474	10930	0.20%	0.027%
44	18.098	2547	2552	2559	rBV	92066	123962	2.28%	0.307%
45	18.981	2700	2702	2709	rVB7	10255	13975	0.26%	0.035%
46	19.122	2722	2726	2733	rBV	38995	59478	1.10%	0.147%
47	19.192	2734	2738	2741	rBV	35500	46020	0.85%	0.114%
48	19.339	2759	2763	2767	rBV3	44055	60748	1.12%	0.150%
49	19.545	2792	2798	2806	rBV	3402617	4667367	86.00%	11.545%
50	21.304	3093	3097	3103	rBV	2042343	2715655	50.04%	6.717%
51	23.522	3466	3474	3489	rBV2	2786273	5426887	100.00%	13.424%
52	23.674	3493	3500	3511	rVB	1491757	3040938	56.03%	7.522%




Sum of corrected areas: 40426792

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019147.D
Acq On : 29 Dec 2023 04:27
Operator : MA/JU
Sample : 05986-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

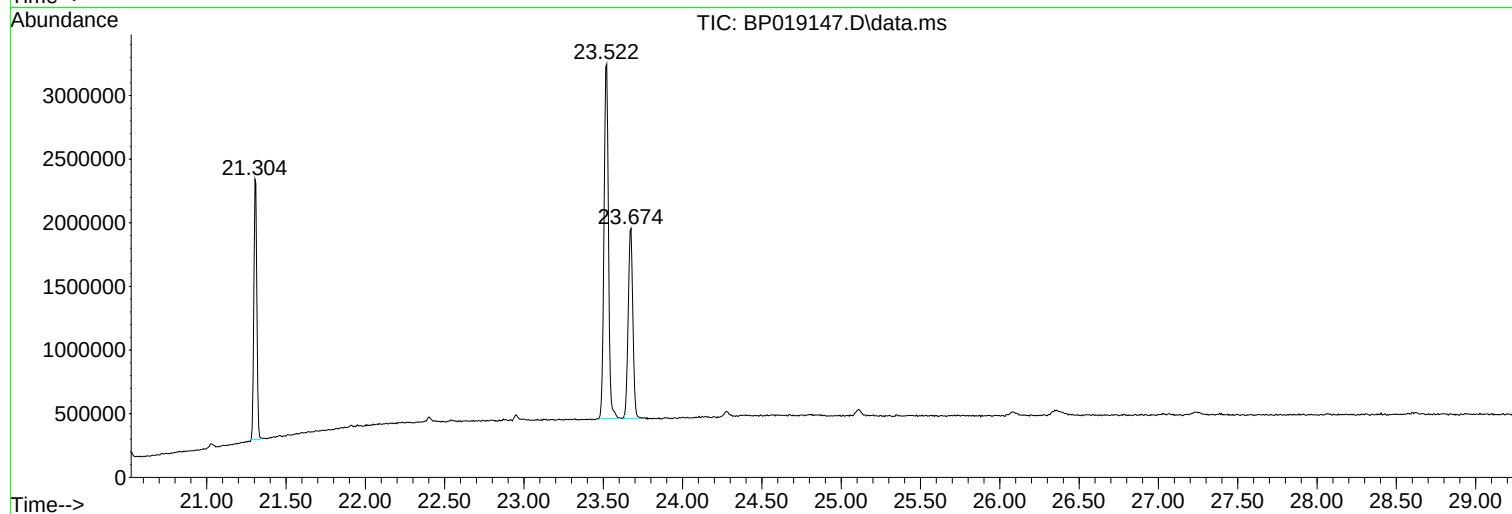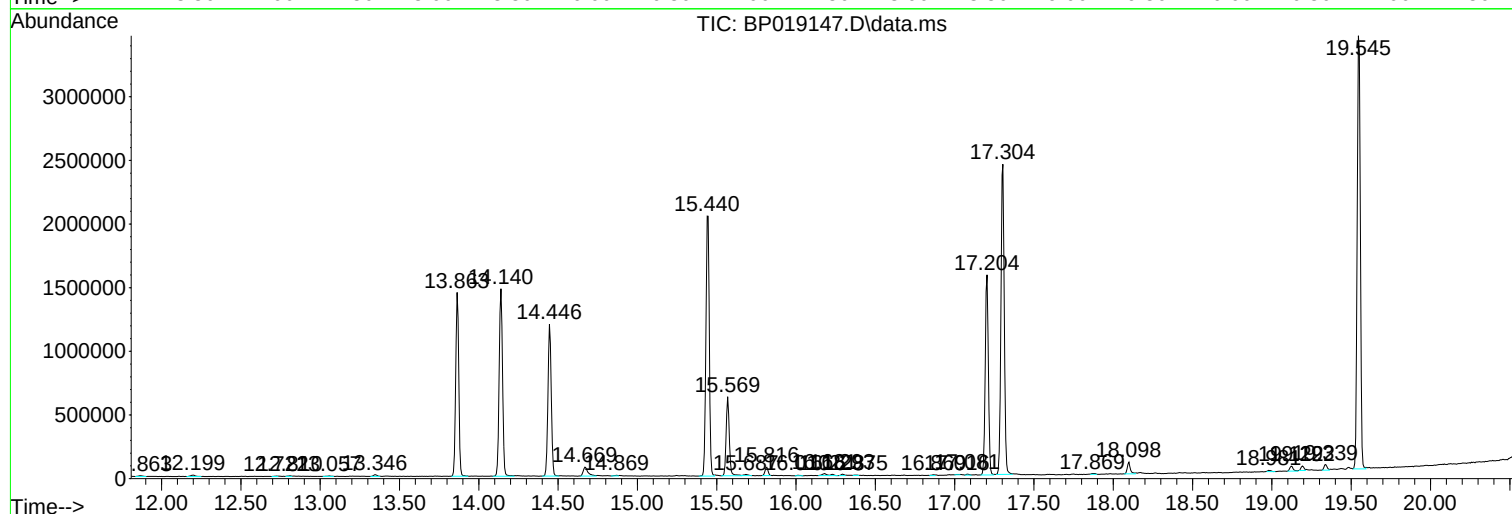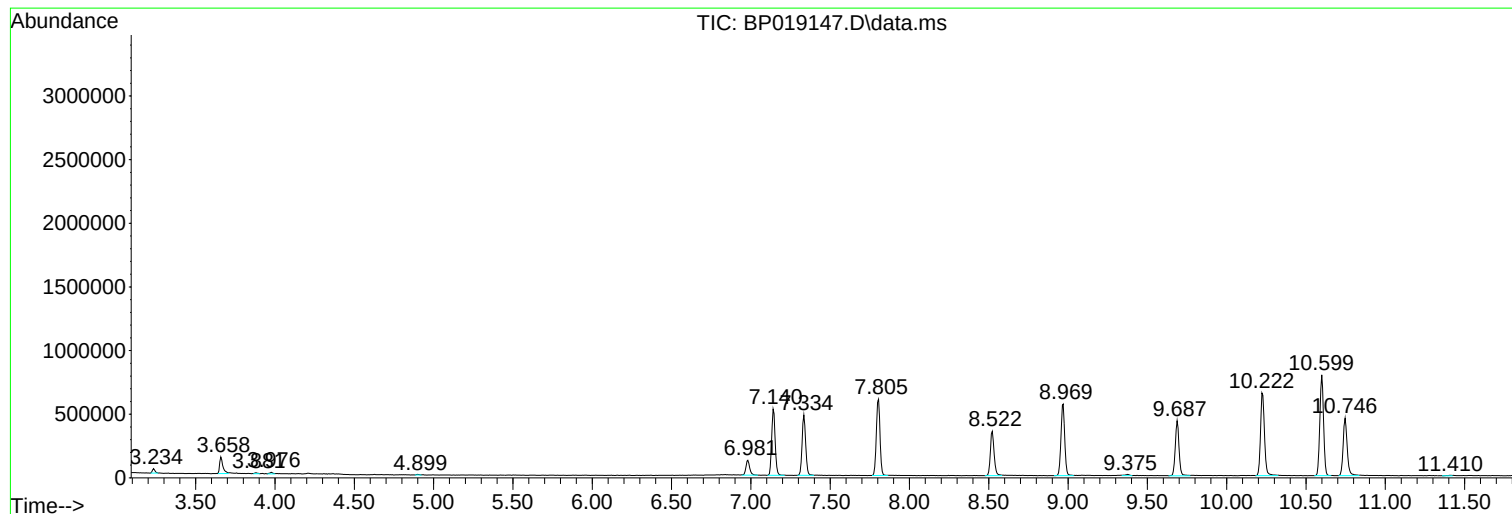

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019147.D
Acq On : 29 Dec 2023 04:27
Operator : MA/JU
Sample : 05986-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019147.D
Acq On : 29 Dec 2023 04:27
Operator : MA/JU
Sample : 05986-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
