

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019149.D
 Acq On : 29 Dec 2023 05:35
 Operator : MA/JU
 Sample : 05986-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	29	rBV	42911	47123	0.66%	0.096%
2	3.658	93	97	106	rBV	199896	298074	4.15%	0.610%
3	3.881	133	135	141	rVB4	7108	10169	0.14%	0.021%
4	3.975	148	151	159	rVB	10716	16640	0.23%	0.034%
5	4.905	305	309	313	rBV3	5253	7855	0.11%	0.016%
6	5.081	335	339	347	rVB	23814	34790	0.48%	0.071%
7	5.858	464	471	477	rVB9	6042	11148	0.16%	0.023%
8	6.981	656	662	674	rVB	168628	273656	3.81%	0.560%
9	7.140	683	689	698	rBV	706156	1081660	15.05%	2.212%
10	7.334	715	722	735	rBV	656145	1011939	14.08%	2.070%
11	7.805	795	802	810	rBV	586240	920683	12.81%	1.883%
12	8.522	916	924	941	rBV	458917	758280	10.55%	1.551%
13	8.969	992	1000	1011	rBV	766958	1261193	17.55%	2.580%
14	9.093	1015	1021	1028	rBV9	5645	12781	0.18%	0.026%
15	9.375	1064	1069	1074	rVB2	10498	16914	0.24%	0.035%
16	9.687	1113	1122	1135	rBV	589786	974918	13.56%	1.994%
17	10.222	1206	1213	1227	rBV	891508	1514653	21.07%	3.098%
18	10.599	1266	1277	1285	rBV	778358	1254855	17.46%	2.567%
19	10.746	1292	1302	1317	rBV	658679	1132430	15.76%	2.316%
20	11.428	1410	1418	1424	rBV3	15589	32149	0.45%	0.066%
21	11.863	1488	1492	1499	rVB8	6843	12663	0.18%	0.026%
22	12.193	1543	1548	1557	rBV2	16523	30187	0.42%	0.062%
23	13.345	1740	1744	1749	rBV3	11365	18261	0.25%	0.037%
24	13.863	1826	1832	1840	rBV	1778592	2486752	34.60%	5.086%
25	14.140	1871	1879	1893	rBV	2064700	2954358	41.11%	6.043%
26	14.316	1903	1909	1913	rBV5	13671	20090	0.28%	0.041%
27	14.445	1923	1931	1939	rBV	1145723	1653993	23.01%	3.383%
28	14.669	1961	1969	1983	rBV	99834	217653	3.03%	0.445%
29	14.875	1999	2004	2012	rVB	6370	13200	0.18%	0.027%
30	15.439	2094	2100	2107	rBV	2714050	3951118	54.98%	8.081%
31	15.492	2107	2109	2114	rVV2	27419	35526	0.49%	0.073%
32	15.569	2116	2122	2136	rVV	872939	1178900	16.40%	2.411%
33	15.686	2138	2142	2149	rVB2	14570	24389	0.34%	0.050%
34	15.816	2158	2164	2168	rBV	35254	50028	0.70%	0.102%
35	16.234	2230	2235	2240	rVB4	11840	18069	0.25%	0.037%
36	17.204	2393	2400	2410	rBV	1402546	1993575	27.74%	4.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019149.D
 Acq On : 29 Dec 2023 05:35
 Operator : MA/JU
 Sample : 05986-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	17.304	2410	2417	2428	rVV	3257578	4606750	64.10%	9.422%
38	17.386	2429	2431	2437	rVB7	7789	12668	0.18%	0.026%
39	17.980	2525	2532	2537	rBV10	5446	13741	0.19%	0.028%
40	18.098	2548	2552	2559	rBV	128131	175321	2.44%	0.359%
41	18.575	2631	2633	2637	rVB4	12805	13636	0.19%	0.028%
42	19.122	2722	2726	2731	rBV2	47166	61170	0.85%	0.125%
43	19.192	2734	2738	2741	rBV	50524	70536	0.98%	0.144%
44	19.333	2759	2762	2772	rBV2	66166	97348	1.35%	0.199%
45	19.480	2785	2787	2791	rVB4	12193	14073	0.20%	0.029%
46	19.545	2792	2798	2808	rBV	4389802	5991746	83.37%	12.255%
47	21.304	3092	3097	3104	rBV	2020657	2502282	34.82%	5.118%
48	23.515	3466	3473	3491	rVB2	3696724	7187033	100.00%	14.700%
49	23.668	3493	3499	3513	rVB	1389489	2815179	39.17%	5.758%




Sum of corrected areas: 48892155

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019149.D
Acq On : 29 Dec 2023 05:35
Operator : MA/JU
Sample : 05986-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

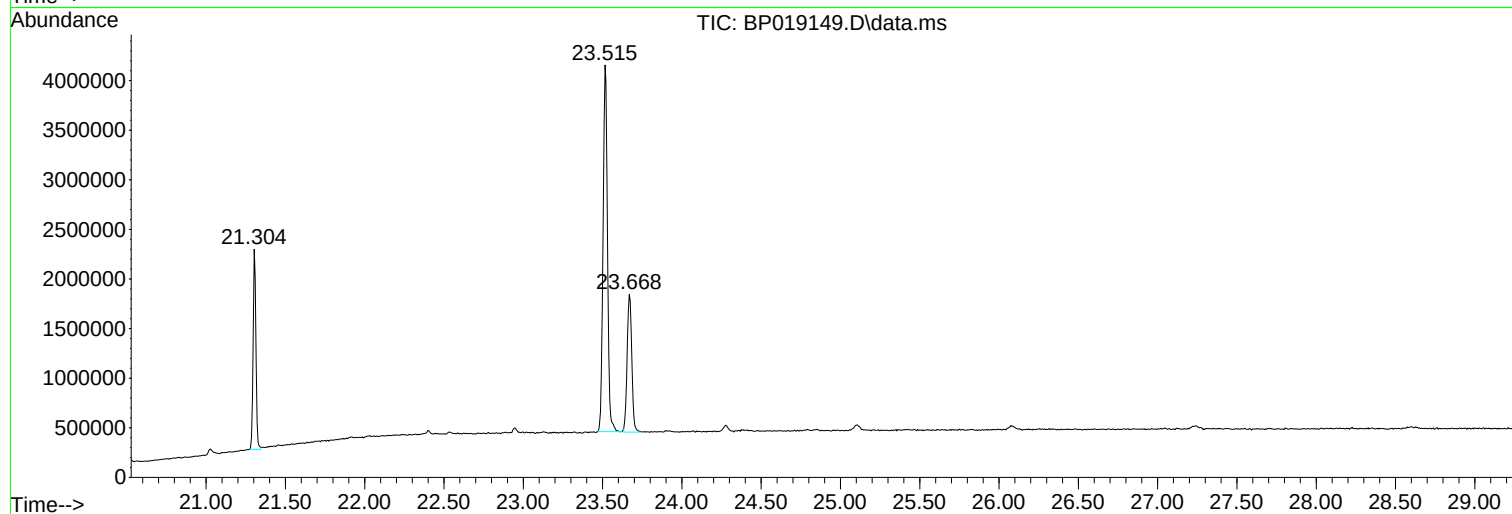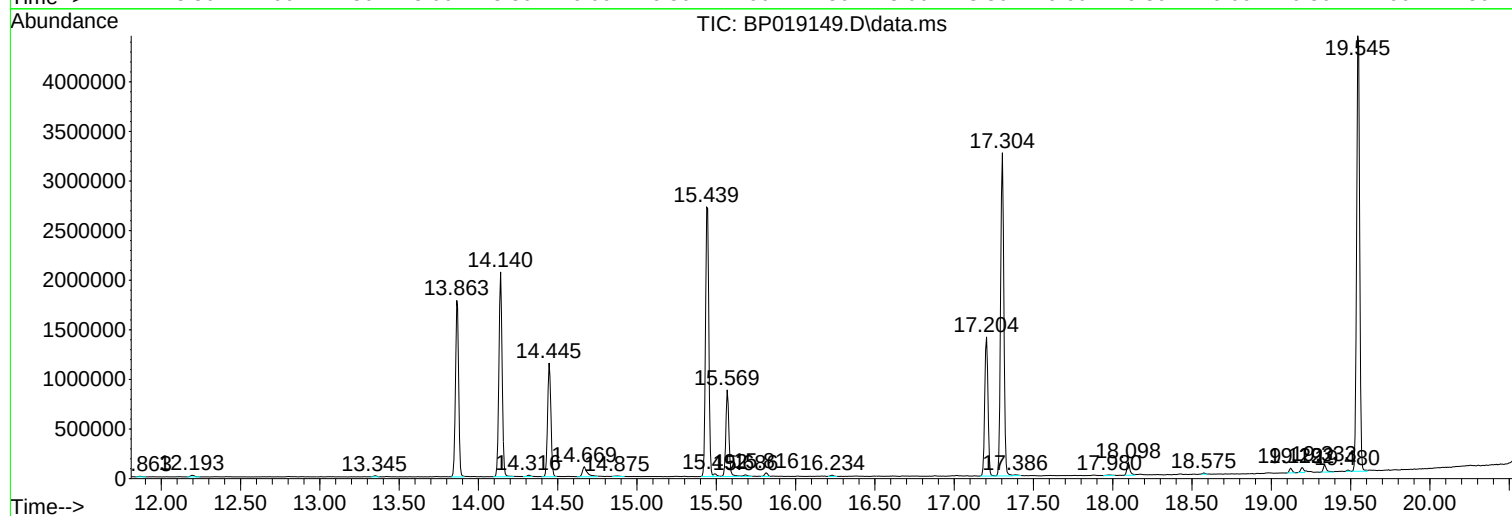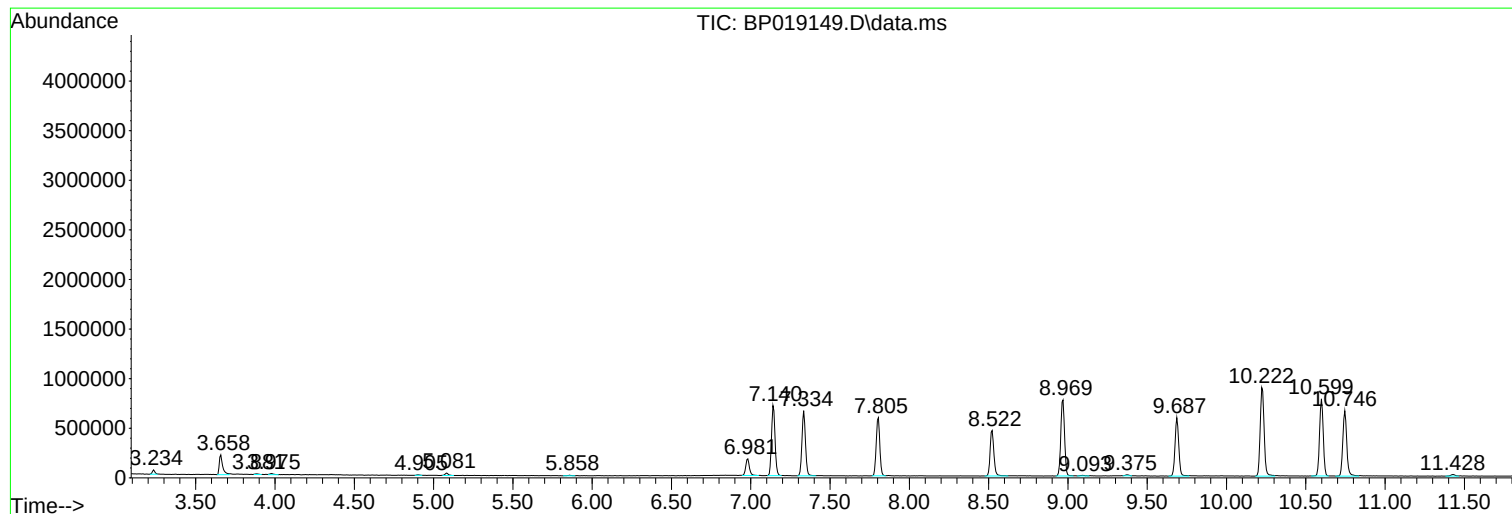

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019149.D
Acq On : 29 Dec 2023 05:35
Operator : MA/JU
Sample : 05986-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019149.D
Acq On : 29 Dec 2023 05:35
Operator : MA/JU
Sample : 05986-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
