

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019155.D
 Acq On : 29 Dec 2023 08:59
 Operator : MA/JU
 Sample : 06021-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	31	rVB	45316	55163	0.78%	0.111%
2	3.658	93	97	113	rBV	265123	388602	5.48%	0.784%
3	3.881	131	135	141	rBV2	11610	17873	0.25%	0.036%
4	3.975	148	151	157	rVB	12457	17635	0.25%	0.036%
5	4.899	304	308	310	rBV3	7052	7793	0.11%	0.016%
6	6.981	656	662	671	rVB	211093	341820	4.82%	0.690%
7	7.140	683	689	698	rBV	704377	1108586	15.62%	2.237%
8	7.334	715	722	733	rBV	715544	1119671	15.78%	2.260%
9	7.805	794	802	810	rBV	628957	1000117	14.09%	2.018%
10	8.522	916	924	937	rBV	566707	925967	13.05%	1.869%
11	8.963	991	999	1011	rBV	765484	1278283	18.01%	2.580%
12	9.087	1015	1020	1025	rVV6	7883	14036	0.20%	0.028%
13	9.375	1065	1069	1075	rVB3	9623	15948	0.22%	0.032%
14	9.687	1114	1122	1139	rBV	608533	1001959	14.12%	2.022%
15	10.222	1205	1213	1229	rBV	906597	1578507	22.24%	3.185%
16	10.599	1270	1277	1285	rBV	794685	1292621	18.21%	2.609%
17	10.746	1294	1302	1316	rBV	709263	1226702	17.29%	2.476%
18	11.869	1486	1493	1499	rVB5	7066	13939	0.20%	0.028%
19	12.199	1543	1549	1555	rVB	15216	25427	0.36%	0.051%
20	12.810	1647	1653	1657	rBV8	3891	7612	0.11%	0.015%
21	13.346	1739	1744	1750	rVB7	6452	11665	0.16%	0.024%
22	13.863	1826	1832	1842	rBV	1797399	2460312	34.67%	4.965%
23	14.140	1870	1879	1895	rBV	2009634	2896113	40.81%	5.844%
24	14.445	1923	1931	1939	rBV	1191048	1696620	23.91%	3.424%
25	14.669	1963	1969	1983	rBV	129202	259419	3.66%	0.524%
26	14.881	1999	2005	2010	rVB10	6034	13232	0.19%	0.027%
27	15.204	2055	2060	2063	rBV6	4199	7312	0.10%	0.015%
28	15.445	2094	2101	2114	rBV	2723335	3810149	53.69%	7.689%
29	15.569	2116	2122	2135	rVV	833463	1127518	15.89%	2.275%
30	15.687	2138	2142	2153	rVB6	13318	26951	0.38%	0.054%
31	16.169	2221	2224	2230	rVV7	4568	7127	0.10%	0.014%
32	16.228	2230	2234	2239	rVB5	11264	16652	0.23%	0.034%
33	16.881	2342	2345	2352	rVB8	5539	9692	0.14%	0.020%
34	17.022	2365	2369	2374	rBV4	9052	12768	0.18%	0.026%
35	17.204	2393	2400	2410	rBV	1520668	2097424	29.55%	4.233%
36	17.304	2410	2417	2426	rBV	3275652	4511356	63.57%	9.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019155.D
Acq On : 29 Dec 2023 08:59
Operator : MA/JU
Sample : 06021-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	17.881	2512	2515	2519	rVB6	8508	10587	0.15%	0.021%
38	18.098	2548	2552	2560	rBV	108704	153234	2.16%	0.309%
39	18.516	2619	2623	2626	rBV3	19728	23751	0.33%	0.048%
40	19.122	2722	2726	2731	rBV	45479	62258	0.88%	0.126%
41	19.198	2735	2739	2742	rBV	42792	61387	0.86%	0.124%
42	19.339	2759	2763	2769	rBV3	51437	75691	1.07%	0.153%
43	19.551	2793	2799	2807	rBV	4331632	5795287	81.66%	11.695%
44	21.028	3047	3050	3057	rBV3	65879	113266	1.60%	0.229%
45	21.304	3093	3097	3105	rBV	2082071	2686702	37.86%	5.422%
46	23.521	3466	3474	3488	rVB2	3613832	7096888	100.00%	14.322%
47	23.674	3493	3500	3512	rVB	1505865	3071736	43.28%	6.199%




Sum of corrected areas: 49553358

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019155.D
Acq On : 29 Dec 2023 08:59
Operator : MA/JU
Sample : 06021-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

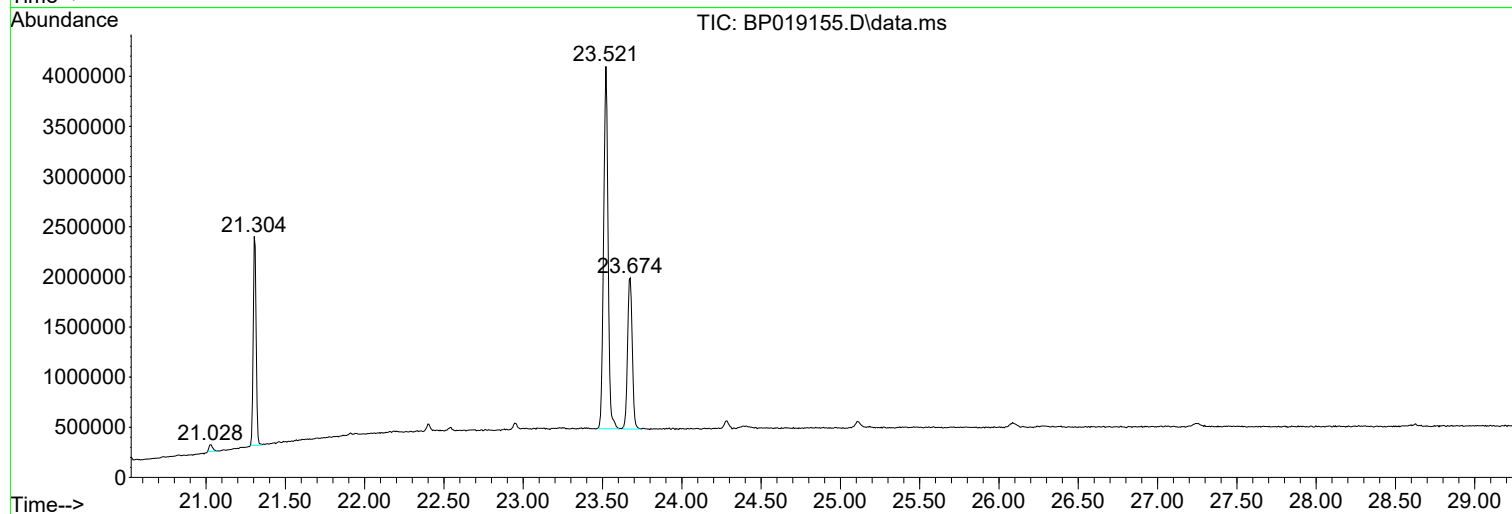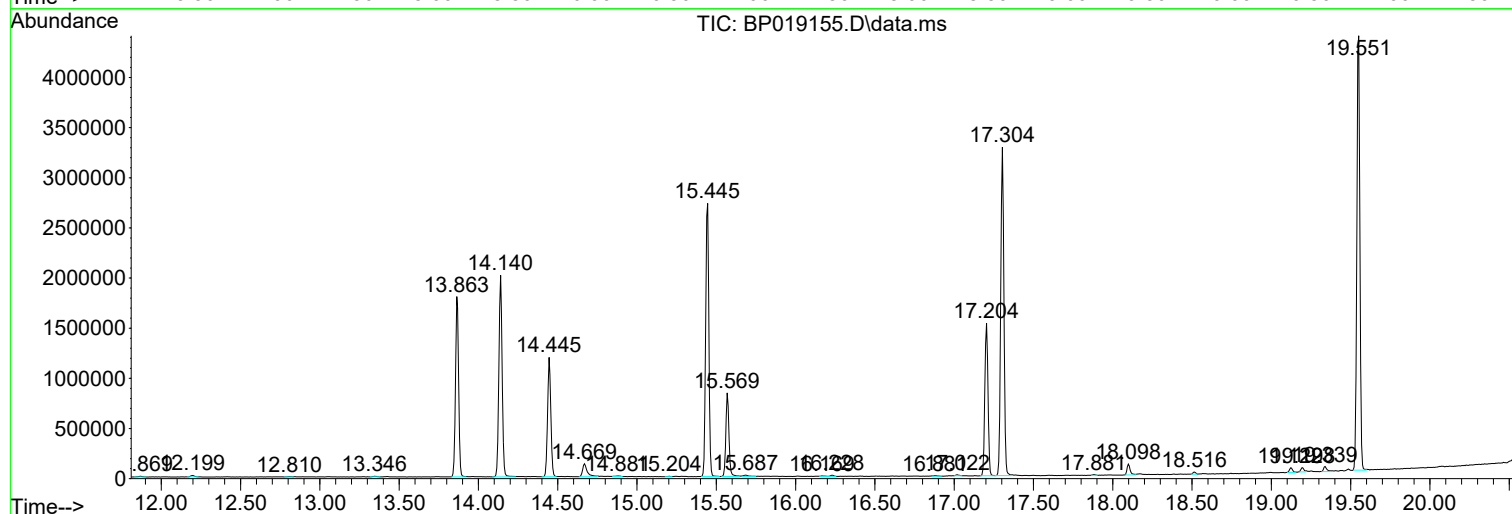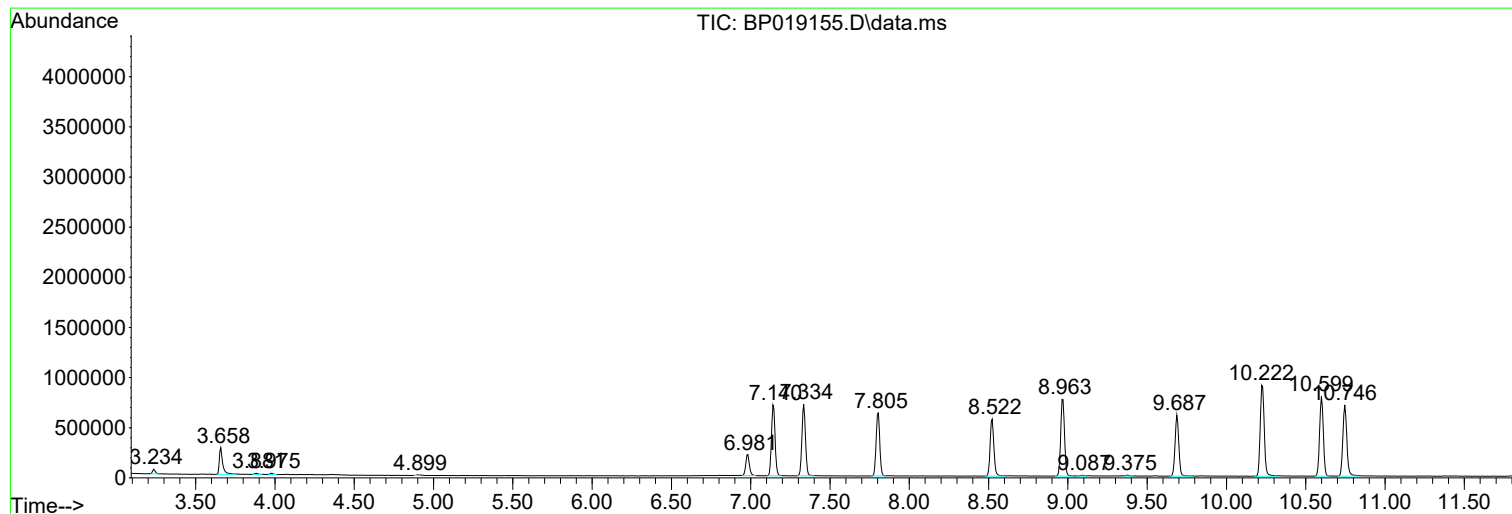

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019155.D
Acq On : 29 Dec 2023 08:59
Operator : MA/JU
Sample : 06021-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019155.D
Acq On : 29 Dec 2023 08:59
Operator : MA/JU
Sample : 06021-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc