

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019162.D
 Acq On : 29 Dec 2023 12:58
 Operator : MA/JU
 Sample : PB158078BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK078

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.886	430	435	446	rVV	150356	229272	5.70%	0.664%
2	2.968	446	449	454	rVB	45558	52082	1.29%	0.151%
3	3.233	491	494	502	rVB	36999	46605	1.16%	0.135%
4	3.651	561	565	583	rBV	460036	687176	17.07%	1.990%
5	6.980	1124	1131	1141	rBV	543598	853194	21.20%	2.471%
6	7.145	1153	1159	1175	rVB	451534	694498	17.25%	2.011%
7	7.333	1184	1191	1201	rBV	531934	840718	20.89%	2.435%
8	7.803	1263	1271	1281	rBV	513160	784013	19.48%	2.271%
9	8.521	1386	1393	1407	rBV	639296	1031751	25.63%	2.988%
10	8.968	1459	1469	1476	rBV	461657	736318	18.29%	2.133%
11	9.691	1585	1592	1600	rBV	235693	396957	9.86%	1.150%
12	10.227	1675	1683	1703	rBV	596736	1047104	26.01%	3.033%
13	10.597	1737	1746	1756	rVB	649792	1088748	27.05%	3.153%
14	10.744	1764	1771	1787	rBV	606256	1072165	26.64%	3.105%
15	13.868	2295	2302	2312	rBV	1051203	1474052	36.62%	4.269%
16	14.138	2339	2348	2360	rBV	1286389	1843651	45.80%	5.340%
17	14.444	2394	2400	2409	rBV	962500	1449668	36.01%	4.199%
18	14.662	2431	2437	2461	rBV	298124	551129	13.69%	1.596%
19	15.444	2563	2570	2579	rBV	1725394	2388024	59.32%	6.916%
20	15.573	2585	2592	2600	rBV	210376	328780	8.17%	0.952%
21	17.203	2863	2869	2879	rBV	1292279	1826895	45.38%	5.291%
22	17.303	2879	2886	2898	rBV	1882371	2634703	65.45%	7.631%
23	19.126	3191	3196	3201	rBV3	26132	41315	1.03%	0.120%
24	19.197	3204	3208	3211	rBV	18470	28307	0.70%	0.082%
25	19.550	3262	3268	3278	rBV	2556609	3369597	83.71%	9.759%
26	21.308	3562	3567	3574	rBV	1893947	2344093	58.23%	6.789%
27	23.520	3936	3943	3959	rVB	2162090	4025373	100.00%	11.658%
28	23.673	3963	3969	3984	rVB	1370373	2661191	66.11%	7.707%




Sum of corrected areas: 34527379

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019162.D
Acq On : 29 Dec 2023 12:58
Operator : MA/JU
Sample : PB158078BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

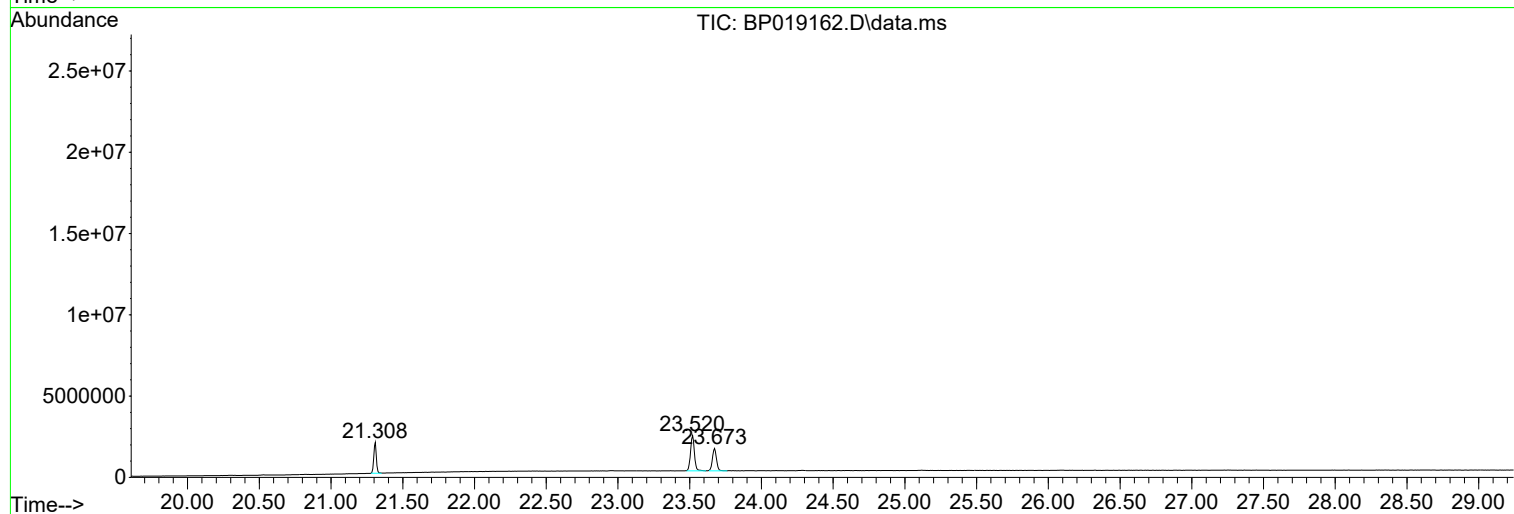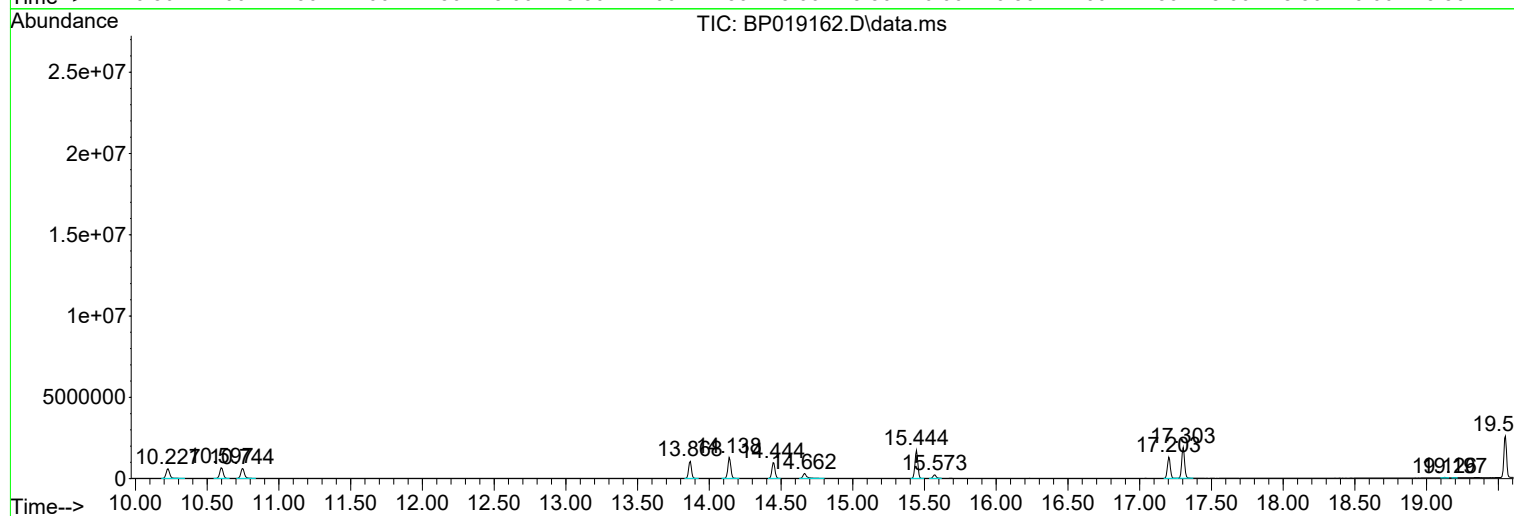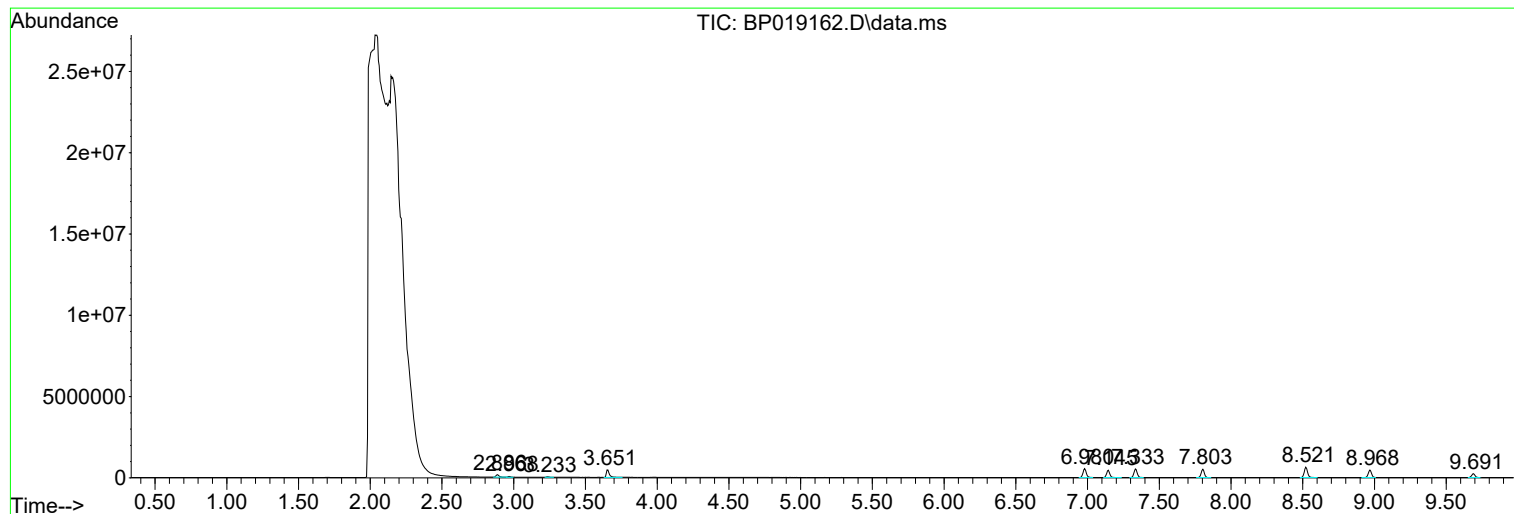

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019162.D
Acq On : 29 Dec 2023 12:58
Operator : MA/JU
Sample : PB158078BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic2.886 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.886	5.85 ng/ul	229272	1,4-Dichlorobenzene-d4	7.803

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	95
2			Cyclohexane	84	C6H12	000110-82-7	91
3			Cyclohexane	84	C6H12	000110-82-7	91
4			Cyclohexane	84	C6H12	000110-82-7	87
5			Cyclopentane, methyl-	84	C6H12	000096-37-7	83

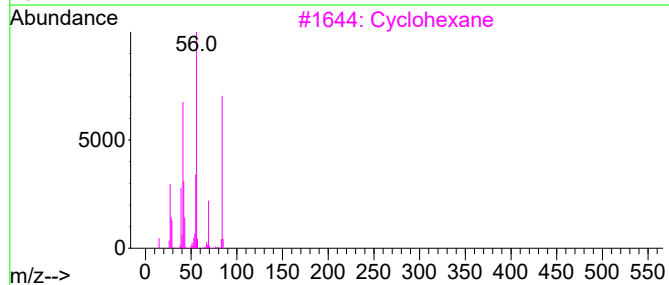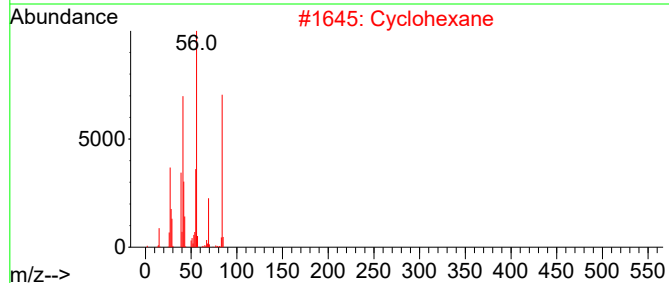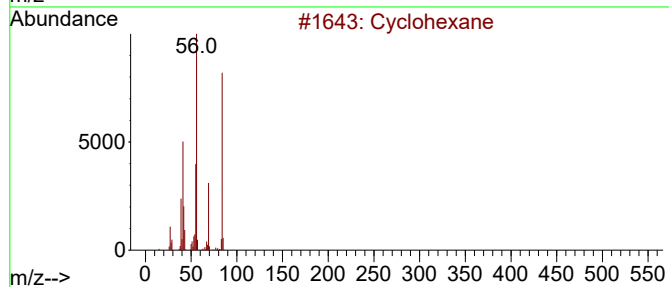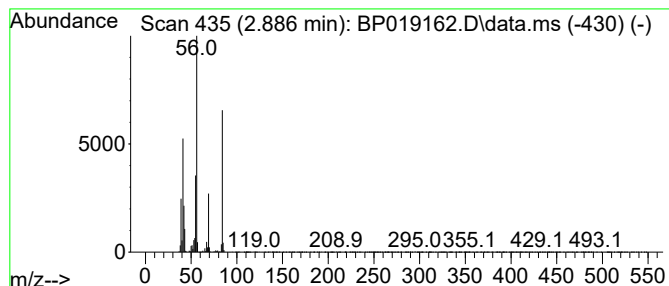

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019162.D
Acq On : 29 Dec 2023 12:58
Operator : MA/JU
Sample : PB158078BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK078

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	2.886	5.8	ng/ul	229272	1	7.803	784013	20.0