

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019163.D
 Acq On : 29 Dec 2023 13:32
 Operator : MA/JU
 Sample : PB158068BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019163.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	33	rVB	66797	84398	1.36%	0.159%
2	3.652	92	96	116	rBV	776555	1169891	18.87%	2.205%
3	3.975	148	151	157	rVB	12320	15161	0.24%	0.029%
4	6.981	655	662	674	rVB	824238	1313434	21.19%	2.475%
5	7.146	683	690	703	rVB	671894	1067830	17.23%	2.012%
6	7.334	715	722	731	rBV	850549	1310415	21.14%	2.470%
7	7.805	793	802	814	rBV	706834	1140617	18.40%	2.150%
8	8.522	915	924	937	rBV	1006387	1601029	25.83%	3.017%
9	8.969	992	1000	1011	rBV	728414	1161810	18.74%	2.190%
10	9.687	1114	1122	1133	rBV	469621	763202	12.31%	1.438%
11	10.222	1206	1213	1226	rBV	933806	1603934	25.88%	3.023%
12	10.599	1269	1277	1290	rVB	944319	1575573	25.42%	2.969%
13	10.746	1290	1302	1319	rBV	945417	1644896	26.54%	3.100%
14	12.198	1543	1549	1556	rBV	14366	29761	0.48%	0.056%
15	13.345	1739	1744	1749	rBV3	12148	20277	0.33%	0.038%
16	13.428	1753	1758	1763	rVV8	3442	6492	0.10%	0.012%
17	13.863	1826	1832	1844	rBV	1667300	2391756	38.59%	4.508%
18	14.140	1872	1879	1894	rBV	2016229	2879944	46.46%	5.428%
19	14.445	1924	1931	1942	rBV	1478327	2146220	34.62%	4.045%
20	14.663	1959	1968	1989	rBV	634762	1039604	16.77%	1.959%
21	14.875	1999	2004	2008	rVB8	3479	6965	0.11%	0.013%
22	15.445	2094	2101	2111	rBV	2585353	3723262	60.07%	7.017%
23	15.569	2116	2122	2134	rVV	455716	670351	10.81%	1.263%
24	15.687	2136	2142	2147	rVB3	11546	21863	0.35%	0.041%
25	16.228	2230	2234	2239	rVB5	8576	13713	0.22%	0.026%
26	16.881	2341	2345	2350	rBV8	5584	9122	0.15%	0.017%
27	16.992	2359	2364	2366	rBV4	4560	6363	0.10%	0.012%
28	17.204	2393	2400	2408	rBV	1963551	2705458	43.65%	5.099%
29	17.304	2410	2417	2431	rVV	2926744	4148506	66.93%	7.818%
30	18.098	2549	2552	2558	rBV6	9741	14079	0.23%	0.027%
31	19.128	2722	2727	2731	rBV2	38959	56674	0.91%	0.107%
32	19.192	2735	2738	2742	rVV2	33269	42600	0.69%	0.080%
33	19.339	2760	2763	2768	rBV5	11930	18527	0.30%	0.035%
34	19.545	2792	2798	2807	rBV	3840581	5201526	83.91%	9.803%
35	21.310	3092	3098	3106	rBV	2582877	3417195	55.13%	6.440%
36	23.521	3466	3474	3487	rBV2	3130654	6198642	100.00%	11.682%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019163.D
Acq On : 29 Dec 2023 13:32
Operator : MA/JU
Sample : PB158068BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK068

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	23.668	3493	3499	3512	rVB	1975291	3840137	61.95%	7.237%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 53061227

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019163.D
Acq On : 29 Dec 2023 13:32
Operator : MA/JU
Sample : PB158068BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

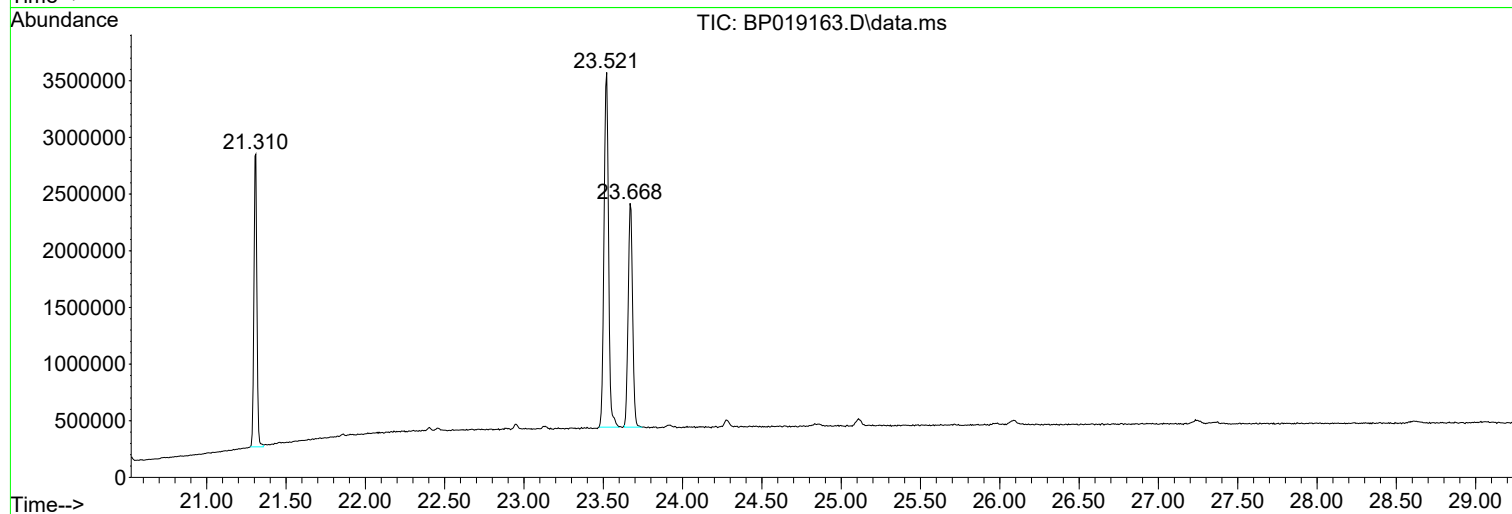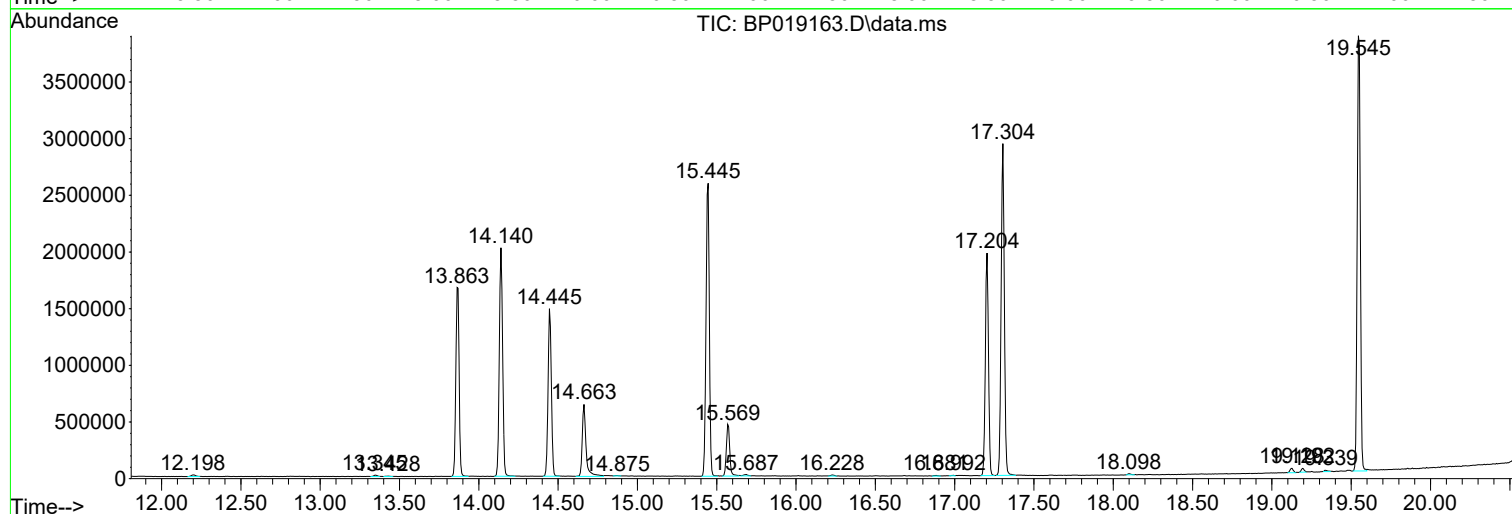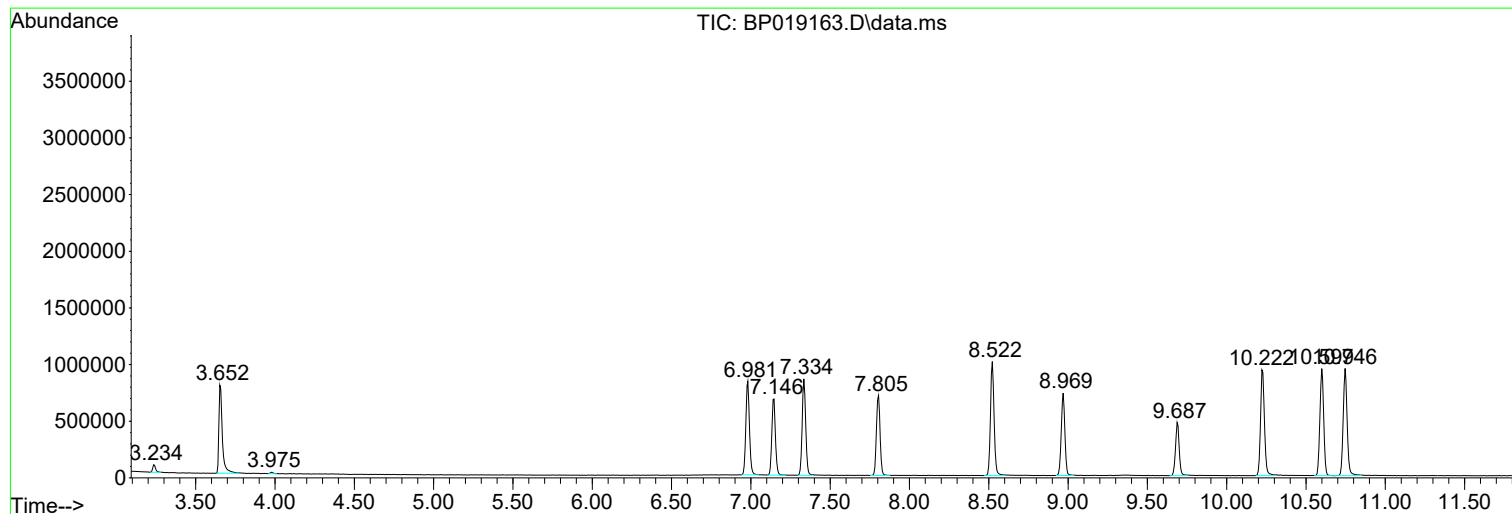

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019163.D
Acq On : 29 Dec 2023 13:32
Operator : MA/JU
Sample : PB158068BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019163.D
Acq On : 29 Dec 2023 13:32
Operator : MA/JU
Sample : PB158068BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK068

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------