

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019166.D
 Acq On : 29 Dec 2023 15:15
 Operator : MA/JU
 Sample : 06021-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	14	19	23	rBV	236007	332596	5.32%	0.726%
2	3.234	23	25	39	rVB	61157	79887	1.28%	0.174%
3	3.528	72	75	81	rBV	13270	18946	0.30%	0.041%
4	3.658	93	97	107	rBV	187935	278517	4.45%	0.608%
5	3.975	148	151	156	rBV	12123	15202	0.24%	0.033%
6	4.423	223	227	238	rVB2	35212	50688	0.81%	0.111%
7	4.805	287	292	298	rVB2	15060	23314	0.37%	0.051%
8	4.899	304	308	313	rBV2	5821	9415	0.15%	0.021%
9	6.981	656	662	670	rVB	169876	272116	4.35%	0.594%
10	7.140	683	689	702	rVB	685158	1061303	16.97%	2.316%
11	7.334	715	722	735	rBV	658861	1027890	16.43%	2.243%
12	7.799	794	801	808	rBV	605739	973451	15.56%	2.124%
13	8.516	916	923	939	rBV	471499	786184	12.57%	1.716%
14	8.963	991	999	1010	rBV	717085	1164151	18.61%	2.541%
15	9.369	1064	1068	1076	rVB8	6749	13219	0.21%	0.029%
16	9.546	1095	1098	1104	rVB8	3815	6954	0.11%	0.015%
17	9.687	1115	1122	1134	rBV	506451	825498	13.20%	1.802%
18	10.222	1206	1213	1224	rBV	839953	1419954	22.70%	3.099%
19	10.599	1269	1277	1287	rVB	787564	1277943	20.43%	2.789%
20	10.746	1295	1302	1318	rBV	695478	1246558	19.93%	2.720%
21	11.375	1402	1409	1414	rBV6	7433	19132	0.31%	0.042%
22	12.193	1544	1548	1558	rVB2	14922	26236	0.42%	0.057%
23	12.804	1646	1652	1658	rVB10	4315	9149	0.15%	0.020%
24	13.346	1739	1744	1751	rVB2	17477	27952	0.45%	0.061%
25	13.863	1826	1832	1842	rBV	1507631	2021558	32.32%	4.412%
26	13.975	1847	1851	1858	rVB10	5159	8289	0.13%	0.018%
27	14.140	1869	1879	1897	rBV	1769949	2600109	41.56%	5.674%
28	14.446	1924	1931	1941	rBV	1081375	1578393	25.23%	3.445%
29	14.669	1960	1969	1983	rBV	1001815	2261325	36.15%	4.935%
30	15.198	2056	2059	2064	rVB3	6333	7687	0.12%	0.017%
31	15.440	2093	2100	2107	rBV	2300758	3306687	52.86%	7.216%
32	15.569	2115	2122	2133	rBV	518887	716434	11.45%	1.563%
33	15.681	2137	2141	2149	rVB4	12287	22574	0.36%	0.049%
34	16.004	2193	2196	2199	rBV5	3666	6309	0.10%	0.014%
35	16.228	2231	2234	2241	rVB4	8606	12842	0.21%	0.028%
36	16.610	2295	2299	2305	rBV9	6496	10081	0.16%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019166.D
 Acq On : 29 Dec 2023 15:15
 Operator : MA/JU
 Sample : 06021-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	17.016	2364	2368	2374	rVB2	18807	29832	0.48%	0.065%
38	17.204	2393	2400	2410	rBV	1265825	1822463	29.13%	3.977%
39	17.298	2410	2416	2428	rBV	2639904	3850808	61.56%	8.404%
40	17.881	2511	2515	2521	rVB6	11112	14614	0.23%	0.032%
41	17.975	2527	2531	2534	rBV5	5919	8539	0.14%	0.019%
42	18.098	2547	2552	2560	rBV	87183	129891	2.08%	0.283%
43	19.022	2706	2709	2715	rVB6	19866	27629	0.44%	0.060%
44	19.122	2722	2726	2733	rBV2	37813	52965	0.85%	0.116%
45	19.192	2734	2738	2741	rBV	36725	46838	0.75%	0.102%
46	19.333	2759	2762	2768	rBV3	51060	62948	1.01%	0.137%
47	19.545	2792	2798	2804	rBV	3695551	4933771	78.87%	10.767%
48	21.304	3092	3097	3104	rBV	1881153	2346654	37.51%	5.121%
49	23.516	3466	3473	3489	rVB	3225940	6255697	100.00%	13.652%
50	23.669	3492	3499	3510	rVB	1376761	2721491	43.50%	5.939%




Sum of corrected areas: 45822683

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019166.D
Acq On : 29 Dec 2023 15:15
Operator : MA/JU
Sample : 06021-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

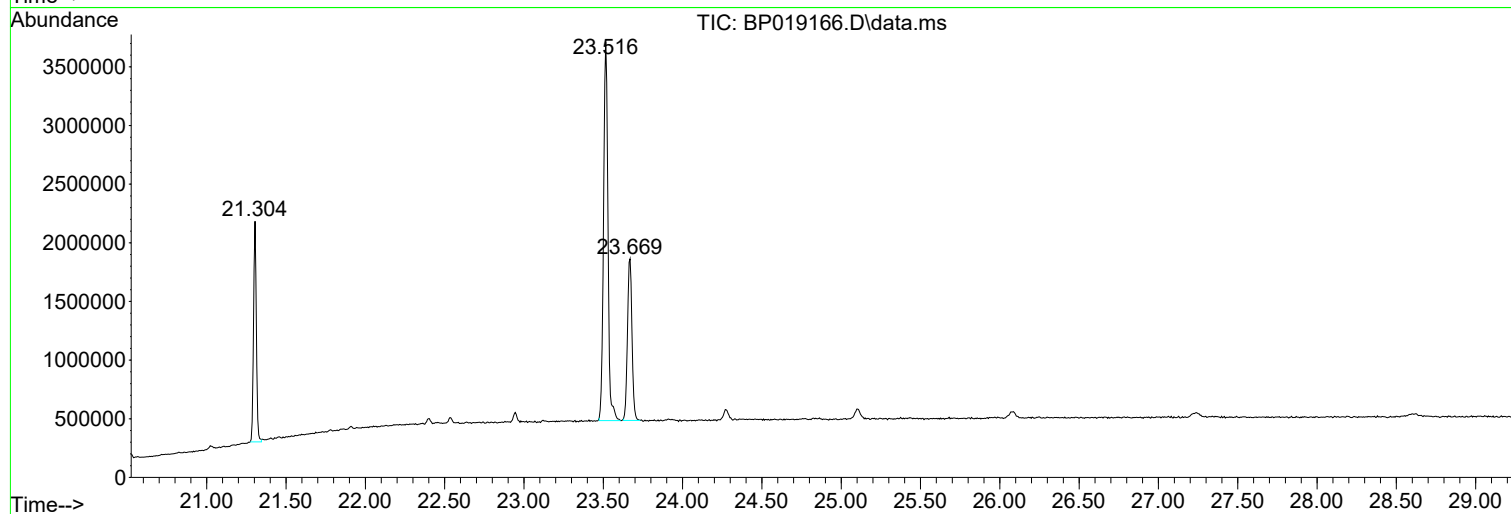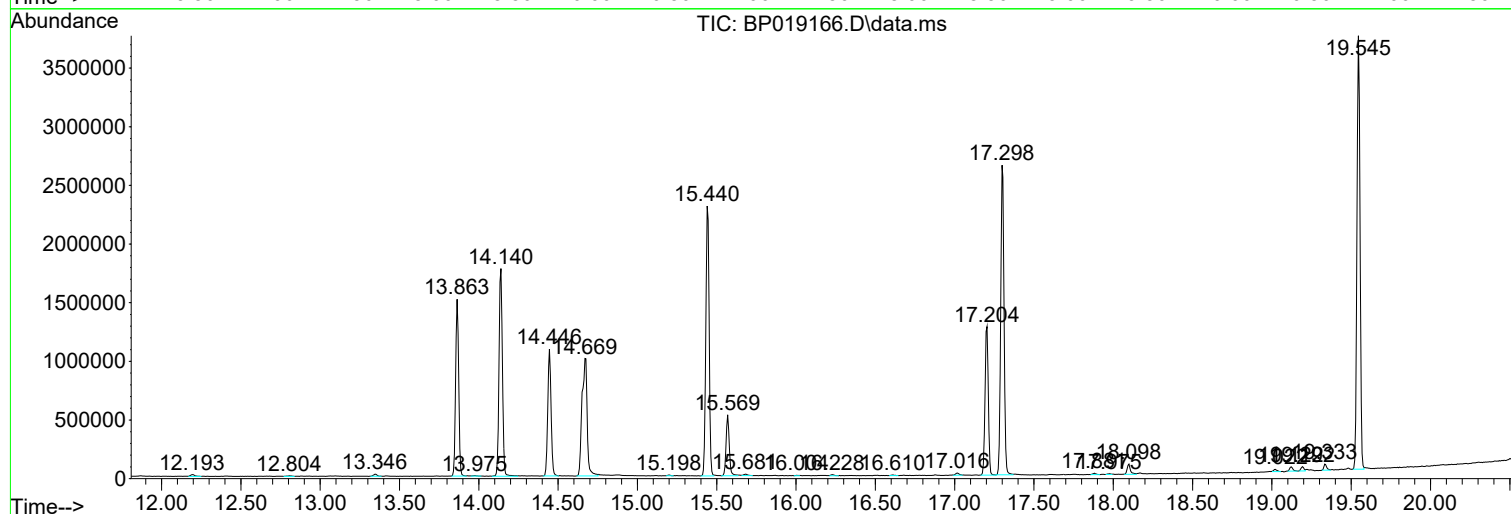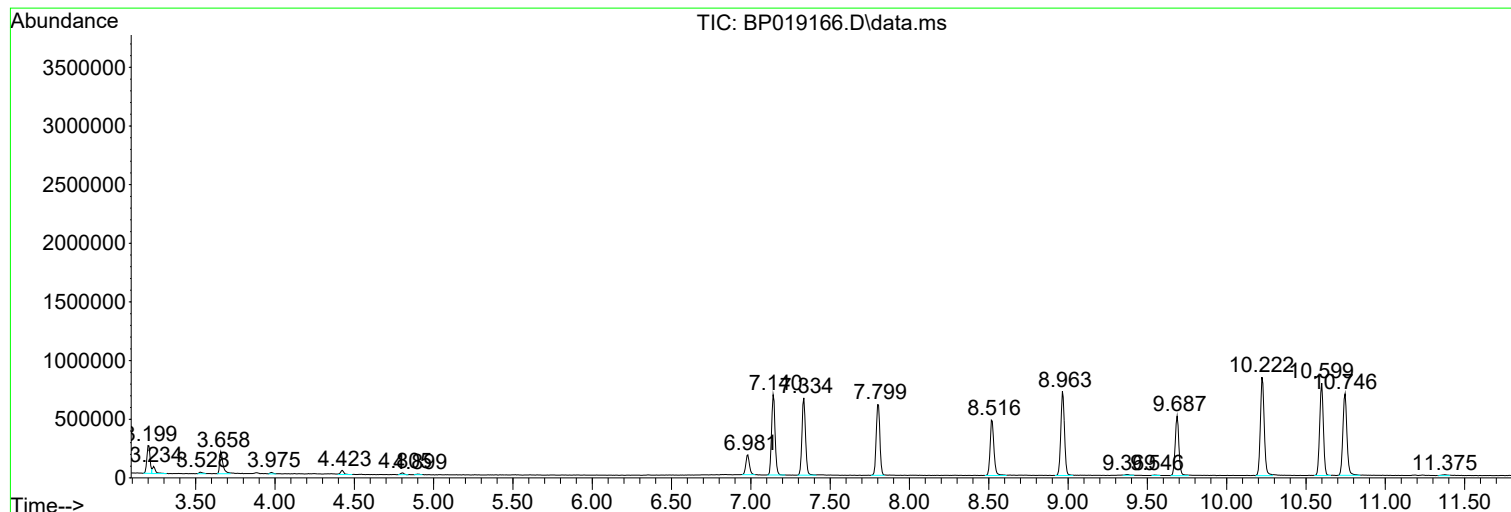

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019166.D
Acq On : 29 Dec 2023 15:15
Operator : MA/JU
Sample : 06021-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019166.D
Acq On : 29 Dec 2023 15:15
Operator : MA/JU
Sample : 06021-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc