

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019167.D
 Acq On : 29 Dec 2023 15:49
 Operator : MA/JU
 Sample : 06021-10
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	15	19	23	rBV	225555	307244	5.34%	0.729%
2	3.234	23	25	39	rVB	49141	71109	1.24%	0.169%
3	3.658	94	97	108	rBV	130831	211039	3.67%	0.501%
4	3.887	130	136	139	rBV2	8005	12947	0.22%	0.031%
5	3.975	147	151	156	rVB	10588	16877	0.29%	0.040%
6	4.422	223	227	232	rVB2	31133	45809	0.80%	0.109%
7	4.805	287	292	298	rVB3	13454	22123	0.38%	0.052%
8	4.916	305	311	314	rBV3	5282	10558	0.18%	0.025%
9	6.981	656	662	672	rVB	135727	226705	3.94%	0.538%
10	7.140	683	689	700	rVB	576693	890239	15.46%	2.112%
11	7.334	715	722	734	rBV	537224	858337	14.91%	2.036%
12	7.799	794	801	809	rBV	616082	995409	17.29%	2.361%
13	8.516	914	923	939	rBV	389602	656695	11.41%	1.558%
14	8.963	992	999	1011	rBV	603275	984098	17.09%	2.334%
15	9.375	1065	1069	1074	rVB3	12521	19219	0.33%	0.046%
16	9.687	1113	1122	1131	rBV	423357	686468	11.92%	1.628%
17	10.222	1205	1213	1228	rBV	702028	1203420	20.90%	2.854%
18	10.598	1269	1277	1287	rVB	807914	1308532	22.73%	3.104%
19	10.745	1295	1302	1320	rBV	613770	1084048	18.83%	2.571%
20	11.863	1489	1492	1498	rVB5	9128	14196	0.25%	0.034%
21	12.198	1542	1549	1555	rBV3	12391	22550	0.39%	0.053%
22	12.798	1648	1651	1656	rBV7	3550	6352	0.11%	0.015%
23	13.345	1736	1744	1751	rVB	19160	34689	0.60%	0.082%
24	13.863	1825	1832	1843	rBV	1415592	1951760	33.90%	4.629%
25	13.975	1846	1851	1859	rVB10	10237	16884	0.29%	0.040%
26	14.139	1867	1879	1892	rBV	1579504	2331938	40.50%	5.531%
27	14.445	1924	1931	1941	rBV	1156508	1669810	29.00%	3.961%
28	14.669	1961	1969	1982	rBV2	60133	148449	2.58%	0.352%
29	15.104	2037	2043	2048	rBV9	5418	8696	0.15%	0.021%
30	15.439	2092	2100	2111	rBV	2294255	3165598	54.98%	7.508%
31	15.569	2115	2122	2135	rVV	494237	707724	12.29%	1.679%
32	15.681	2137	2141	2146	rVB2	10143	14737	0.26%	0.035%
33	16.228	2230	2234	2239	rVB7	8967	13582	0.24%	0.032%
34	16.875	2341	2344	2350	rVB8	4652	7271	0.13%	0.017%
35	17.010	2361	2367	2378	rBV	169214	249223	4.33%	0.591%
36	17.198	2393	2399	2409	rBV	1396703	2030812	35.27%	4.817%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019167.D
 Acq On : 29 Dec 2023 15:49
 Operator : MA/JU
 Sample : 06021-10
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Z2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	17.298	2410	2416	2429	rVV	2620777	3750774	65.15%	8.896%
38	18.092	2547	2551	2556	rBV	57379	81791	1.42%	0.194%
39	18.169	2560	2564	2572	rVV2	18323	33034	0.57%	0.078%
40	18.516	2619	2623	2625	rBV5	9507	11241	0.20%	0.027%
41	19.122	2722	2726	2731	rBV2	39949	52670	0.91%	0.125%
42	19.192	2734	2738	2741	rBV	38348	50397	0.88%	0.120%
43	19.333	2759	2762	2766	rBV3	28910	37591	0.65%	0.089%
44	19.545	2792	2798	2807	rBV	3729882	4808382	83.52%	11.405%
45	21.304	3092	3097	3104	rBV	2064387	2609330	45.32%	6.189%
46	23.515	3466	3473	3490	rVB2	2970031	5757456	100.00%	13.656%
47	23.668	3493	3499	3510	rVB	1498402	2962549	51.46%	7.027%




Sum of corrected areas: 42160362

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019167.D
Acq On : 29 Dec 2023 15:49
Operator : MA/JU
Sample : 06021-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

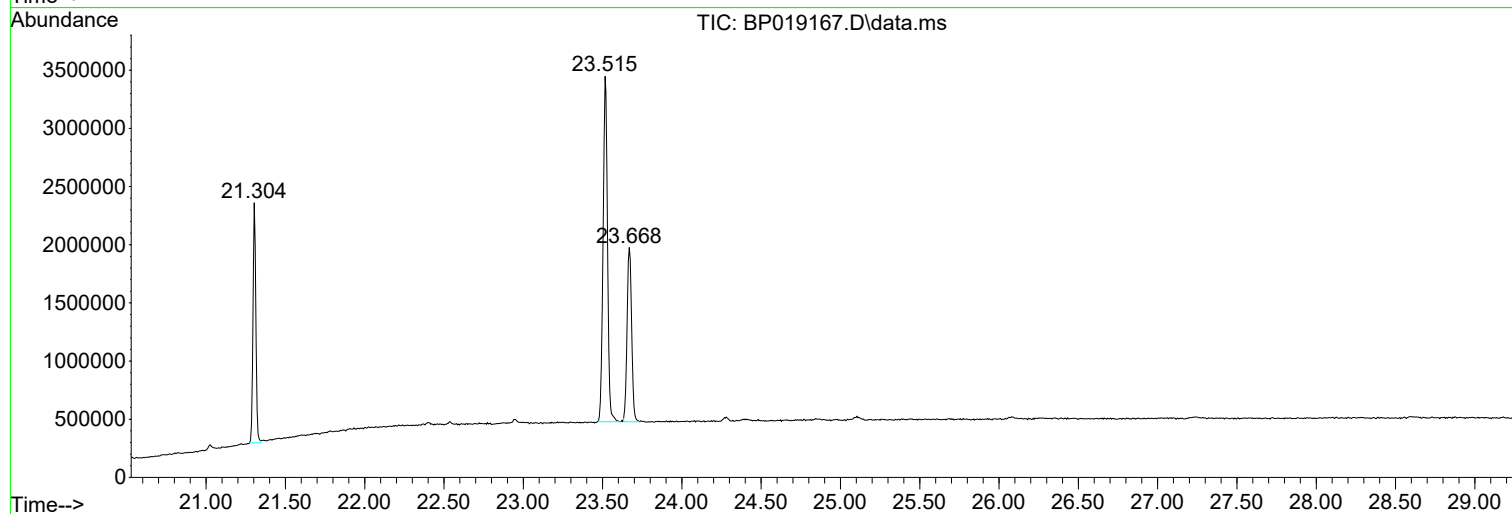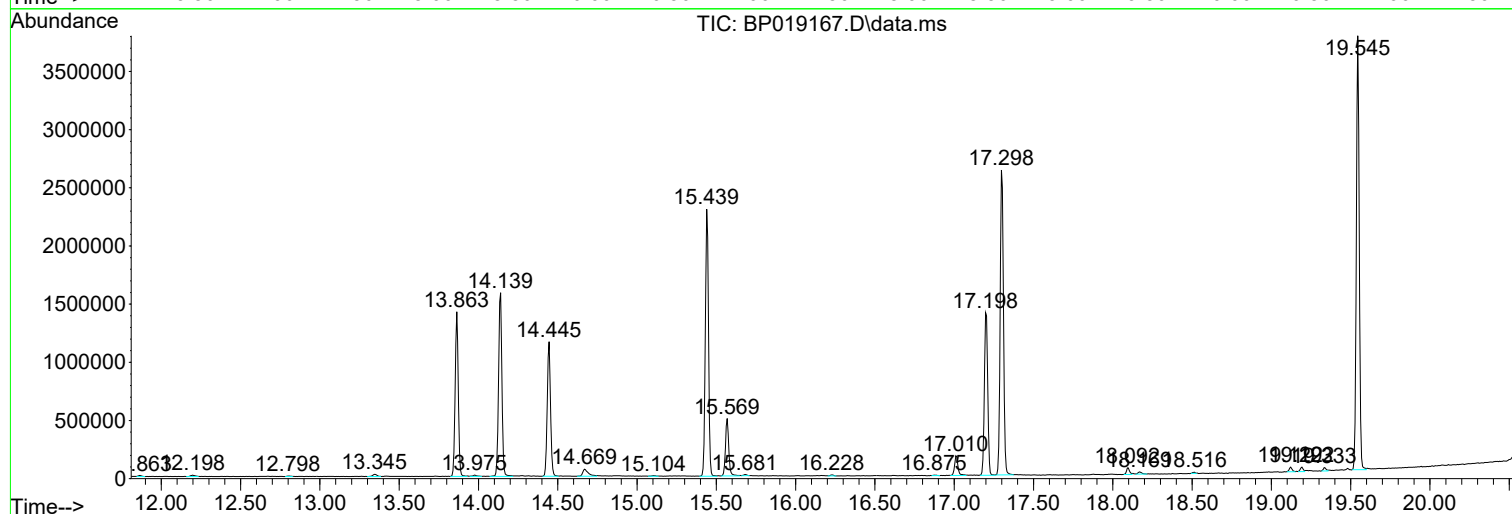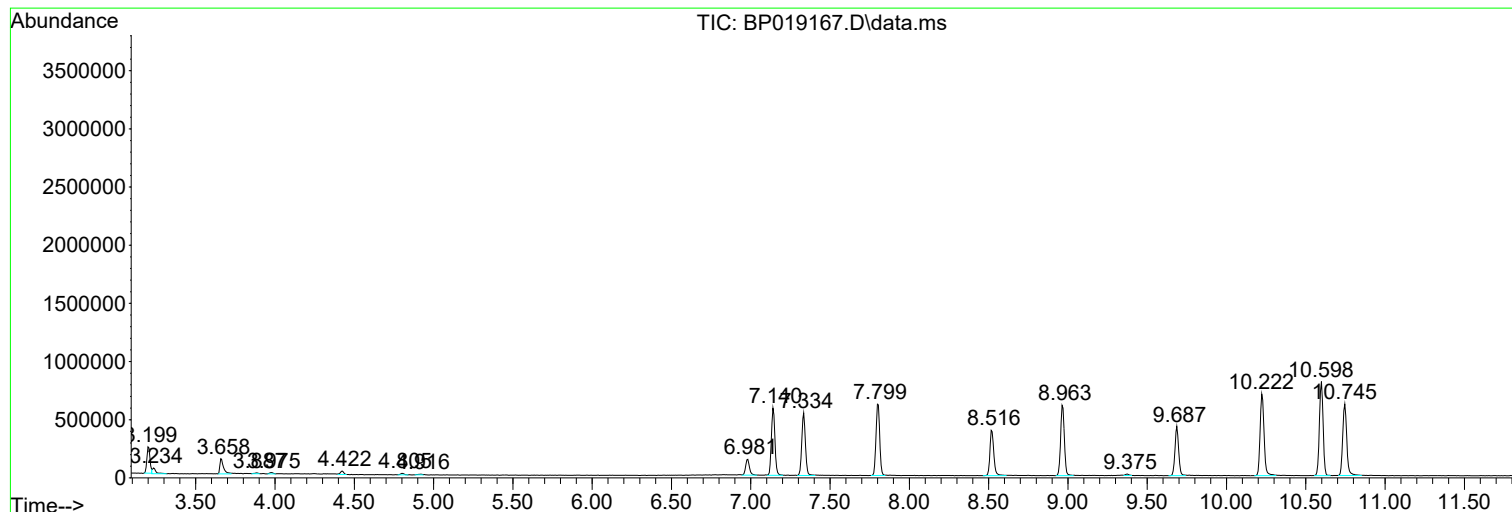

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019167.D
Acq On : 29 Dec 2023 15:49
Operator : MA/JU
Sample : 06021-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-butyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.010	2.45 ng/ul	249223	Phenanthrene-d10	17.198

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	90
2			2-propenoic acid, 2-methyl-, 2-[...]	269	C12H15NO4S	1000401-71-8	64
3			[(Phenylsulfonyl)amino]acetic acid	215	C8H9NO4S	005398-96-9	64
4			N-Octylbenzenesulfonamide	269	C14H23NO2S	016358-32-0	64
5			N-Benzenesulfonyloxy-2,2-bis(tri...]	335	C10H7F6NO3S	055734-41-3	50

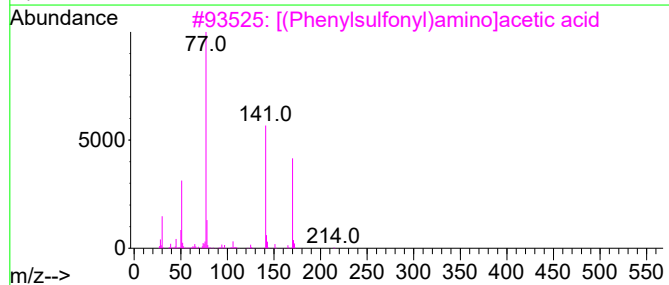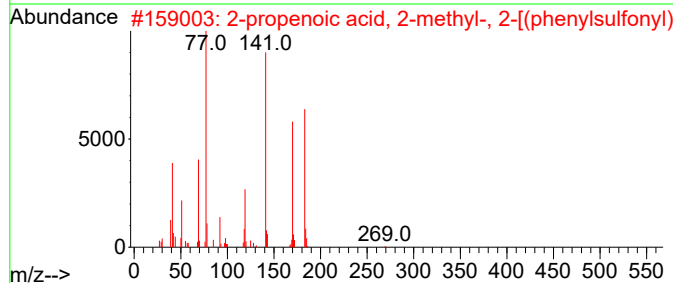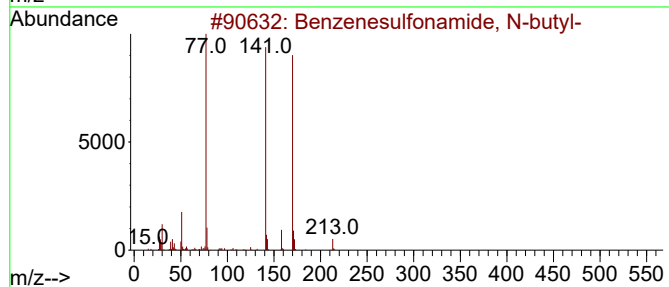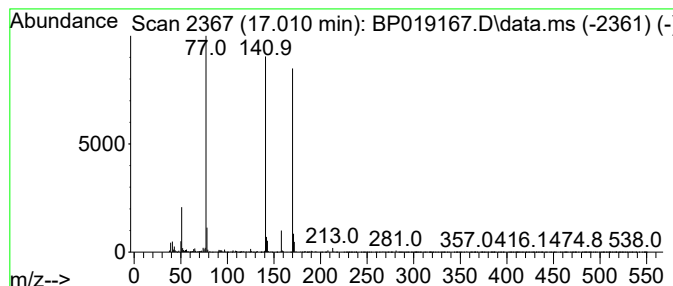

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019167.D
Acq On : 29 Dec 2023 15:49
Operator : MA/JU
Sample : 06021-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Z2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	17.010	2.5	ng/ul	249223	4	17.198	2030810	20.0