

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019169.D
 Acq On : 29 Dec 2023 16:57
 Operator : MA/JU
 Sample : 06020-07
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	30	rVB	46277	55019	0.80%	0.112%
2	3.658	93	97	108	rBV	239159	353601	5.17%	0.720%
3	3.881	133	135	141	rVB3	10538	12608	0.18%	0.026%
4	3.975	148	151	156	rVB	11863	14150	0.21%	0.029%
5	4.422	224	227	232	rVB2	18131	23833	0.35%	0.049%
6	4.805	288	292	297	rVB5	7683	11623	0.17%	0.024%
7	4.899	303	308	317	rBV4	6182	15497	0.23%	0.032%
8	6.975	656	661	671	rVB	186397	303189	4.43%	0.617%
9	7.140	682	689	701	rVB	708366	1093736	15.99%	2.227%
10	7.334	715	722	731	rBV	683979	1075693	15.73%	2.190%
11	7.799	794	801	810	rBV	684058	1085996	15.88%	2.211%
12	8.516	916	923	939	rBV	517710	855611	12.51%	1.742%
13	8.963	992	999	1010	rBV	759310	1227667	17.95%	2.500%
14	9.369	1064	1068	1077	rVB	5087	12029	0.18%	0.024%
15	9.687	1114	1122	1131	rBV	544411	885603	12.95%	1.803%
16	10.222	1204	1213	1225	rBV	910346	1508007	22.05%	3.071%
17	10.599	1267	1277	1285	rBV	853254	1423038	20.81%	2.898%
18	10.746	1292	1302	1317	rBV	811863	1405976	20.56%	2.863%
19	11.863	1488	1492	1497	rVB4	6849	11306	0.17%	0.023%
20	12.199	1544	1549	1561	rVB	13682	26790	0.39%	0.055%
21	13.346	1738	1744	1749	rBV6	10832	18688	0.27%	0.038%
22	13.863	1825	1832	1845	rBV	1797263	2445201	35.76%	4.979%
23	14.140	1871	1879	1890	rBV	1906633	2824926	41.31%	5.752%
24	14.445	1922	1931	1938	rBV	1211220	1790269	26.18%	3.645%
25	14.663	1963	1968	1990	rBV	90603	212286	3.10%	0.432%
26	14.887	2000	2006	2009	rVB8	4913	9926	0.15%	0.020%
27	15.440	2092	2100	2109	rBV	2839127	3916918	57.28%	7.976%
28	15.569	2116	2122	2133	rBV	709988	958270	14.01%	1.951%
29	15.681	2137	2141	2147	rVB3	12576	21250	0.31%	0.043%
30	15.810	2159	2163	2168	rBV2	8242	11793	0.17%	0.024%
31	16.228	2229	2234	2239	rVB4	10465	16118	0.24%	0.033%
32	16.881	2339	2345	2350	rBV9	4929	8368	0.12%	0.017%
33	17.016	2363	2368	2379	rVB	26970	48010	0.70%	0.098%
34	17.204	2393	2400	2409	rBV	1536278	2194049	32.08%	4.468%
35	17.298	2410	2416	2429	rBV	3124497	4550544	66.54%	9.266%
36	18.098	2547	2552	2558	rBV2	44793	70246	1.03%	0.143%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019169.D
Acq On : 29 Dec 2023 16:57
Operator : MA/JU
Sample : 06020-07
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	19.122	2722	2726	2733	rBV2	41659	62513	0.91%	0.127%
38	19.192	2734	2738	2742	rBV	42049	59199	0.87%	0.121%
39	19.333	2759	2762	2771	rBV4	29752	46106	0.67%	0.094%
40	19.545	2792	2798	2809	rBV	4429457	5749029	84.07%	11.706%
41	21.304	3092	3097	3103	rBV	2228548	2770212	40.51%	5.641%
42	23.516	3466	3473	3487	rVB2	3518973	6838531	100.00%	13.925%
43	23.669	3493	3499	3509	rVB	1601995	3087767	45.15%	6.287%




Sum of corrected areas: 49111191

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019169.D
Acq On : 29 Dec 2023 16:57
Operator : MA/JU
Sample : 06020-07
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

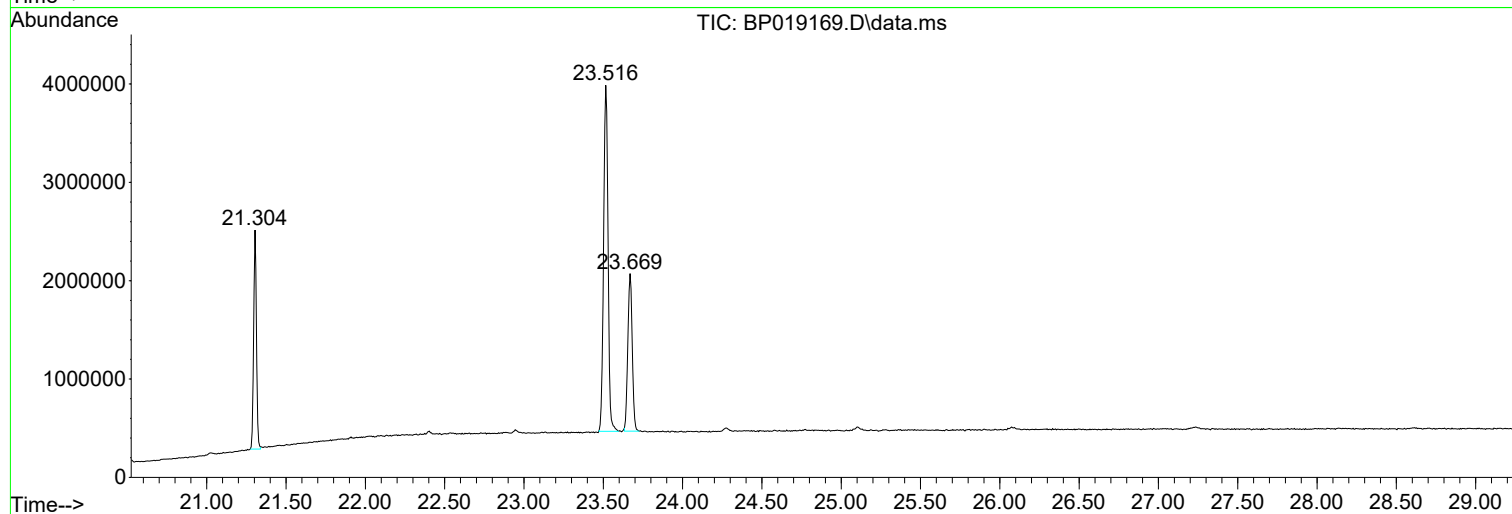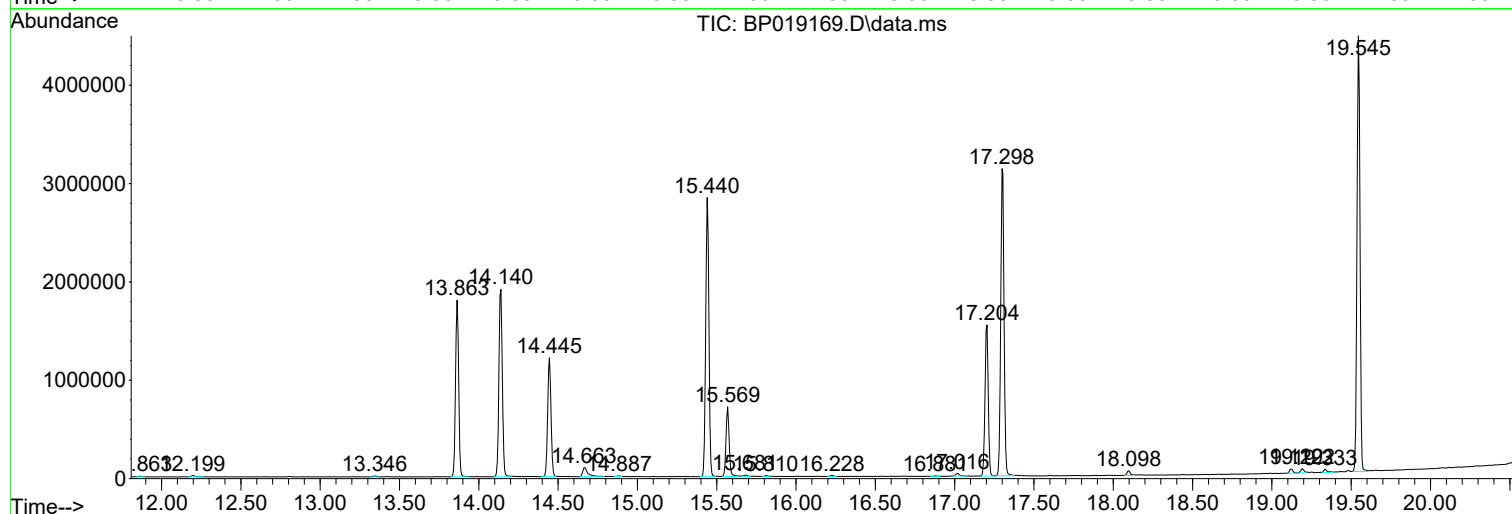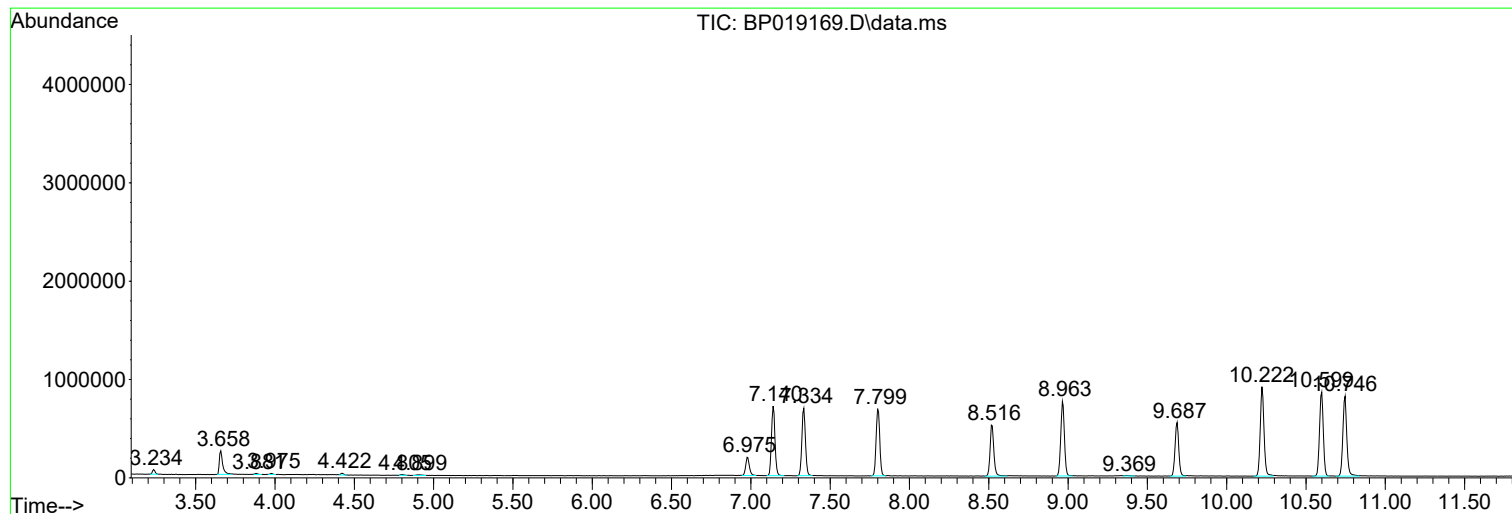

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019169.D
Acq On : 29 Dec 2023 16:57
Operator : MA/JU
Sample : 06020-07
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019169.D
Acq On : 29 Dec 2023 16:57
Operator : MA/JU
Sample : 06020-07
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7W8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc