

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019173.D
 Acq On : 29 Dec 2023 19:14
 Operator : MA/JU
 Sample : 06021-01
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7Y3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	15	19	22	rBV	80542	96552	0.72%	0.157%
2	3.234	22	25	31	rVB	45804	57099	0.43%	0.093%
3	3.652	92	96	108	rBV	292000	429712	3.21%	0.699%
4	3.975	148	151	156	rVB2	12297	15788	0.12%	0.026%
5	6.975	656	661	673	rVB	199853	320173	2.39%	0.521%
6	7.140	682	689	698	rBV	680753	1042987	7.79%	1.698%
7	7.328	714	721	734	rBV	645705	1042212	7.79%	1.697%
8	7.799	792	801	810	rBV	686866	1083939	8.10%	1.764%
9	8.516	916	923	937	rBV	535671	875422	6.54%	1.425%
10	8.963	991	999	1008	rBV	751671	1186253	8.86%	1.931%
11	9.687	1114	1122	1134	rBV	543234	896510	6.70%	1.459%
12	10.222	1205	1213	1228	rBV	883378	1506259	11.25%	2.452%
13	10.593	1268	1276	1286	rBV	874167	1473309	11.01%	2.398%
14	10.745	1293	1302	1319	rBV	768054	1383983	10.34%	2.253%
15	12.192	1541	1548	1558	rVB3	14320	32466	0.24%	0.053%
16	13.345	1738	1744	1750	rBV	22093	37448	0.28%	0.061%
17	13.863	1825	1832	1840	rBV	1700409	2304258	17.22%	3.751%
18	14.134	1868	1878	1888	rBV	1813143	2743459	20.50%	4.466%
19	14.445	1922	1931	1946	rBV	1317014	1938251	14.48%	3.155%
20	14.663	1961	1968	1981	rBV2	125489	272912	2.04%	0.444%
21	14.875	1999	2004	2012	rVB2	10286	23939	0.18%	0.039%
22	15.439	2090	2100	2107	rBV	2503995	3592463	26.84%	5.848%
23	15.569	2115	2122	2135	rBV	634800	918628	6.86%	1.495%
24	15.681	2135	2141	2151	rVB6	13767	28041	0.21%	0.046%
25	16.228	2229	2234	2238	rVB4	11425	16442	0.12%	0.027%
26	17.033	2361	2371	2375	rBV	8159301	13385153	100.00%	21.788%
27	17.198	2393	2399	2410	rVB	1625827	2287132	17.09%	3.723%
28	17.298	2410	2416	2427	rBV2	2885068	4090157	30.56%	6.658%
29	18.092	2547	2551	2558	rBV	79992	117174	0.88%	0.191%
30	18.380	2597	2600	2605	rVB3	16212	13926	0.10%	0.023%
31	19.033	2707	2711	2715	rBV	54707	65386	0.49%	0.106%
32	19.122	2721	2726	2729	rBV	44675	64058	0.48%	0.104%
33	19.192	2734	2738	2740	rBV	40704	50012	0.37%	0.081%
34	19.333	2758	2762	2769	rBV3	60474	84874	0.63%	0.138%
35	19.545	2792	2798	2806	rBV	3971755	5251297	39.23%	8.548%
36	21.304	3092	3097	3104	rBV	2392272	2920161	21.82%	4.753%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019173.D
Acq On : 29 Dec 2023 19:14
Operator : MA/JU
Sample : 06021-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Y3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	21.398	3110	3113	3118	rVB	159374	184640	1.38%	0.301%
38	23.515	3465	3473	3489	rVB2	3213569	6337702	47.35%	10.317%
39	23.662	3492	3498	3508	rVB	1655878	3262318	24.37%	5.310%




Sum of corrected areas: 61432495

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019173.D
Acq On : 29 Dec 2023 19:14
Operator : MA/JU
Sample : 06021-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Y3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

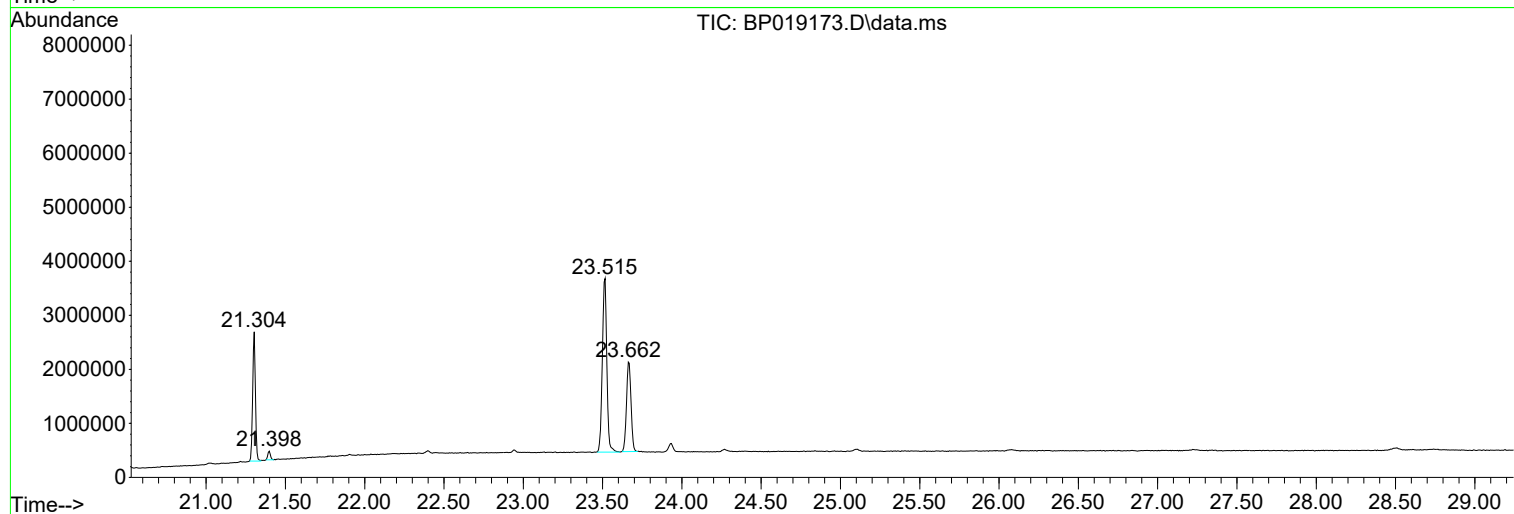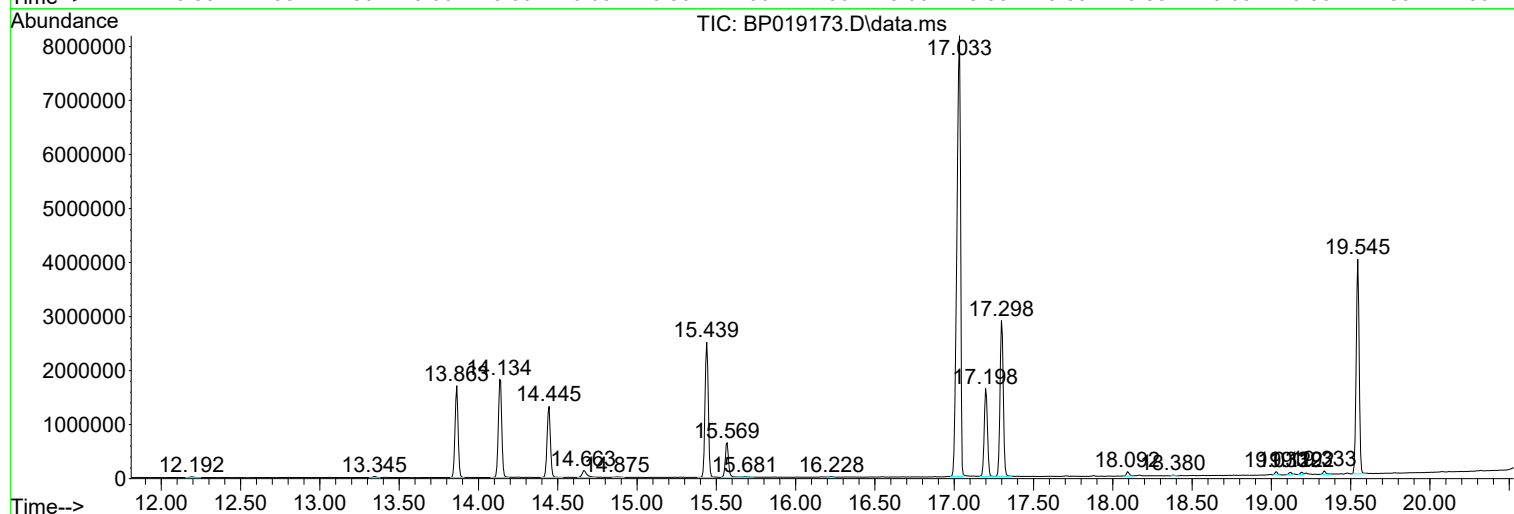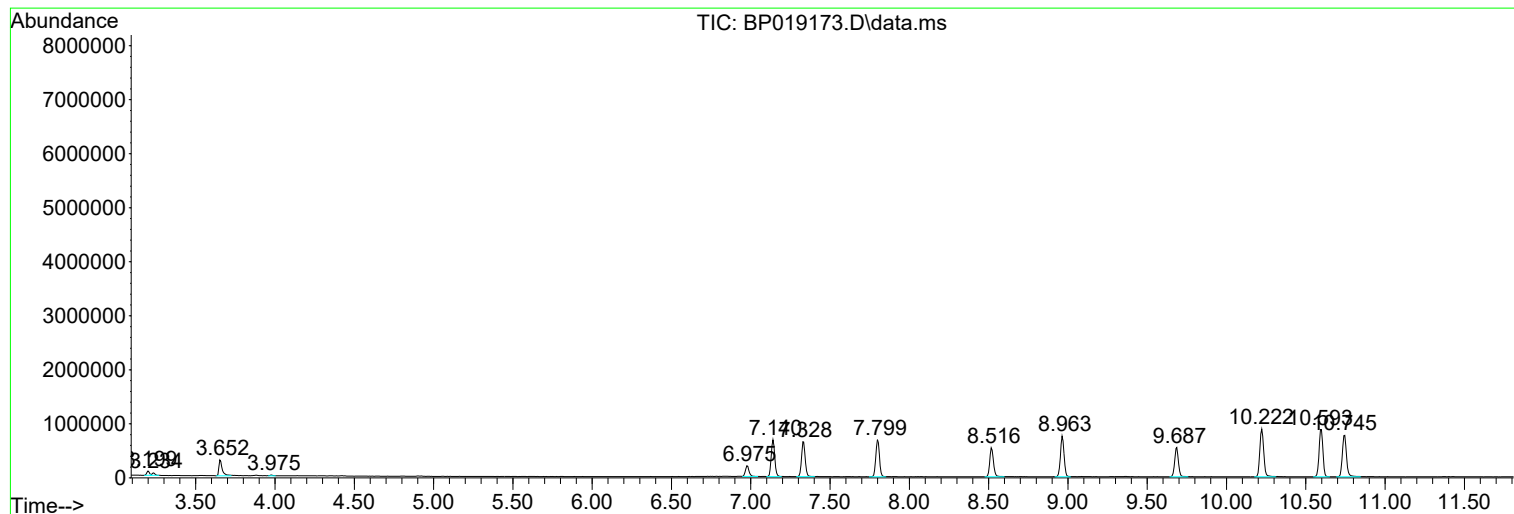

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019173.D
Acq On : 29 Dec 2023 19:14
Operator : MA/JU
Sample : 06021-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Y3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-butyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.033	117.05 ng/ul	13385200	Phenanthrene-d10	17.198

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	90
2			Benzenesulfonamide, N-butyl-	213	C10H15NO2S	003622-84-2	80
3			2-propenoic acid, 2-methyl-, 2-[...]	269	C12H15NO4S	1000401-71-8	64
4			N-(2-Cyano-ethyl)-benzenesulfona...	210	C9H10N2O2S	002619-21-8	64
5			N-Benzenesulfonyloxy-2,2-bis(tri...	335	C10H7F6NO3S	055734-41-3	50

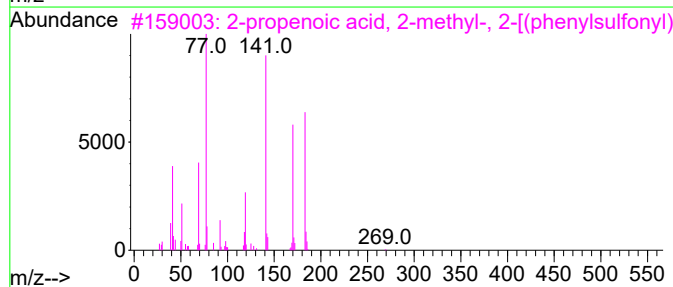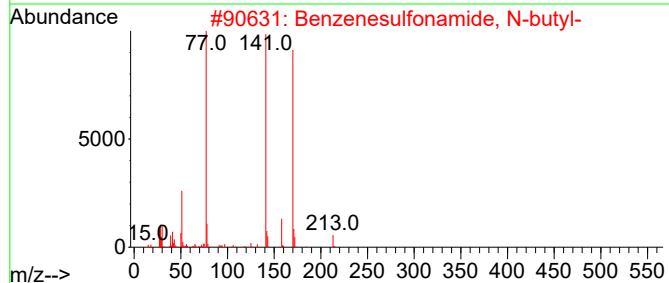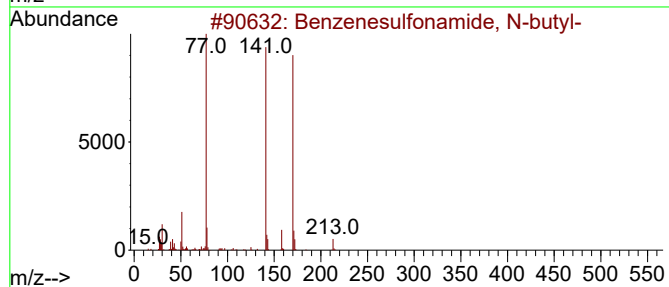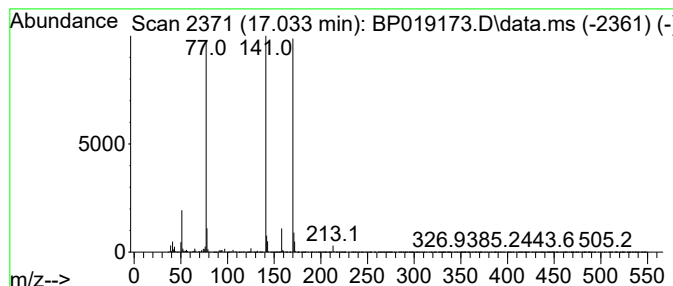

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019173.D
Acq On : 29 Dec 2023 19:14
Operator : MA/JU
Sample : 06021-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7Y3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	17.033	117.1	ng/ul	13385200	4	17.198	2287130	20.0