

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019180.D
 Acq On : 29 Dec 2023 23:47
 Operator : MA/JU
 Sample : PB158075BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK075

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	32	rVB	75674	91634	1.70%	0.188%
2	3.652	92	96	110	rBV	835567	1189239	22.04%	2.434%
3	3.975	148	151	156	rVB	13413	17758	0.33%	0.036%
4	6.716	608	617	620	rBV10	3480	9641	0.18%	0.020%
5	6.975	655	661	672	rVV	866422	1340211	24.83%	2.743%
6	7.140	682	689	700	rVB	727238	1108472	20.54%	2.268%
7	7.328	715	721	736	rBV	872741	1389241	25.74%	2.843%
8	7.799	791	801	811	rBV	804871	1241670	23.01%	2.541%
9	8.516	913	923	936	rBV	1012840	1619689	30.01%	3.315%
10	8.963	992	999	1012	rBV	770998	1242791	23.03%	2.543%
11	9.681	1115	1121	1133	rBV	573838	956638	17.73%	1.958%
12	10.222	1205	1213	1231	rBV	958624	1645492	30.49%	3.367%
13	10.593	1269	1276	1287	rVB	959960	1613685	29.90%	3.302%
14	10.740	1293	1301	1323	rBV	899029	1582382	29.32%	3.238%
15	12.204	1541	1550	1555	rBV4	12069	24795	0.46%	0.051%
16	13.346	1738	1744	1751	rBV6	12275	22391	0.41%	0.046%
17	13.416	1751	1756	1759	rBV6	3468	5934	0.11%	0.012%
18	13.863	1825	1832	1842	rBV	1464387	2039845	37.80%	4.174%
19	14.134	1871	1878	1890	rBV	1775000	2560712	47.45%	5.240%
20	14.446	1921	1931	1939	rBV	1323799	1969684	36.50%	4.031%
21	14.657	1960	1967	1991	rBV	543569	943607	17.48%	1.931%
22	15.440	2093	2100	2113	rBV	2296966	3189050	59.09%	6.526%
23	15.563	2114	2121	2135	rBV	551727	804602	14.91%	1.647%
24	15.681	2138	2141	2149	rVB4	11763	20019	0.37%	0.041%
25	16.228	2230	2234	2240	rVB7	8317	14051	0.26%	0.029%
26	16.875	2340	2344	2348	rVB5	3941	5501	0.10%	0.011%
27	17.198	2393	2399	2409	rBV	1671373	2343853	43.43%	4.797%
28	17.298	2409	2416	2428	rBV	2429379	3464710	64.20%	7.090%
29	18.092	2547	2551	2555	rBV7	11501	19874	0.37%	0.041%
30	19.116	2722	2725	2731	rVB2	32824	44705	0.83%	0.091%
31	19.186	2734	2737	2742	rBV2	29470	42827	0.79%	0.088%
32	19.539	2792	2797	2811	rBV	3232406	4397061	81.48%	8.998%
33	21.298	3092	3096	3104	rBV	2339190	3032057	56.18%	6.205%
34	23.516	3465	3473	3489	rVB	2677237	5396750	100.00%	11.044%
35	23.663	3492	3498	3515	rVB	1739323	3474681	64.38%	7.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019180.D
Acq On : 29 Dec 2023 23:47
Operator : MA/JU
Sample : PB158075BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK075

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 48865252

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019180.D
Acq On : 29 Dec 2023 23:47
Operator : MA/JU
Sample : PB158075BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK075

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

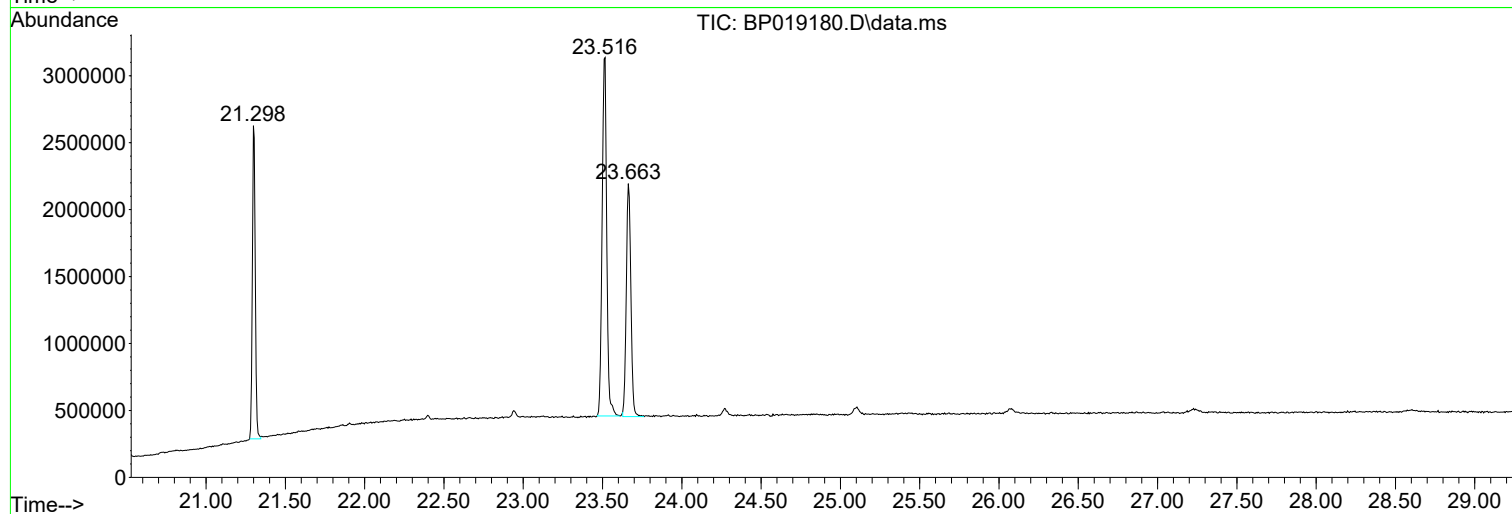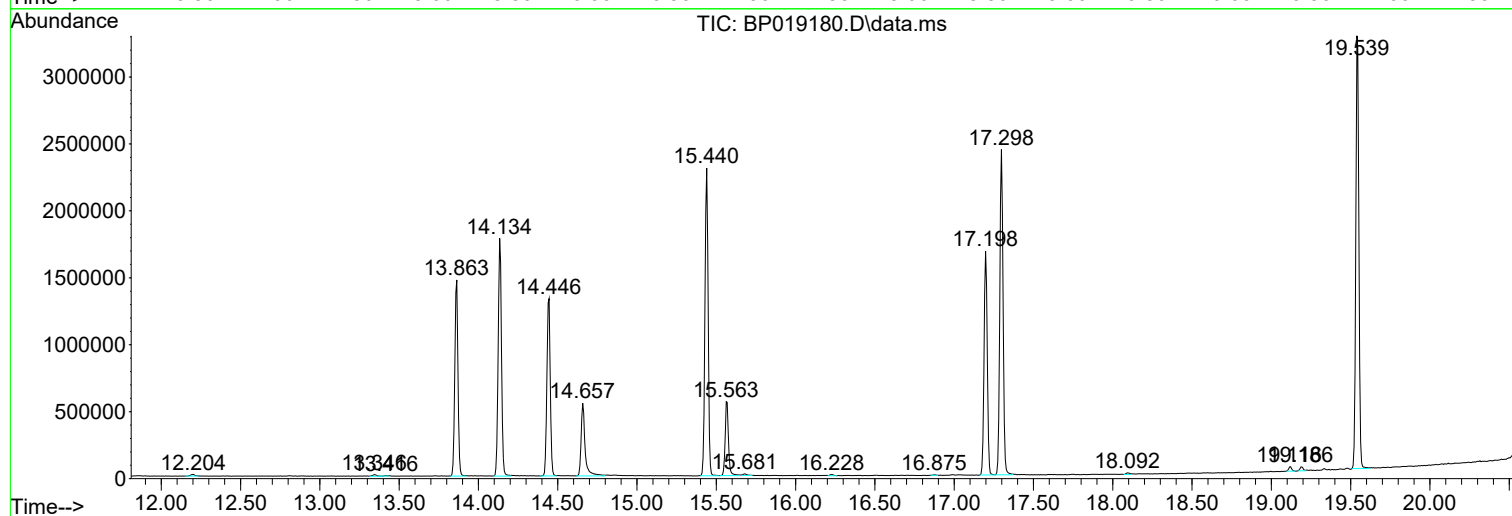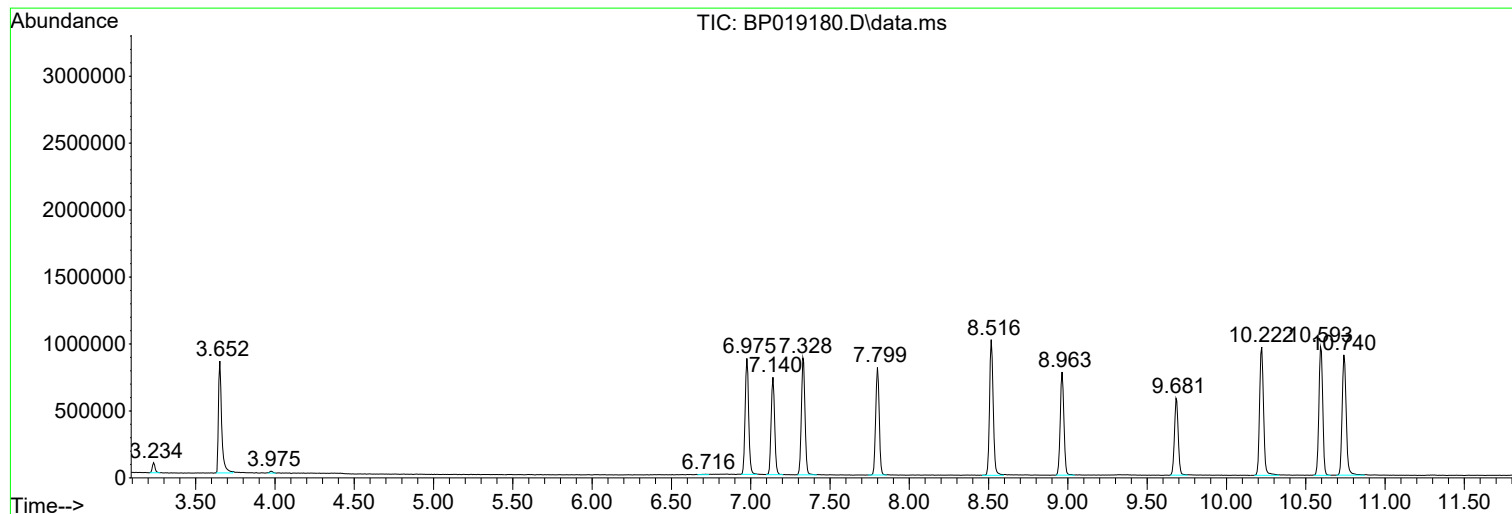

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019180.D
Acq On : 29 Dec 2023 23:47
Operator : MA/JU
Sample : PB158075BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK075

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019180.D
Acq On : 29 Dec 2023 23:47
Operator : MA/JU
Sample : PB158075BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK075

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------