

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019184.D
 Acq On : 30 Dec 2023 02:05
 Operator : MA/JU
 Sample : 06020-01
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3N9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	32	rVB	51187	63736	1.03%	0.144%
2	3.658	93	97	112	rBV	223886	342461	5.52%	0.771%
3	3.876	132	134	140	rVB2	9559	14074	0.23%	0.032%
4	3.976	148	151	154	rVB	9380	11519	0.19%	0.026%
5	6.975	655	661	675	rVB	192013	313593	5.06%	0.706%
6	7.140	683	689	700	rVB	710631	1099040	17.72%	2.474%
7	7.328	714	721	731	rBV	683213	1078541	17.39%	2.428%
8	7.799	792	801	809	rBV	640336	1005923	16.22%	2.265%
9	8.516	916	923	936	rBV	500635	789225	12.72%	1.777%
10	8.964	991	999	1009	rBV	756799	1226666	19.77%	2.762%
11	9.369	1064	1068	1079	rVB7	8430	20046	0.32%	0.045%
12	9.681	1114	1121	1134	rBV	562361	915055	14.75%	2.060%
13	10.222	1204	1213	1230	rBV	835899	1463014	23.58%	3.294%
14	10.593	1269	1276	1289	rVB	790378	1295155	20.88%	2.916%
15	10.740	1292	1301	1322	rBV	719557	1304872	21.03%	2.938%
16	11.863	1487	1492	1499	rVB5	6920	12021	0.19%	0.027%
17	12.193	1542	1548	1556	rVB	12165	24663	0.40%	0.056%
18	12.804	1647	1652	1655	rBV6	3988	6343	0.10%	0.014%
19	13.340	1739	1743	1749	rBV3	13068	21293	0.34%	0.048%
20	13.863	1825	1832	1841	rBV	1522075	2140350	34.50%	4.819%
21	14.134	1871	1878	1890	rBV	1763987	2585415	41.68%	5.821%
22	14.440	1923	1930	1938	rBV	1065039	1560337	25.15%	3.513%
23	14.663	1963	1968	1981	rBV	82771	186087	3.00%	0.419%
24	15.440	2093	2100	2115	rBV	2329964	3424625	55.21%	7.711%
25	15.563	2115	2121	2136	rVV	650611	902423	14.55%	2.032%
26	15.681	2137	2141	2147	rVB3	9908	17791	0.29%	0.040%
27	16.222	2229	2233	2239	rBV4	8429	13799	0.22%	0.031%
28	16.875	2340	2344	2348	rVB7	4802	6458	0.10%	0.015%
29	17.010	2362	2367	2375	rBV	64831	96265	1.55%	0.217%
30	17.198	2392	2399	2407	rBV	1319196	1862080	30.02%	4.192%
31	17.298	2409	2416	2430	rVV	2761785	3955774	63.77%	8.906%
32	18.092	2546	2551	2560	rBV	49581	76084	1.23%	0.171%
33	19.116	2721	2725	2730	rBV2	40956	57528	0.93%	0.130%
34	19.187	2733	2737	2742	rBV	37717	52424	0.85%	0.118%
35	19.334	2758	2762	2767	rBV5	34984	47058	0.76%	0.106%
36	19.545	2792	2798	2809	rBV	3772003	5039666	81.24%	11.347%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019184.D
Acq On : 30 Dec 2023 02:05
Operator : MA/JU
Sample : 06020-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3N9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	21.298	3091	3096	3105	rBV	1863874	2429316	39.16%	5.470%
38	23.510	3465	3472	3486	rVB2	3154473	6203396	100.00%	13.967%
39	23.663	3491	3498	3513	rVB	1384776	2750545	44.34%	6.193%




Sum of corrected areas: 44414661

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019184.D
Acq On : 30 Dec 2023 02:05
Operator : MA/JU
Sample : 06020-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

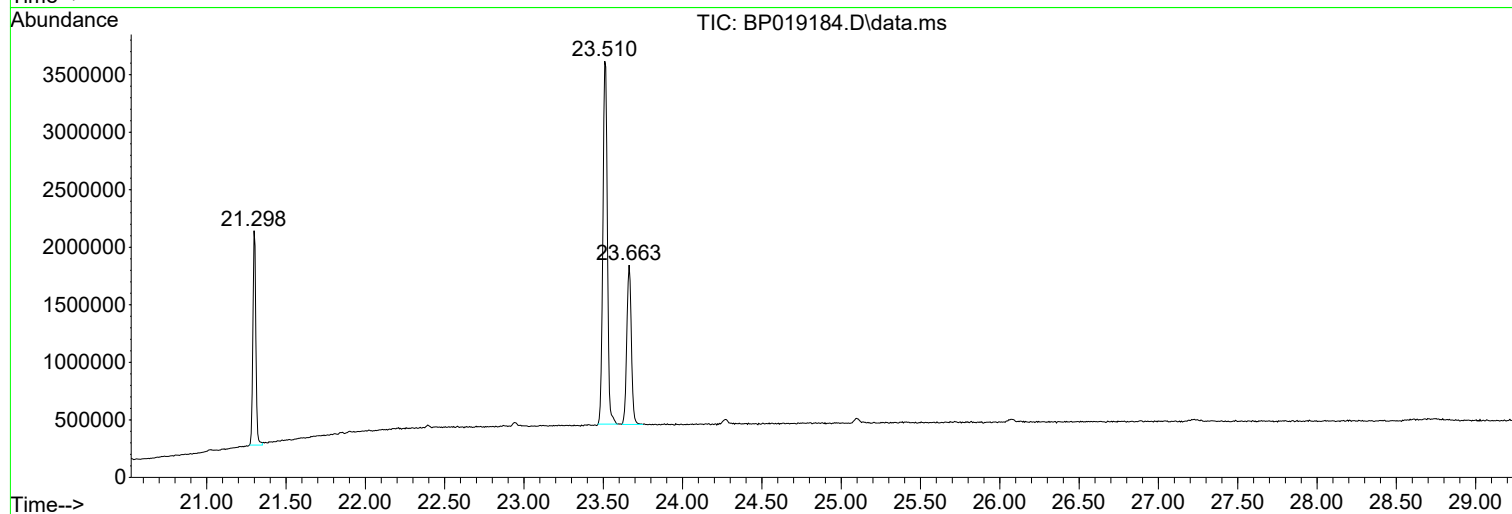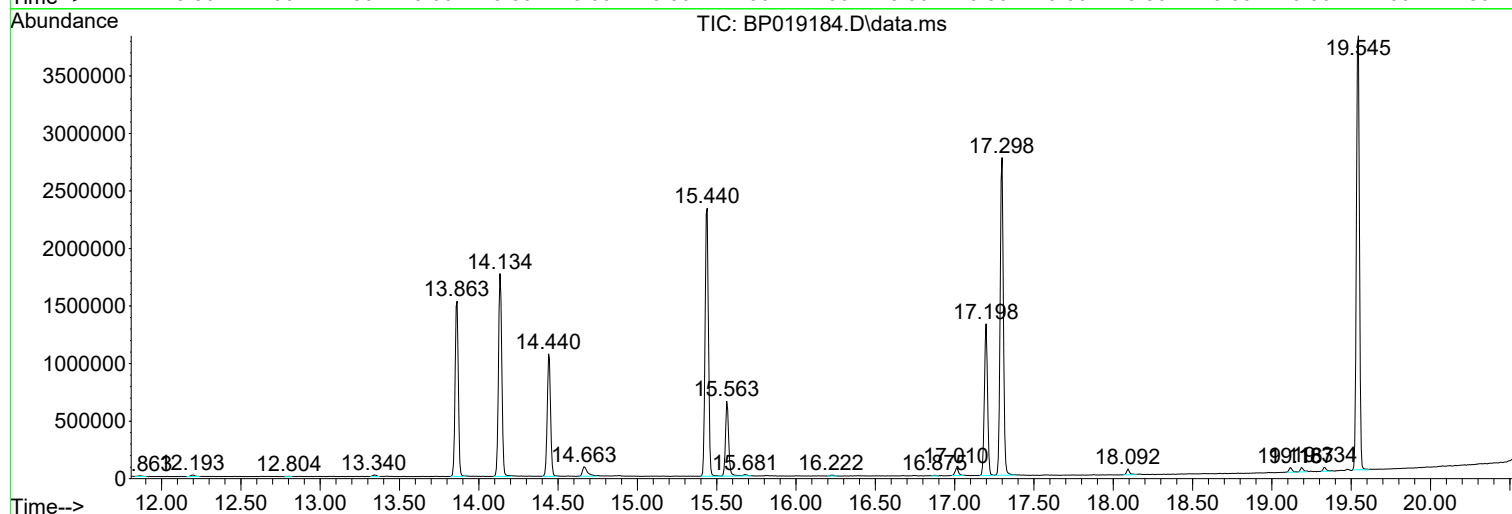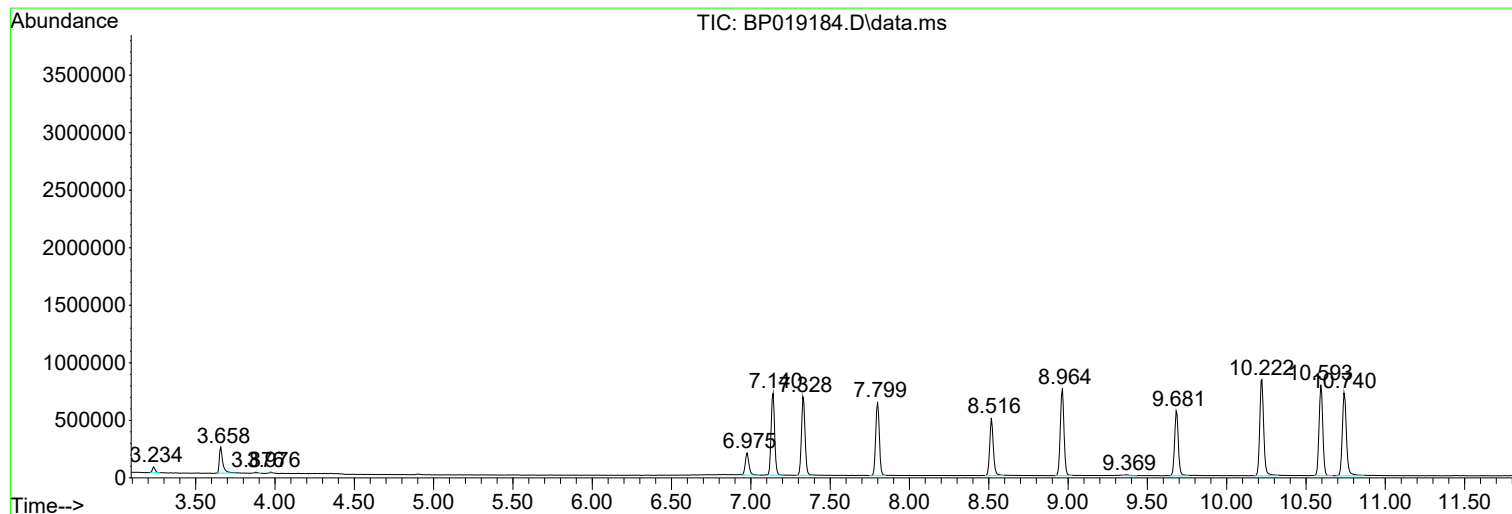

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019184.D
Acq On : 30 Dec 2023 02:05
Operator : MA/JU
Sample : 06020-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019184.D
Acq On : 30 Dec 2023 02:05
Operator : MA/JU
Sample : 06020-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3N9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc