

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019185.D
 Acq On : 30 Dec 2023 02:39
 Operator : MA/JU
 Sample : 06020-02
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	30	rBV	55802	65288	1.27%	0.159%
2	3.652	93	96	109	rBV	309961	482768	9.36%	1.173%
3	3.881	132	135	139	rVB	9742	12501	0.24%	0.030%
4	3.975	147	151	155	rBV	11337	17110	0.33%	0.042%
5	4.905	306	309	316	rVB2	7495	11660	0.23%	0.028%
6	6.975	656	661	677	rVB	222601	355153	6.88%	0.863%
7	7.140	683	689	698	rVB	714624	1094069	21.21%	2.659%
8	7.328	714	721	732	rBV	713902	1105004	21.42%	2.686%
9	7.799	794	801	812	rBV	674718	1038287	20.13%	2.523%
10	8.516	916	923	936	rBV	553606	900452	17.45%	2.188%
11	8.963	991	999	1009	rBV	759148	1231232	23.87%	2.992%
12	9.369	1062	1068	1074	rVB2	22379	36737	0.71%	0.089%
13	9.681	1114	1121	1130	rBV	546911	900121	17.45%	2.188%
14	10.222	1204	1213	1230	rBV	845979	1475257	28.60%	3.585%
15	10.593	1267	1276	1285	rVV	838494	1346805	26.11%	3.273%
16	10.740	1291	1301	1324	rBV	827922	1469855	28.49%	3.572%
17	11.863	1488	1492	1497	rVB2	13679	20683	0.40%	0.050%
18	12.193	1539	1548	1559	rBV3	13488	31215	0.61%	0.076%
19	13.075	1695	1698	1707	rBV8	2948	5592	0.11%	0.014%
20	13.345	1739	1744	1751	rVB2	14261	24134	0.47%	0.059%
21	13.416	1751	1756	1761	rBV7	2827	6461	0.13%	0.016%
22	13.863	1825	1832	1845	rBV	1398599	1964951	38.09%	4.776%
23	14.134	1870	1878	1891	rBV2	1698525	2469405	47.87%	6.002%
24	14.439	1924	1930	1944	rVB	1062656	1589154	30.80%	3.862%
25	14.663	1961	1968	1984	rBV	73327	182765	3.54%	0.444%
26	14.875	1999	2004	2010	rVB10	5008	11164	0.22%	0.027%
27	15.439	2093	2100	2108	rBV	2223799	3132993	60.73%	7.614%
28	15.563	2115	2121	2135	rBV	510426	730027	14.15%	1.774%
29	15.681	2137	2141	2150	rVB3	13205	20686	0.40%	0.050%
30	16.228	2229	2234	2239	rVB5	6717	10101	0.20%	0.025%
31	16.881	2339	2345	2349	rVB8	4560	8117	0.16%	0.020%
32	17.022	2366	2369	2377	rVB5	5728	10737	0.21%	0.026%
33	17.198	2392	2399	2409	rBV	1295944	1756200	34.04%	4.268%
34	17.298	2409	2416	2430	rVV	2436452	3415541	66.20%	8.301%
35	18.092	2547	2551	2561	rBV	52308	82089	1.59%	0.200%
36	19.122	2721	2726	2729	rBV5	31570	47263	0.92%	0.115%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019185.D
Acq On : 30 Dec 2023 02:39
Operator : MA/JU
Sample : 06020-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	19.192	2734	2738	2741	rBV2	31127	41408	0.80%	0.101%
38	19.333	2758	2762	2766	rBV2	51972	64506	1.25%	0.157%
39	19.545	2792	2798	2810	rBV	3161905	4169565	80.82%	10.133%
40	21.304	3092	3097	3105	rBV	1650218	2142750	41.53%	5.208%
41	23.515	3466	3473	3490	rVB	2641013	5159058	100.00%	12.538%
42	23.663	3492	3498	3513	rVB	1264318	2507562	48.61%	6.094%




Sum of corrected areas: 41146426

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019185.D
Acq On : 30 Dec 2023 02:39
Operator : MA/JU
Sample : 06020-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

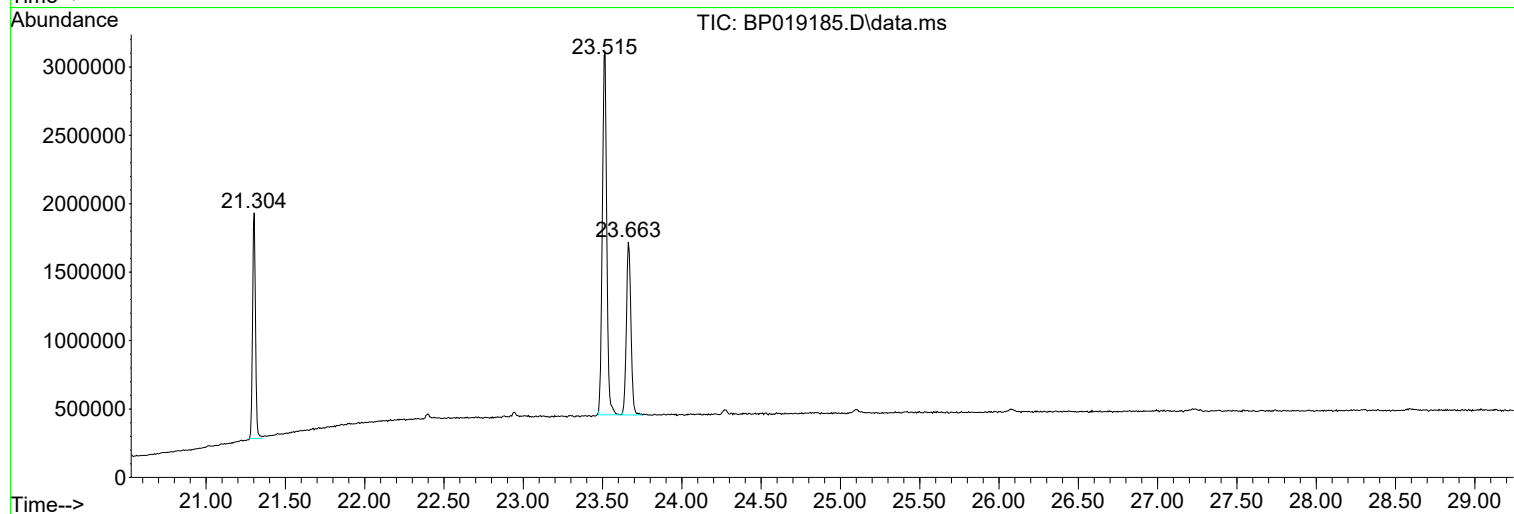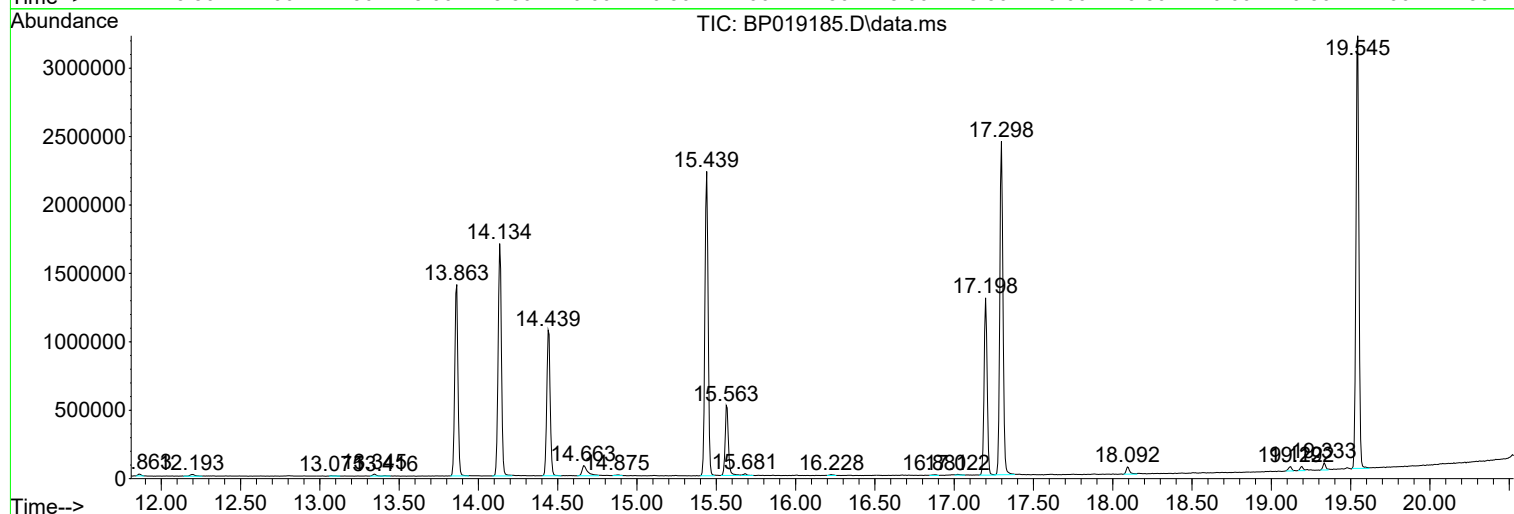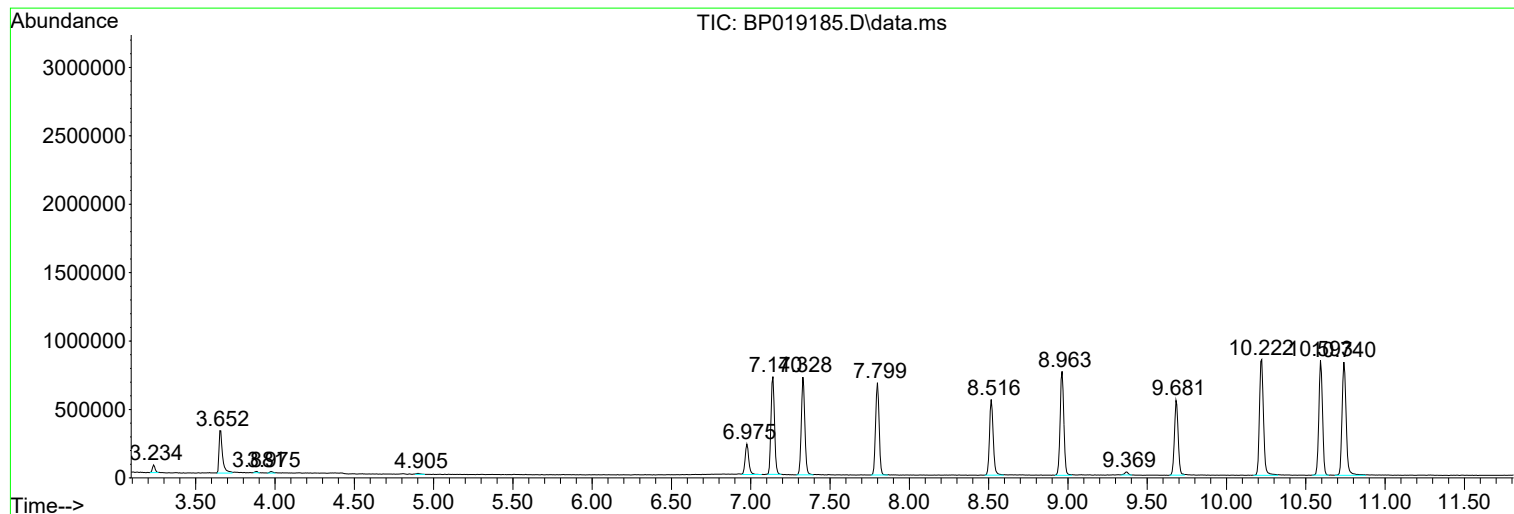

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019185.D
Acq On : 30 Dec 2023 02:39
Operator : MA/JU
Sample : 06020-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019185.D
Acq On : 30 Dec 2023 02:39
Operator : MA/JU
Sample : 06020-02
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------