

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019187.D
 Acq On : 30 Dec 2023 03:47
 Operator : MA/JU
 Sample : 06020-04
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH3P2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	15	19	22	rBV	22549	27433	0.45%	0.063%
2	3.234	22	25	33	rVB	51559	63826	1.04%	0.146%
3	3.652	93	96	107	rBV	254462	377748	6.13%	0.864%
4	3.881	131	135	140	rVB2	9027	13518	0.22%	0.031%
5	3.975	148	151	155	rVB	10929	13218	0.21%	0.030%
6	4.352	211	215	220	rVB5	3818	7420	0.12%	0.017%
7	4.899	304	308	311	rBV3	5886	8126	0.13%	0.019%
8	6.975	655	661	675	rVB	188433	305236	4.95%	0.698%
9	7.140	680	689	702	rBV	707930	1105061	17.93%	2.527%
10	7.328	712	721	735	rBV	685565	1079751	17.52%	2.469%
11	7.799	794	801	810	rBV	640628	975471	15.83%	2.230%
12	8.516	916	923	939	rBV	516015	826918	13.42%	1.891%
13	8.963	991	999	1013	rBV	763945	1233371	20.02%	2.820%
14	9.369	1063	1068	1075	rVB4	9963	17773	0.29%	0.041%
15	9.681	1114	1121	1133	rBV	549011	905527	14.69%	2.071%
16	10.222	1205	1213	1231	rBV	836903	1466278	23.79%	3.353%
17	10.593	1267	1276	1285	rBV	770241	1279037	20.76%	2.925%
18	10.740	1293	1301	1321	rBV	752237	1323386	21.48%	3.026%
19	11.863	1485	1492	1499	rVB4	9698	19033	0.31%	0.044%
20	12.193	1543	1548	1555	rBV2	12265	24257	0.39%	0.055%
21	13.346	1738	1744	1751	rVB7	9696	17563	0.29%	0.040%
22	13.863	1825	1832	1844	rBV	1494996	2096328	34.02%	4.793%
23	14.134	1868	1878	1888	rBV2	1764205	2561553	41.57%	5.857%
24	14.440	1923	1930	1937	rBV	1045430	1544286	25.06%	3.531%
25	14.669	1962	1969	1991	rBV2	71852	189934	3.08%	0.434%
26	15.440	2091	2100	2113	rBV	2392516	3377778	54.81%	7.723%
27	15.563	2115	2121	2137	rVV	613774	882481	14.32%	2.018%
28	15.681	2137	2141	2148	rVB6	11402	20662	0.34%	0.047%
29	16.222	2229	2233	2238	rVB6	7995	12903	0.21%	0.030%
30	16.875	2339	2344	2350	rBV9	4951	8432	0.14%	0.019%
31	17.016	2362	2368	2373	rBV	43209	68469	1.11%	0.157%
32	17.198	2392	2399	2409	rBV	1320012	1797593	29.17%	4.110%
33	17.298	2409	2416	2433	rBV	2874725	3979578	64.58%	9.099%
34	18.092	2548	2551	2557	rBV2	18800	26761	0.43%	0.061%
35	19.122	2722	2726	2733	rVB	35900	47101	0.76%	0.108%
36	19.186	2734	2737	2742	rBV	31114	43810	0.71%	0.100%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019187.D
Acq On : 30 Dec 2023 03:47
Operator : MA/JU
Sample : 06020-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	19.333	2759	2762	2769	rBV6	21501	31387	0.51%	0.072%
38	19.545	2792	2798	2809	rBV	3683810	4985694	80.91%	11.400%
39	21.304	3092	3097	3105	rBV	1744122	2245724	36.44%	5.135%
40	23.516	3465	3473	3489	rVB2	3193654	6162183	100.00%	14.090%
41	23.663	3492	3498	3508	rVB	1311522	2561475	41.57%	5.857%




Sum of corrected areas: 43734083

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019187.D
Acq On : 30 Dec 2023 03:47
Operator : MA/JU
Sample : 06020-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

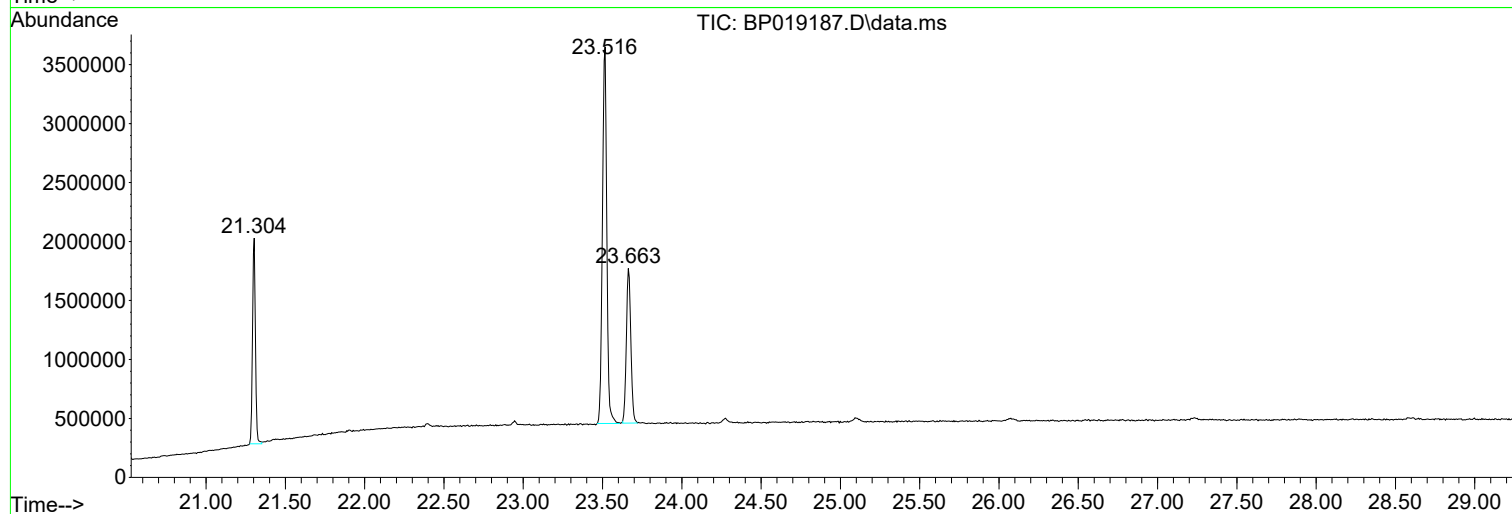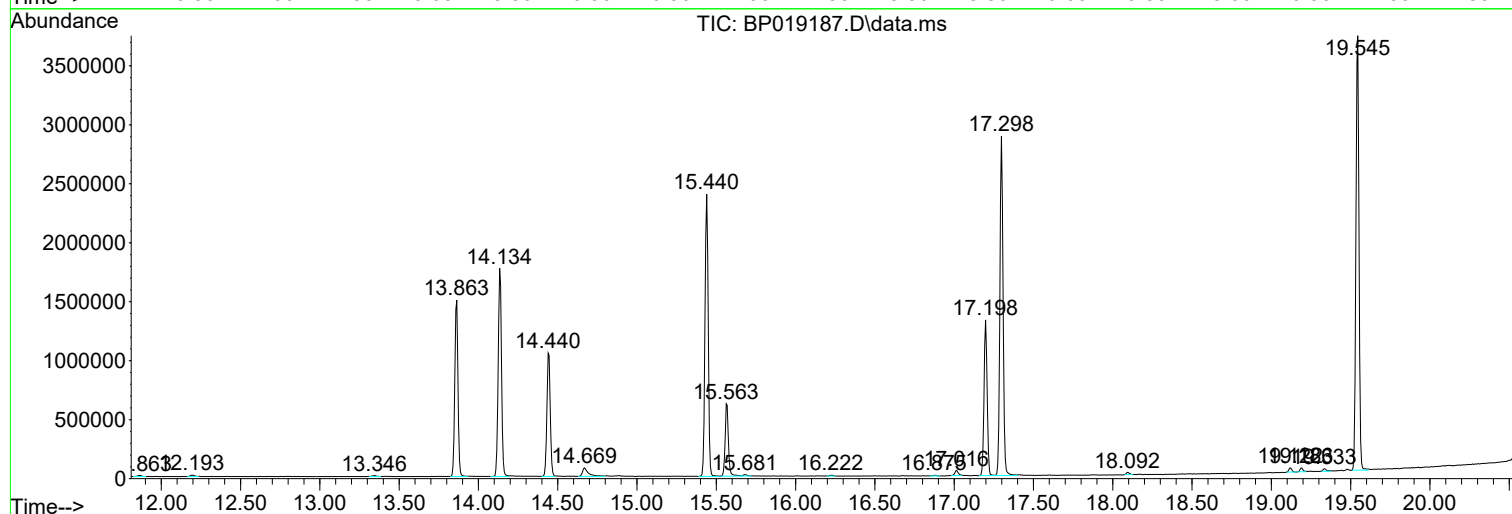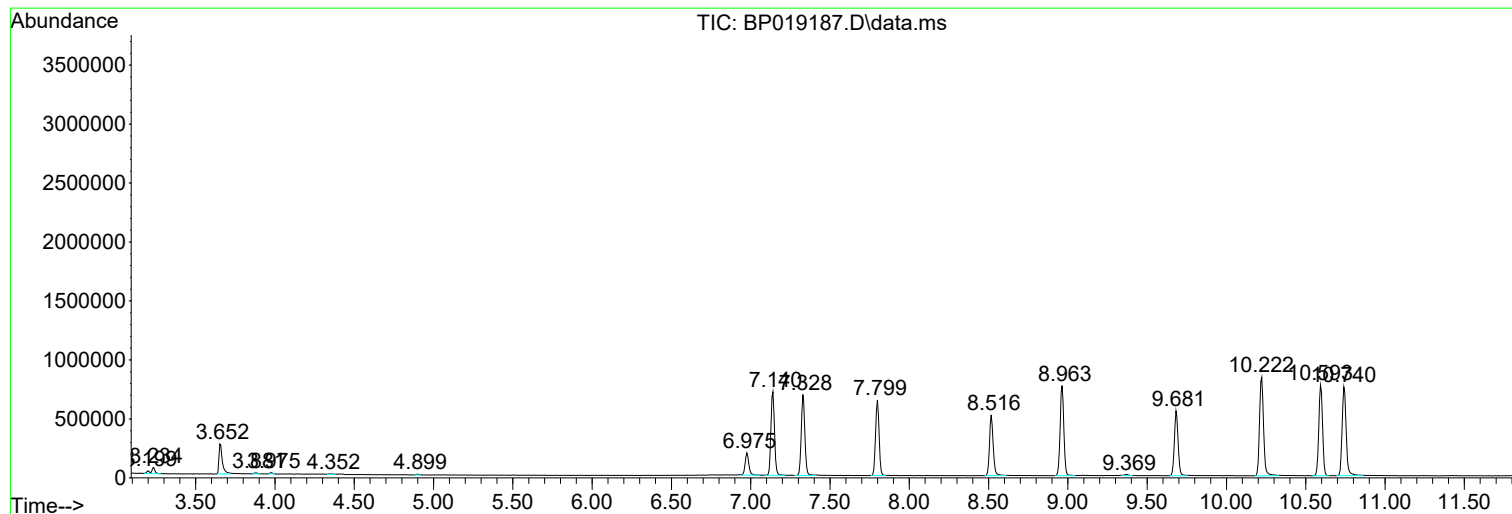

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019187.D
Acq On : 30 Dec 2023 03:47
Operator : MA/JU
Sample : 06020-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019187.D
Acq On : 30 Dec 2023 03:47
Operator : MA/JU
Sample : 06020-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH3P2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------