

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019189.D
 Acq On : 30 Dec 2023 04:55
 Operator : MA/JU
 Sample : 06020-11
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	30	rVB	38313	45257	0.75%	0.106%
2	3.658	93	97	111	rBV	204139	315362	5.24%	0.740%
3	3.881	129	135	140	rBV2	10796	19138	0.32%	0.045%
4	3.975	147	151	157	rVB	11865	16571	0.28%	0.039%
5	4.899	305	308	313	rBV2	4544	8272	0.14%	0.019%
6	6.975	656	661	678	rVB	181807	294316	4.89%	0.691%
7	7.140	682	689	703	rVB	651218	1019096	16.92%	2.392%
8	7.328	715	721	734	rBV	635741	997127	16.56%	2.341%
9	7.799	793	801	808	rBV	590570	916563	15.22%	2.152%
10	8.516	914	923	940	rBV	477243	782458	12.99%	1.837%
11	8.963	990	999	1011	rBV	703645	1131735	18.79%	2.657%
12	9.369	1062	1068	1073	rVB2	18448	29984	0.50%	0.070%
13	9.681	1113	1121	1134	rBV	496808	826562	13.73%	1.940%
14	10.222	1206	1213	1233	rBV	785467	1343112	22.30%	3.153%
15	10.593	1268	1276	1285	rBV	712517	1200638	19.94%	2.819%
16	10.740	1293	1301	1318	rBV	685133	1208669	20.07%	2.838%
17	11.857	1486	1491	1497	rVB3	13844	23785	0.39%	0.056%
18	12.198	1544	1549	1556	rVB3	11047	21329	0.35%	0.050%
19	13.345	1736	1744	1749	rBV6	10729	19600	0.33%	0.046%
20	13.857	1825	1831	1841	rBV	1441483	2080690	34.55%	4.885%
21	14.134	1871	1878	1891	rBV	1685493	2405239	39.94%	5.647%
22	14.440	1924	1930	1941	rVB	1029615	1476801	24.52%	3.467%
23	14.663	1961	1968	1982	rBV2	79927	194608	3.23%	0.457%
24	14.881	1998	2005	2015	rVB2	7572	20823	0.35%	0.049%
25	15.439	2093	2100	2108	rBV	2321843	3299189	54.78%	7.745%
26	15.563	2115	2121	2132	rBV	632531	883532	14.67%	2.074%
27	15.687	2137	2142	2146	rVB5	9966	18935	0.31%	0.044%
28	16.222	2230	2233	2240	rVB7	8075	13792	0.23%	0.032%
29	17.198	2393	2399	2409	rBV	1303857	1808052	30.02%	4.245%
30	17.298	2409	2416	2431	rVV	2833527	3955554	65.68%	9.286%
31	18.092	2547	2551	2557	rBV2	47449	65305	1.08%	0.153%
32	19.122	2721	2726	2731	rBV2	39597	57814	0.96%	0.136%
33	19.186	2733	2737	2745	rBV	41110	72626	1.21%	0.171%
34	19.333	2758	2762	2768	rBV3	44802	63263	1.05%	0.149%
35	19.545	2792	2798	2806	rBV	3784240	5029063	83.51%	11.806%
36	21.304	3092	3097	3105	rBV	1795543	2297752	38.16%	5.394%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019189.D
Acq On : 30 Dec 2023 04:55
Operator : MA/JU
Sample : 06020-11
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Title : SVOA CALIBRATION

37	23.515	3465	3473	3484	rBV	3163725	6022104	100.00%	14.138%
38	23.663	3492	3498	3509	rVB	1298753	2611067	43.36%	6.130%




Sum of corrected areas: 42595783

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019189.D
Acq On : 30 Dec 2023 04:55
Operator : MA/JU
Sample : 06020-11
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

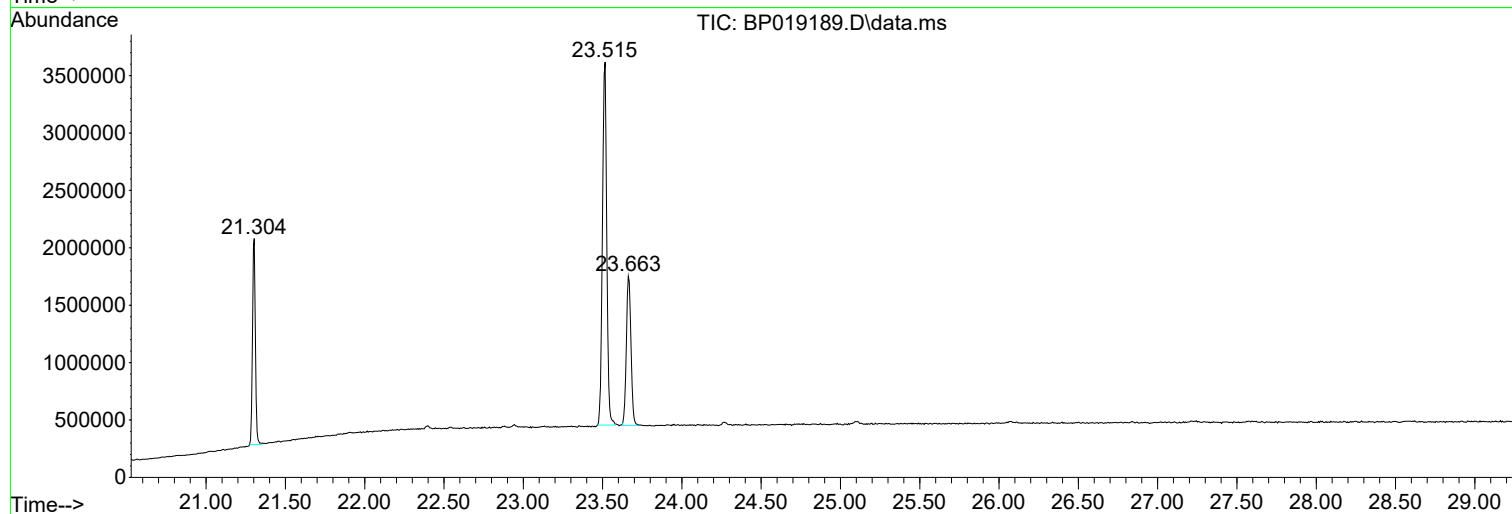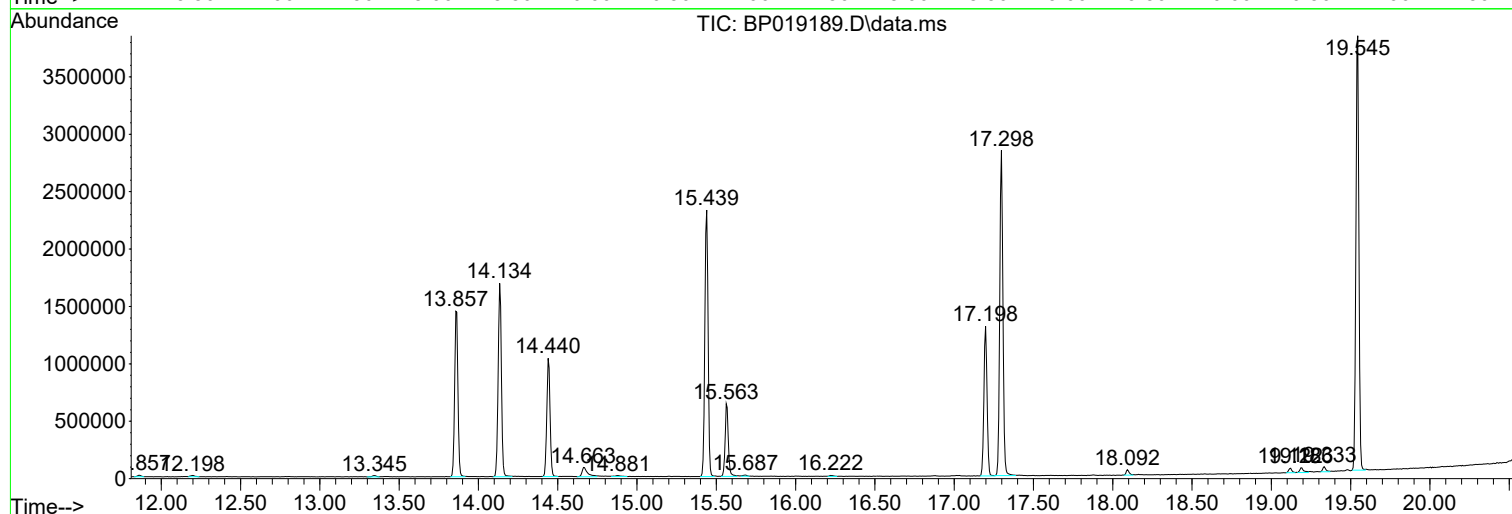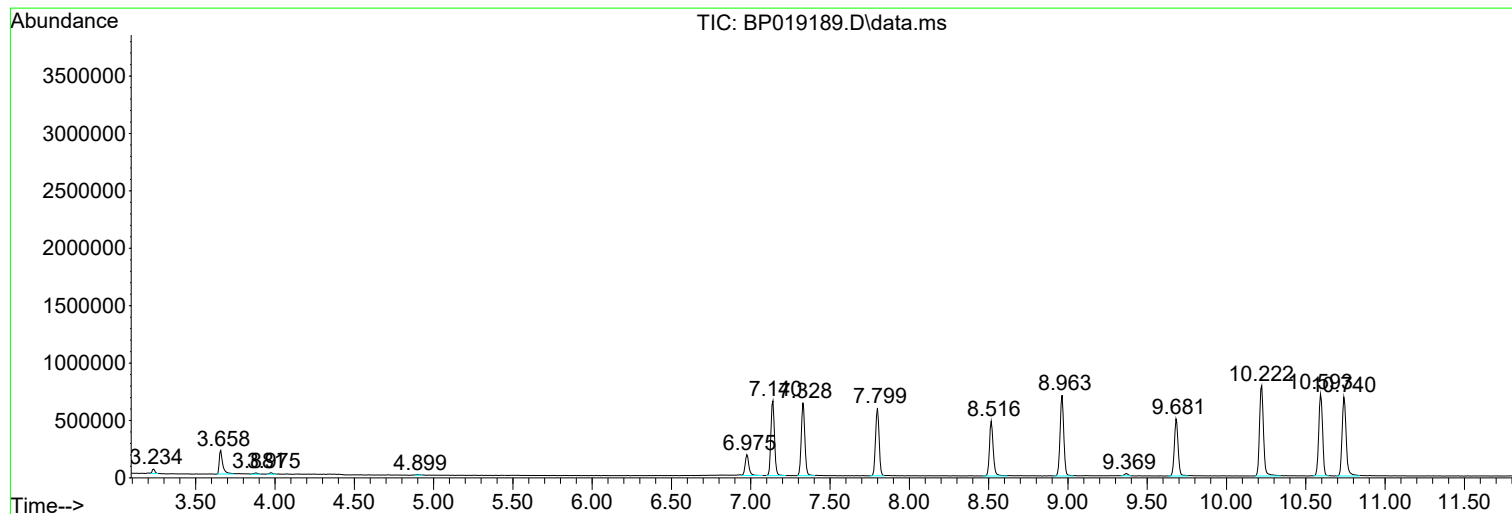

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019189.D
Acq On : 30 Dec 2023 04:55
Operator : MA/JU
Sample : 06020-11
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019189.D
Acq On : 30 Dec 2023 04:55
Operator : MA/JU
Sample : 06020-11
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc