

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019191.D
 Acq On : 30 Dec 2023 06:03
 Operator : MA/JU
 Sample : 06020-13
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	33	rVB	49202	64083	0.80%	0.110%
2	3.658	93	97	111	rBV	263063	462647	5.75%	0.793%
3	3.975	148	151	156	rVB2	14094	19777	0.25%	0.034%
4	4.899	306	308	319	rVB4	8691	23288	0.29%	0.040%
5	6.975	656	661	672	rVB	205432	324357	4.03%	0.556%
6	7.140	682	689	700	rVB	737689	1143126	14.22%	1.958%
7	7.328	714	721	731	rBV	693360	1097378	13.65%	1.880%
8	7.799	794	801	808	rBV	724810	1150712	14.31%	1.971%
9	8.516	916	923	936	rBV	568580	921146	11.46%	1.578%
10	8.963	989	999	1009	rBV	817377	1338367	16.64%	2.293%
11	9.310	1051	1058	1067	rBV2	63743	153789	1.91%	0.263%
12	9.681	1114	1121	1139	rBV	609131	1008660	12.54%	1.728%
13	10.216	1205	1212	1238	rBV	946747	1633569	20.32%	2.798%
14	10.593	1269	1276	1285	rVB	945006	1577907	19.62%	2.703%
15	10.740	1294	1301	1320	rBV	904487	1595659	19.84%	2.733%
16	10.910	1324	1330	1334	rBV5	9526	19165	0.24%	0.033%
17	11.857	1487	1491	1500	rVB8	5439	12152	0.15%	0.021%
18	12.193	1541	1548	1554	rBV	19557	33927	0.42%	0.058%
19	13.346	1738	1744	1749	rBV2	20143	33642	0.42%	0.058%
20	13.863	1825	1832	1844	rBV	1967809	2832159	35.22%	4.852%
21	14.134	1870	1878	1891	rBV	2263993	3254661	40.48%	5.575%
22	14.304	1901	1907	1911	rBV5	12376	25728	0.32%	0.044%
23	14.440	1924	1930	1939	rBV	1465434	2163607	26.91%	3.706%
24	14.557	1947	1950	1959	rVB	4741	10799	0.13%	0.018%
25	14.663	1961	1968	1983	rBV	138540	290653	3.61%	0.498%
26	14.881	1996	2005	2009	rBV	8721	19412	0.24%	0.033%
27	15.440	2093	2100	2108	rBV	3133218	4482250	55.74%	7.678%
28	15.563	2115	2121	2136	rBV	915924	1271344	15.81%	2.178%
29	15.675	2136	2140	2147	rVB3	14604	24706	0.31%	0.042%
30	15.810	2158	2163	2171	rVB	79630	108195	1.35%	0.185%
31	16.228	2229	2234	2240	rVB2	12193	18305	0.23%	0.031%
32	16.369	2254	2258	2264	rVB3	13401	20146	0.25%	0.035%
33	16.881	2340	2345	2351	rVB10	5529	10376	0.13%	0.018%
34	17.198	2392	2399	2409	rBV	2026797	2794972	34.76%	4.788%
35	17.298	2409	2416	2429	rVV	3793195	5348257	66.51%	9.162%
36	17.869	2510	2513	2517	rBV6	10422	12979	0.16%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
 Data File : BP019191.D
 Acq On : 30 Dec 2023 06:03
 Operator : MA/JU
 Sample : 06020-13
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH7X8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
 Title : SVOA CALIBRATION

37	17.975	2524	2531	2535	rBV10	8951	19557	0.24%	0.034%
38	18.092	2546	2551	2558	rBV2	134892	177758	2.21%	0.305%
39	18.163	2561	2563	2568	rVB	12490	15902	0.20%	0.027%
40	19.116	2721	2725	2730	rBV	57190	77400	0.96%	0.133%
41	19.186	2733	2737	2745	rBV	59054	96928	1.21%	0.166%
42	19.328	2758	2761	2767	rBV2	58805	83889	1.04%	0.144%
43	19.481	2784	2787	2791	rVB5	13559	13900	0.17%	0.024%
44	19.539	2791	2797	2804	rBV	4941536	6881429	85.58%	11.788%
45	21.022	3045	3049	3058	rBV4	97323	214065	2.66%	0.367%
46	21.298	3091	3096	3104	rBV	2732075	3561253	44.29%	6.101%
47	23.516	3465	3473	3490	rVB	4170096	8040702	100.00%	13.774%
48	23.663	3492	3498	3510	rVB	1940067	3891710	48.40%	6.667%




Sum of corrected areas: 58376393

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019191.D
Acq On : 30 Dec 2023 06:03
Operator : MA/JU
Sample : 06020-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

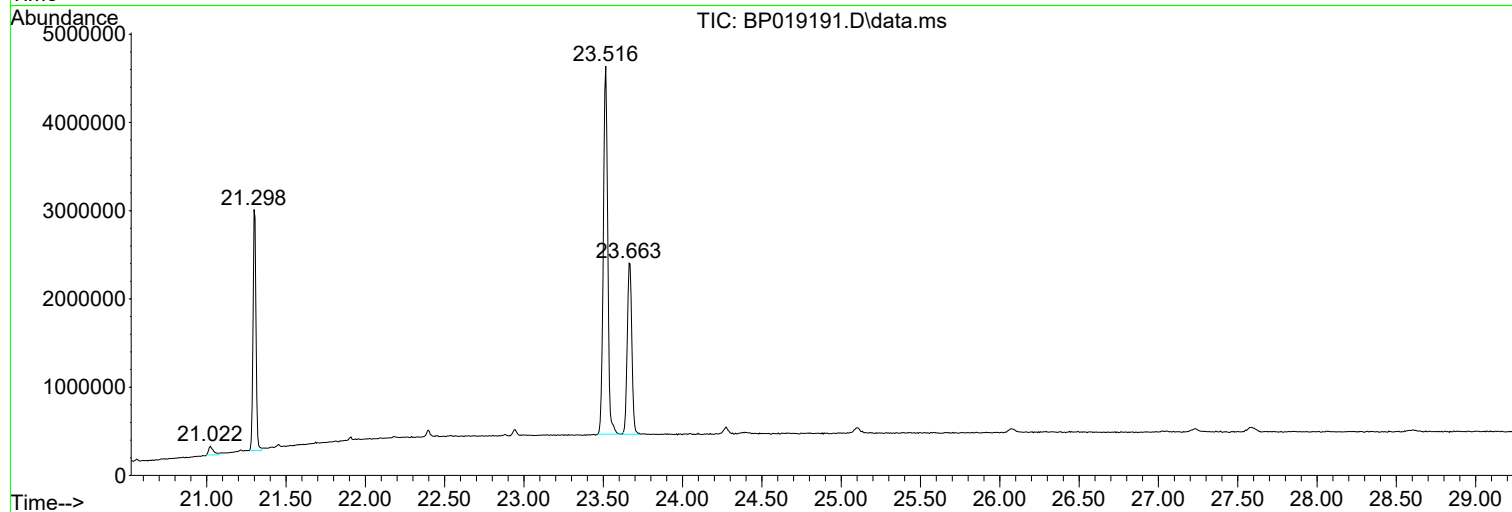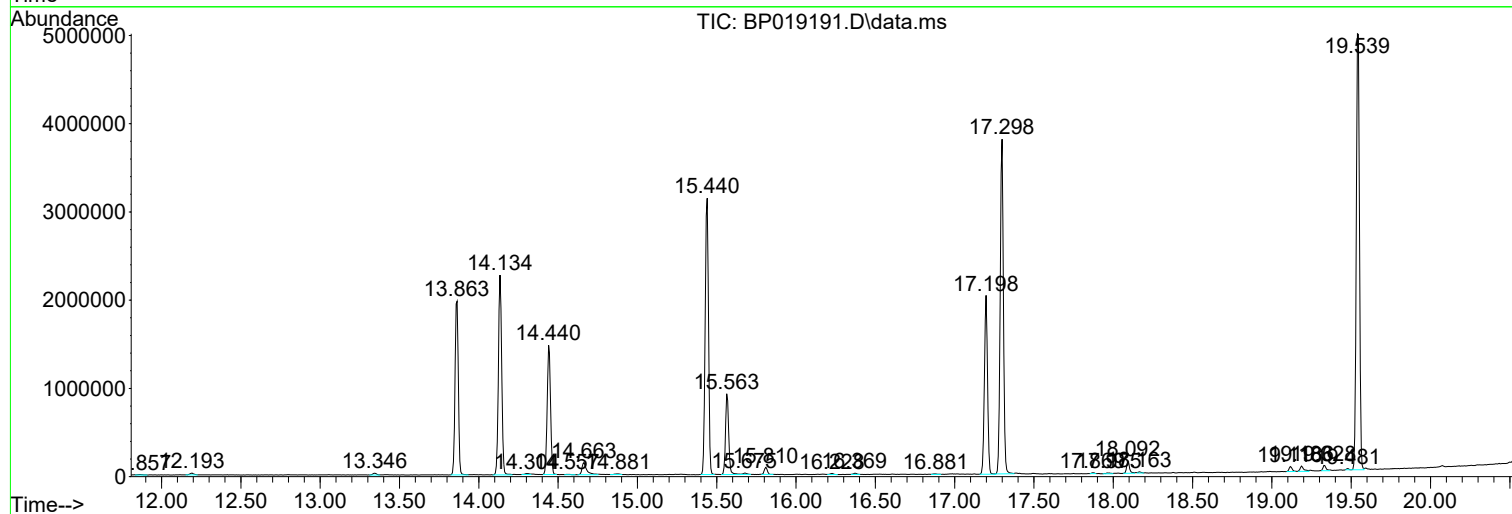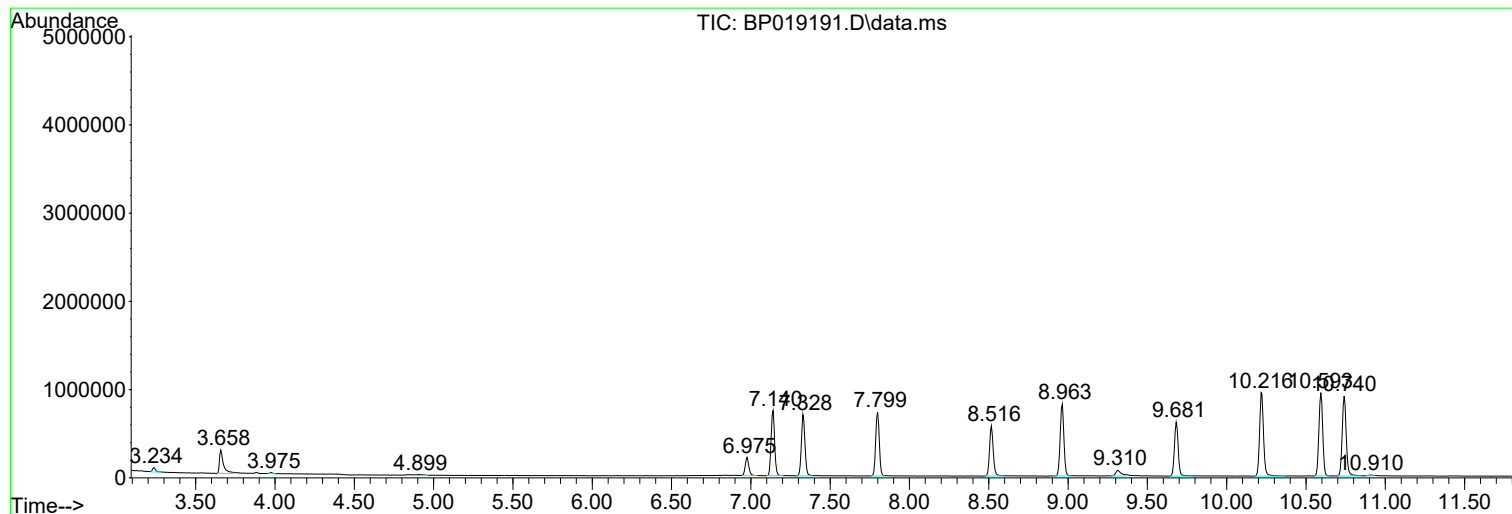

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019191.D
Acq On : 30 Dec 2023 06:03
Operator : MA/JU
Sample : 06020-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122823\
Data File : BP019191.D
Acq On : 30 Dec 2023 06:03
Operator : MA/JU
Sample : 06020-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH7X8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP122723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc