




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
 Data File : BP013361.D
 Acq On : 29 Dec 2022 13:49
 Operator : CG/JU
 Sample : N6128-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T3

Manual IntegrationsAPPROVED

Quant Time: Dec 29 15:29:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 12/29/2022
 Supervised By :Sohil Jodhani 12/29/2022

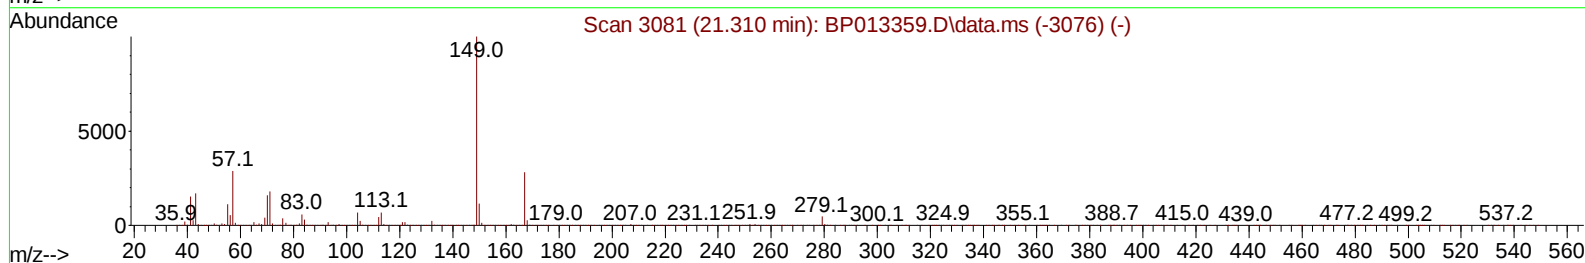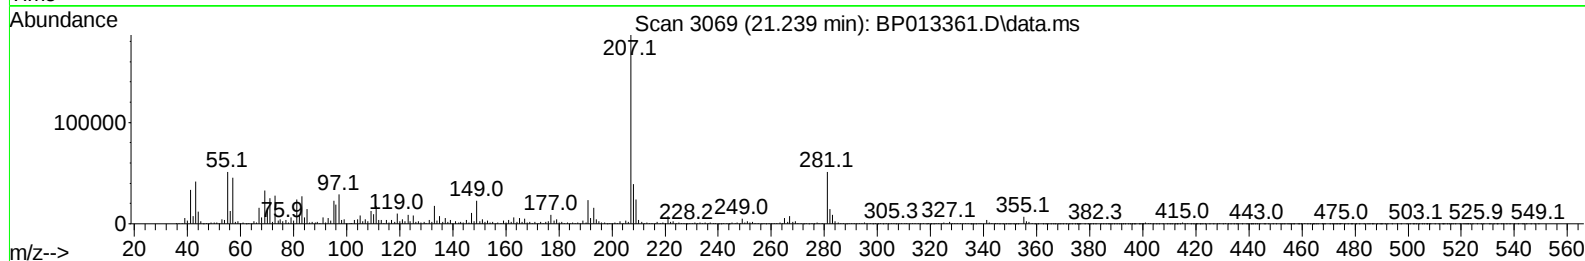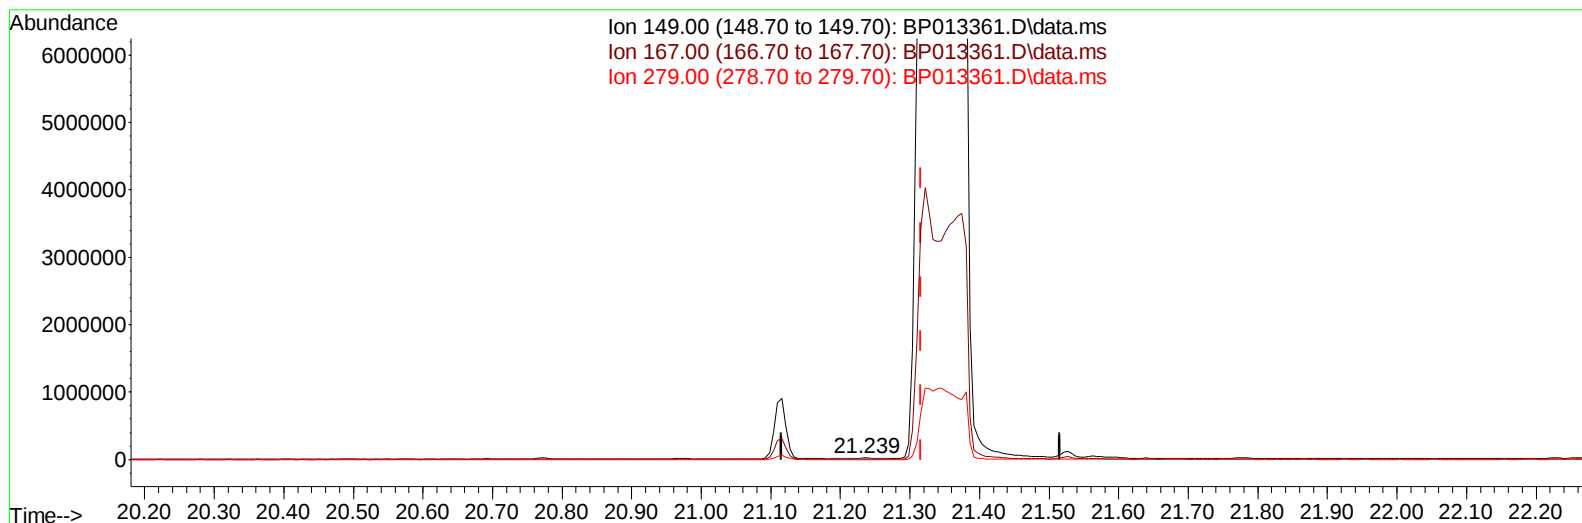

TIC: BP013361.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.239min (-0.076) 0.28 ng/u1

response 31584

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	28.10	21.13#
279.00	4.80	4.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
 Data File : BP013361.D
 Acq On : 29 Dec 2022 13:49
 Operator : CG/JU
 Sample : N6128-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T3

Manual IntegrationsAPPROVED

Quant Time: Dec 29 15:29:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 12/29/2022
 Supervised By :Sohil Jodhani 12/29/2022

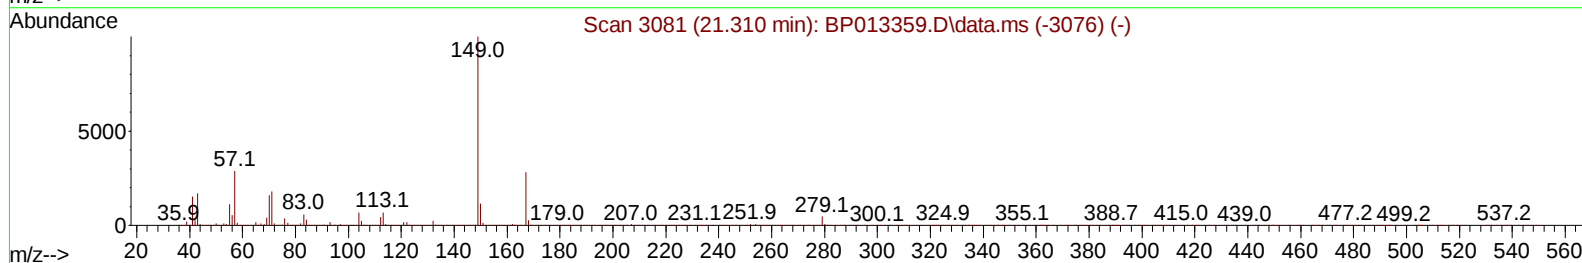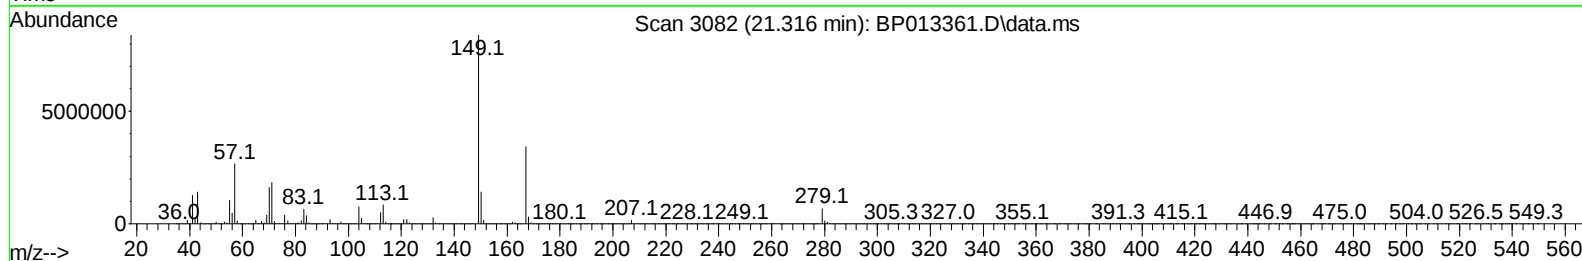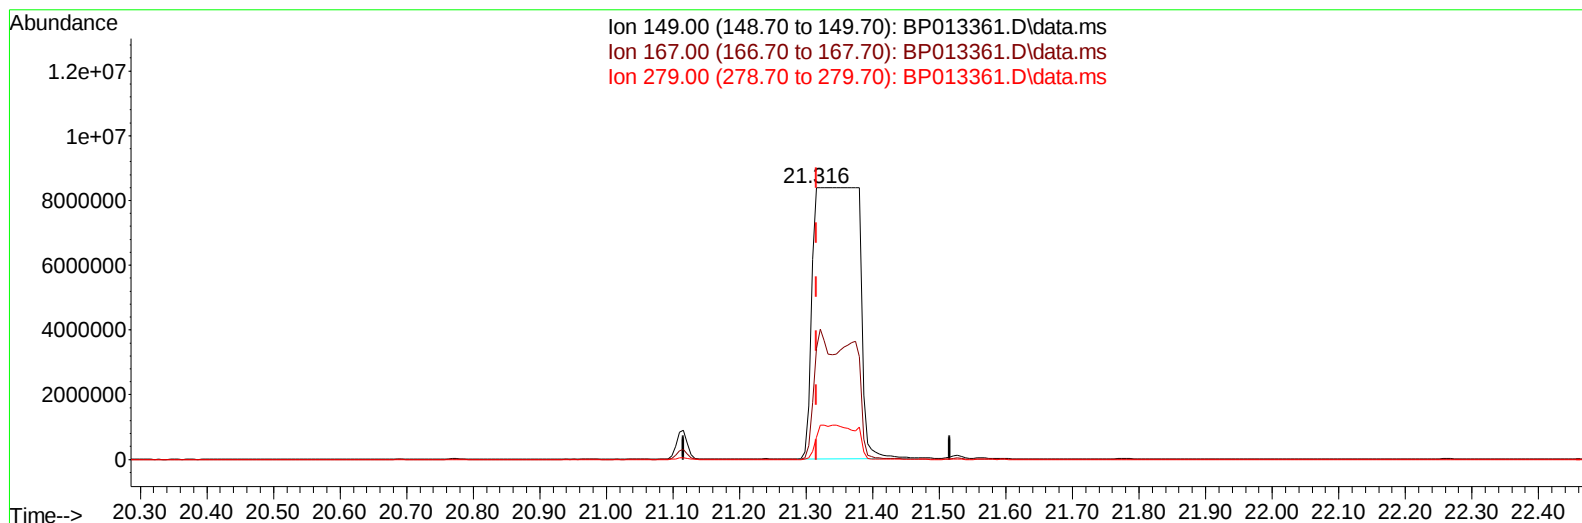

TIC: BP013361.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.316min (-0.000) 351.61 ng/ul m

response 39596948

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	28.10	40.88#
279.00	4.80	8.27#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
 Data File : BP013361.D
 Acq On : 29 Dec 2022 13:49
 Operator : CG/JU
 Sample : N6128-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T3

Manual IntegrationsAPPROVED

Quant Time: Dec 29 15:29:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 12/29/2022
 Supervised By :Sohil Jodhani 12/29/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.934	152		494971	20.000	ng/ul	0.00
20) Naphthalene-d8	10.746	136		2157305	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.581	164		1470688	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188		3500843	20.000	ng/ul	0.00
79) Chrysene-d12	21.427	240		3075082	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264		2766446	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.322	96		48963	4.230	ng/uL	0.00
4) Pyridine-d5	3.758	84		188422	5.730	ng/ul	0.01
7) Phenol-d5	7.093	99		1161485	28.809	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67		747431	30.733	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132		915800	28.855	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113		969627	29.352	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128		455650	28.747	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143		521382	29.218	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165		1017094	29.345	ng/ul	0.00
31) 4-Chloroaniline-d4	10.887	131		1329344	27.168	ng/ul	0.00
46) Dimethylphthalate-d6	13.987	166		3187240	28.198	ng/ul	0.00
49) Acenaphthylene-d8	14.275	160		3782557	30.455	ng/ul	0.00
54) 4-Nitrophenol-d4	14.781	143		501119	24.647	ng/ul	0.00
60) Fluorene-d10	15.575	176		2940976	30.756	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200		473357	21.011	ng/ul	0.00
73) Anthracene-d10	17.439	188		4455215	28.208	ng/ul	0.00
81) Pyrene-d10	19.669	212		5411950	30.661	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264		4258892	30.886	ng/ul	0.00
Target Compounds							
86) Bis(2-ethylhexyl)phtha...	21.316	149		39596948m	351.607	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
Data File : BP013361.D
Acq On : 29 Dec 2022 13:49
Operator : CG/JU
Sample : N6128-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43T3

Manual IntegrationsAPPROVED

Quant Time: Dec 29 15:29:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 28 00:16:35 2022
Response via : Initial Calibration

Reviewed By :Christian Giraldo 12/29/2022
Supervised By :Sohil Jodhani 12/29/2022

