

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
 Data File : BP013361.D
 Acq On : 29 Dec 2022 13:49
 Operator : CG/JU
 Sample : N6128-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T3

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 12/29/2022
 Supervised By : Sohil Jodhani 12/29/2022

Quant Time: Dec 29 15:29:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	494971	20.000	ng/u1	0.00
20) Naphthalene-d8	10.746	136	2157305	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.581	164	1470688	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.339	188	3500843	20.000	ng/u1	0.00
79) Chrysene-d12	21.427	240	3075082	20.000	ng/u1	0.00
88) Perylene-d12	23.898	264	2766446	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	48963	4.230	ng/uL	0.00
4) Pyridine-d5	3.758	84	188422	5.730	ng/u1	0.01
7) Phenol-d5	7.093	99	1161485	28.809	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	747431	30.733	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	915800	28.855	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	969627	29.352	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	455650	28.747	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	521382	29.218	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	1017094	29.345	ng/u1	0.00
31) 4-Chloroaniline-d4	10.887	131	1329344	27.168	ng/u1	0.00
46) Dimethylphthalate-d6	13.987	166	3187240	28.198	ng/u1	0.00
49) Acenaphthylene-d8	14.275	160	3782557	30.455	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	501119	24.647	ng/u1	0.00
60) Fluorene-d10	15.575	176	2940976	30.756	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	473357	21.011	ng/u1	0.00
73) Anthracene-d10	17.439	188	4455215	28.208	ng/u1	0.00
81) Pyrene-d10	19.669	212	5411950	30.661	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.739	264	4258892	30.886	ng/u1	0.00

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.316	149	39596948m	351.607	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
Data File : BP013361.D
Acq On : 29 Dec 2022 13:49
Operator : CG/JU
Sample : N6128-04
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A43T3

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 12/29/2022
Supervised By : Sohil Jodhani 12/29/2022


Quant Time: Dec 29 15:29:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 28 00:16:35 2022
Response via : Initial Calibration

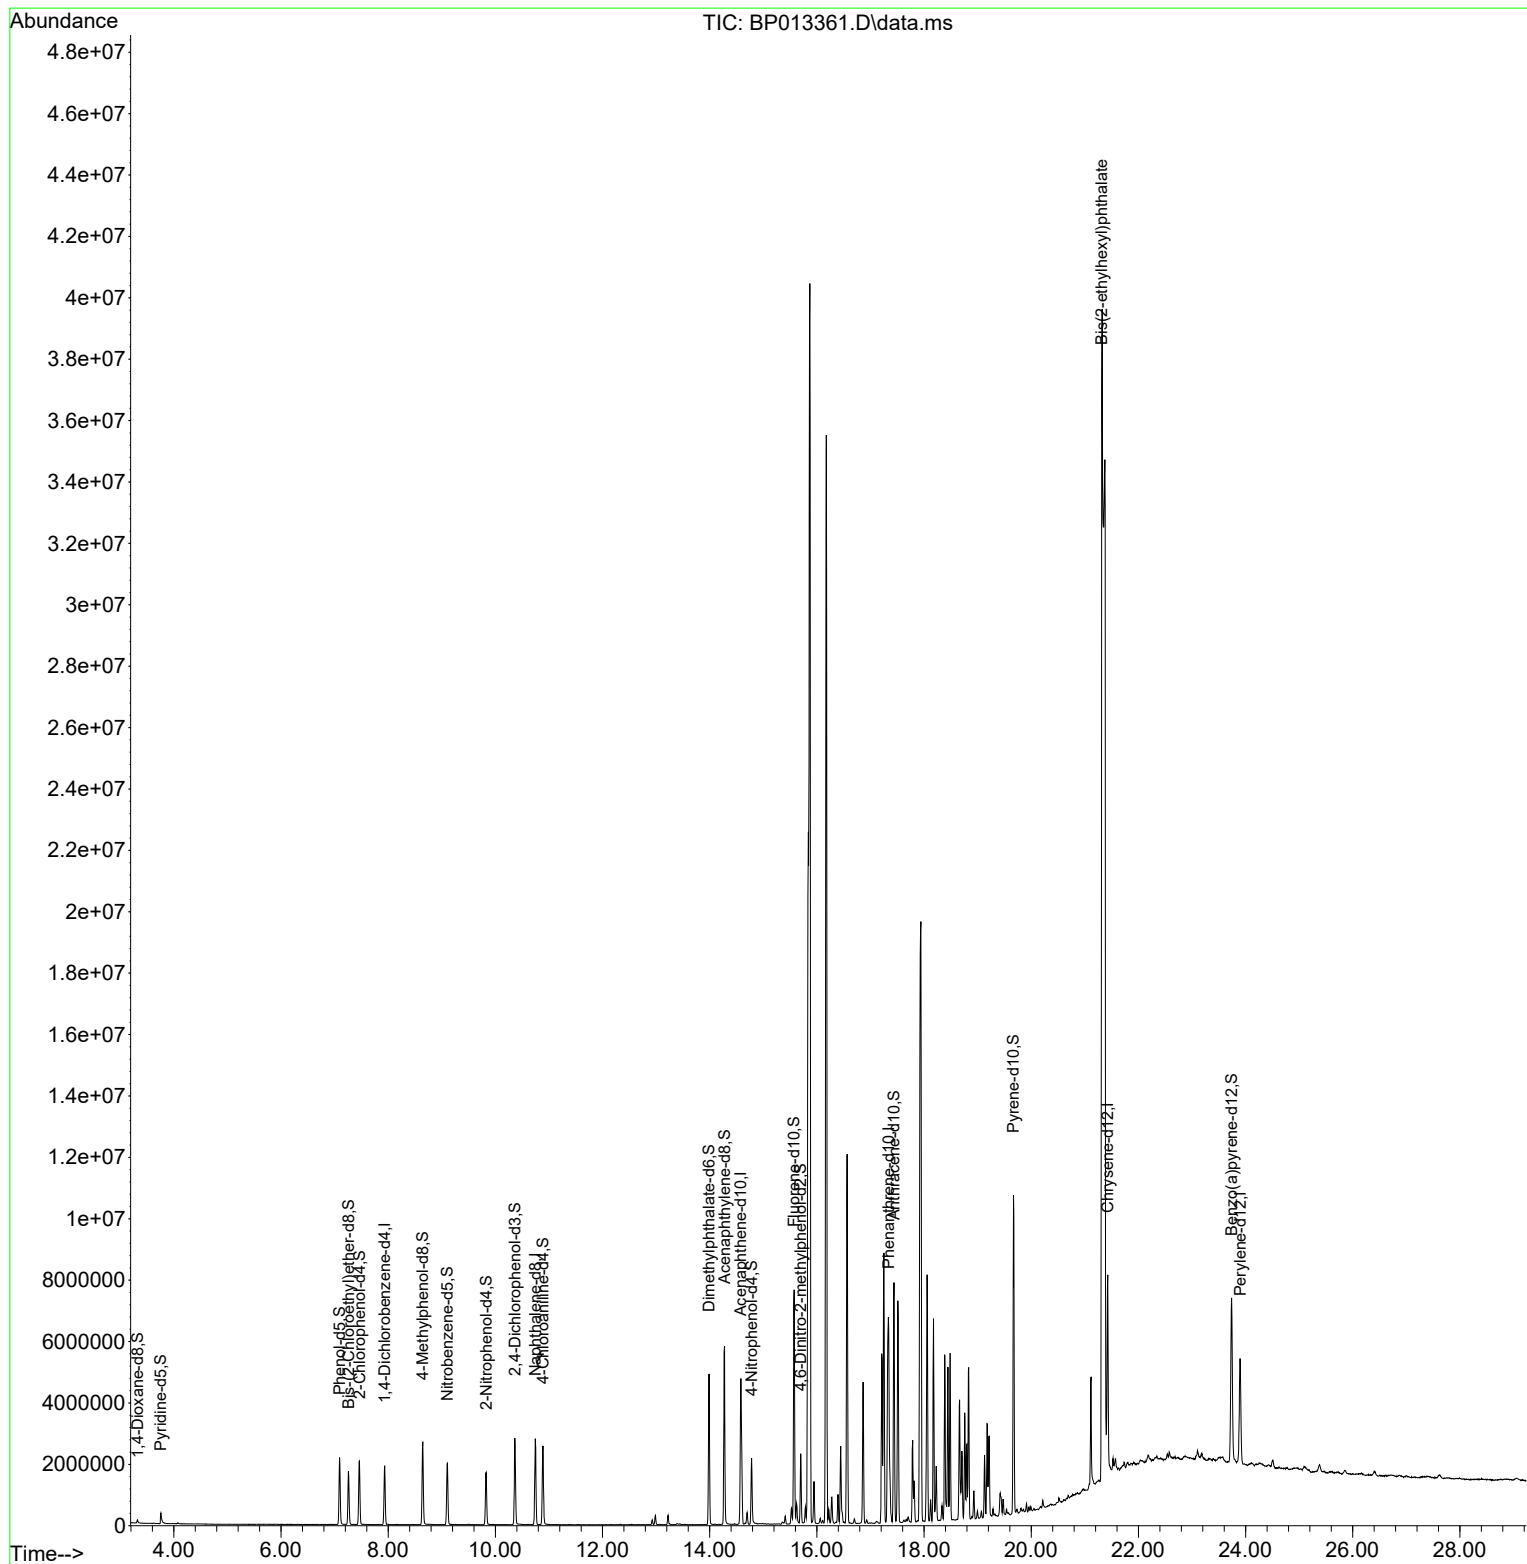

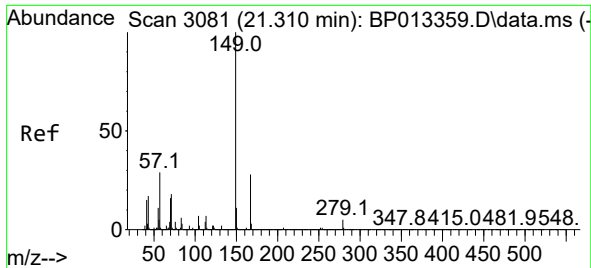

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 351.607 ng/ul m
 RT: 21.316 min Scan# 3081
 Delta R.T. -0.000 min
 Lab File: BP013361.D
 Acq: 29 Dec 2022 13:49

Instrument :
 BNA_P
 ClientSampleId :
 A43T3

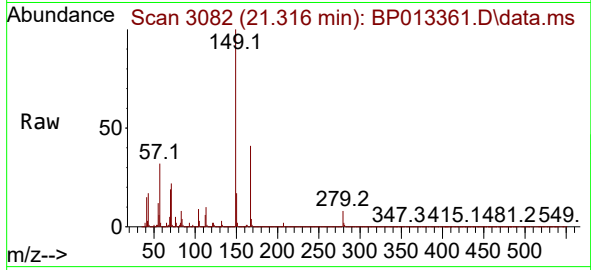

Tgt Ion:149 Resp:3959694
 Ion Ratio Lower Upper
 149 100
 167 40.9 22.5 33.7
 279 8.3 3.8 5.8

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 12/29/2022
 Supervised By :Sohil Jodhani 12/29/2022

