

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
 Data File : BP013363.D
 Acq On : 29 Dec 2022 15:29
 Operator : CG/JU
 Sample : N6128-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4492

Quant Time: Dec 29 16:02:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 28 00:16:35 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	451124	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	1947578	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	1354480	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	3117443	20.000	ng/ul	0.00
79) Chrysene-d12	21.416	240	2337569	20.000	ng/ul	0.00
88) Perylene-d12	23.880	264	2034371	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.323	96	45881	4.349	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.093	99	1041328	28.339	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.258	67	623185	28.114	ng/ul	0.00
11) 2-Chlorophenol-d4	7.458	132	785056	27.140	ng/ul	0.00
15) 4-Methylphenol-d8	8.640	113	791733	26.296	ng/ul	0.00
21) Nitrobenzene-d5	9.099	128	392254	27.412	ng/ul	0.00
24) 2-Nitrophenol-d4	9.822	143	452407	28.083	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	855140	27.329	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131	901873	20.416	ng/ul	0.00
46) Dimethylphthalate-d6	13.981	166	3257980	31.297	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	3305350	28.896	ng/ul	0.00
54) 4-Nitrophenol-d4	14.775	143	491933	26.271	ng/ul	0.00
60) Fluorene-d10	15.569	176	2865337	32.536	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	423666	21.118	ng/ul	0.00
73) Anthracene-d10	17.434	188	4701630	33.430	ng/ul	0.00
81) Pyrene-d10	19.663	212	5434191	40.500	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.722	264	3498997	34.506	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.310	149	4343943	50.742	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP122922\
Data File : BP013363.D
Acq On : 29 Dec 2022 15:29
Operator : CG/JU
Sample : N6128-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4492

Quant Time: Dec 29 16:02:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 28 00:16:35 2022
Response via : Initial Calibration

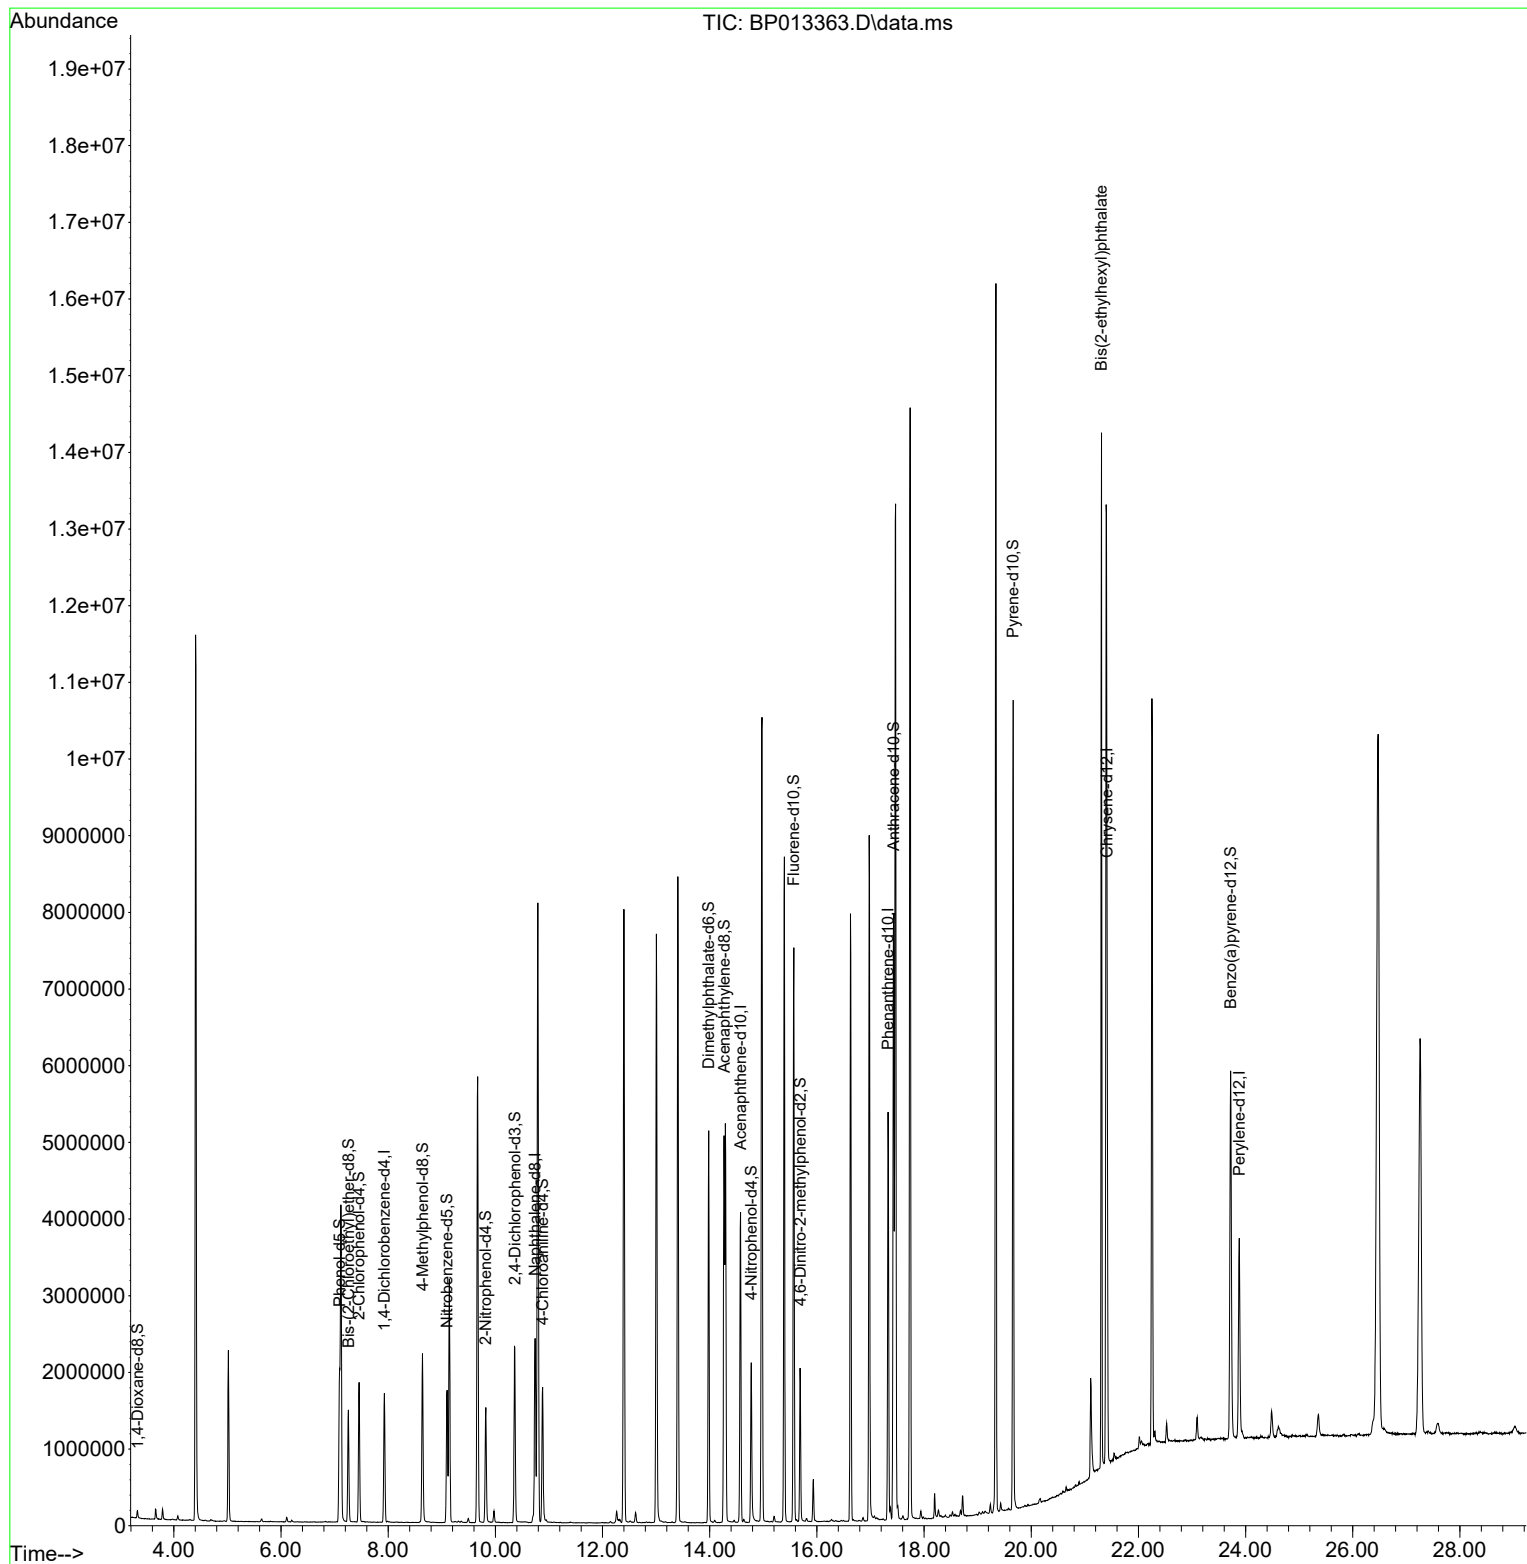

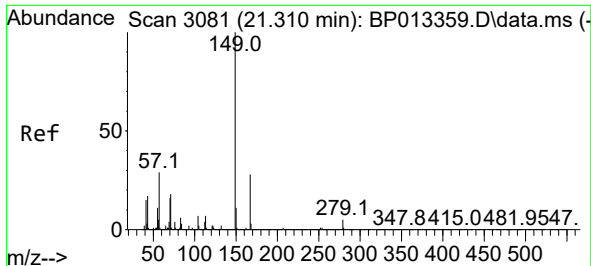

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 50.742 ng/ul
 RT: 21.310 min Scan# 3081
 Delta R.T. -0.006 min
 Lab File: BP013363.D
 Acq: 29 Dec 2022 15:29

Instrument :
 BNA_P
 ClientSampleId :
 A4492

Tgt Ion:149 Resp: 4343943
 Ion Ratio Lower Upper
 149 100
 167 28.5 22.5 33.7
 279 5.1 3.8 5.8

