

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
 Data File : BP013367.D
 Acq On : 30 Dec 2022 12:04
 Operator : CG/JU
 Sample : PB149944BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK944

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	19	23	29	rVB	124129	159925	1.79%	0.157%
2	3.746	92	95	116	rBV	1593706	2332041	26.04%	2.283%
3	4.075	147	151	155	rVB	26636	37278	0.42%	0.036%
4	7.087	656	663	673	rBV	1732894	2641151	29.50%	2.585%
5	7.257	685	692	709	rVB	1410734	2256190	25.20%	2.209%
6	7.457	719	726	736	rBV	1729259	2710586	30.27%	2.653%
7	7.928	798	806	814	rBV	1496478	2306930	25.76%	2.258%
8	8.640	919	927	944	rBV	2047155	3339820	37.30%	3.269%
9	9.093	997	1004	1017	rBV	1670618	2739947	30.60%	2.682%
10	9.822	1118	1128	1139	rBV	1359977	2280600	25.47%	2.232%
11	10.357	1212	1219	1231	rBV	2098483	3503152	39.12%	3.429%
12	10.740	1275	1284	1293	rBV	2150087	3477663	38.84%	3.404%
13	10.881	1300	1308	1329	rBV	2103965	3710379	41.44%	3.632%
14	12.328	1546	1554	1560	rBV	38387	67256	0.75%	0.066%
15	13.545	1757	1761	1765	rVB7	7412	10204	0.11%	0.010%
16	13.981	1824	1835	1845	rBV	4043751	5784005	64.59%	5.662%
17	14.263	1876	1883	1898	rBV	4546199	6675589	74.55%	6.535%
18	14.569	1928	1935	1944	rBV	3506979	5085122	56.79%	4.978%
19	14.769	1963	1969	1993	rBV	1268364	2159223	24.11%	2.114%
20	14.981	2003	2005	2010	rVB6	9291	10661	0.12%	0.010%
21	15.563	2097	2104	2119	rBV	6036598	8621034	96.28%	8.439%
22	15.686	2119	2125	2141	rVV	1708623	2264293	25.29%	2.217%
23	15.804	2141	2145	2151	rVB2	30955	50856	0.57%	0.050%
24	16.351	2234	2238	2244	rVB9	9512	13777	0.15%	0.013%
25	16.998	2346	2348	2354	rBV7	7724	11352	0.13%	0.011%
26	17.110	2364	2367	2370	rBV5	9365	11499	0.13%	0.011%
27	17.328	2397	2404	2413	rBV	4333599	5863300	65.48%	5.740%
28	17.428	2414	2421	2435	rVV	6108699	8611425	96.17%	8.430%
29	19.239	2725	2729	2733	rBV	67467	85450	0.95%	0.084%
30	19.304	2736	2740	2744	rBV	65684	98343	1.10%	0.096%
31	19.663	2795	2801	2810	rBV	6729897	8954299	100.00%	8.765%
32	21.416	3094	3099	3107	rBV	3503340	4596630	51.33%	4.500%
33	23.715	3484	3490	3501	rVB2	3602952	7146425	79.81%	6.996%
34	23.880	3512	3518	3527	rVB2	2222988	4539740	50.70%	4.444%

Sum of corrected areas: 102156145




Instrument :
BNA_P
ClientSampleId :
SBLK944

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
Data File : BP013367.D
Acq On : 30 Dec 2022 12:04
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

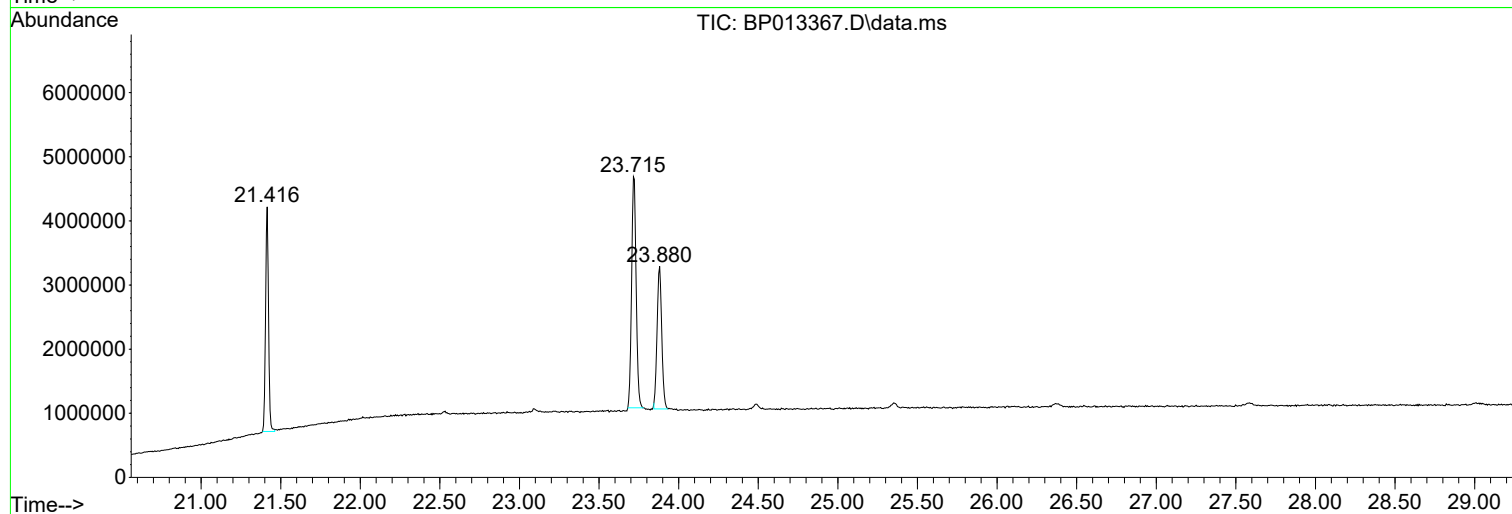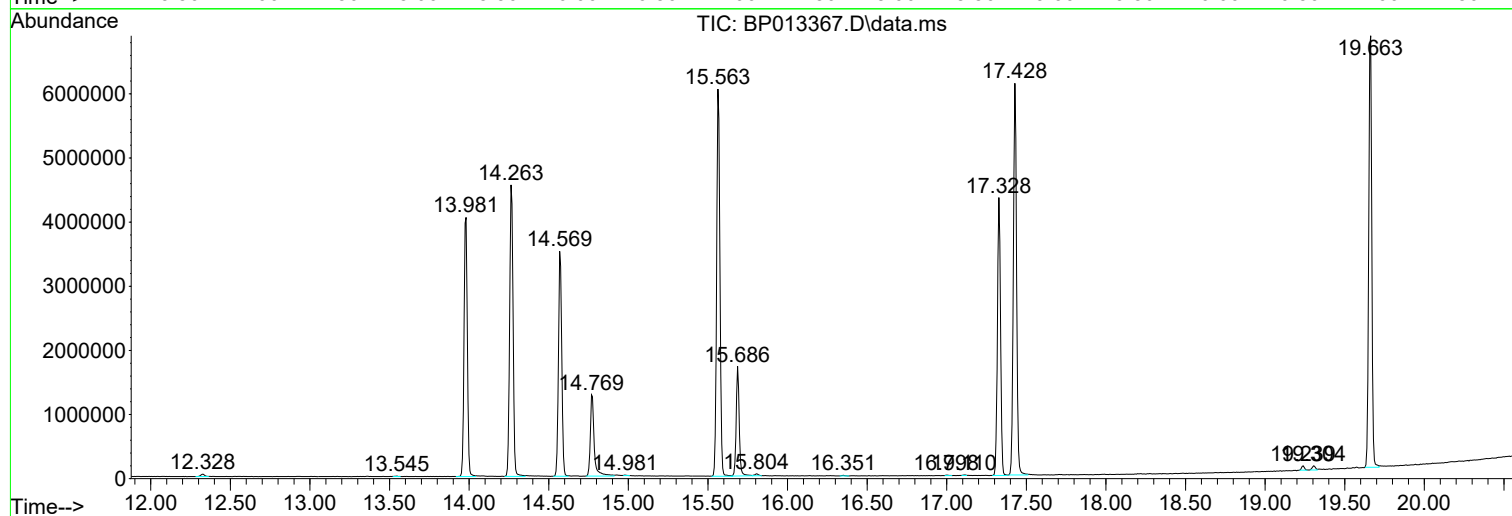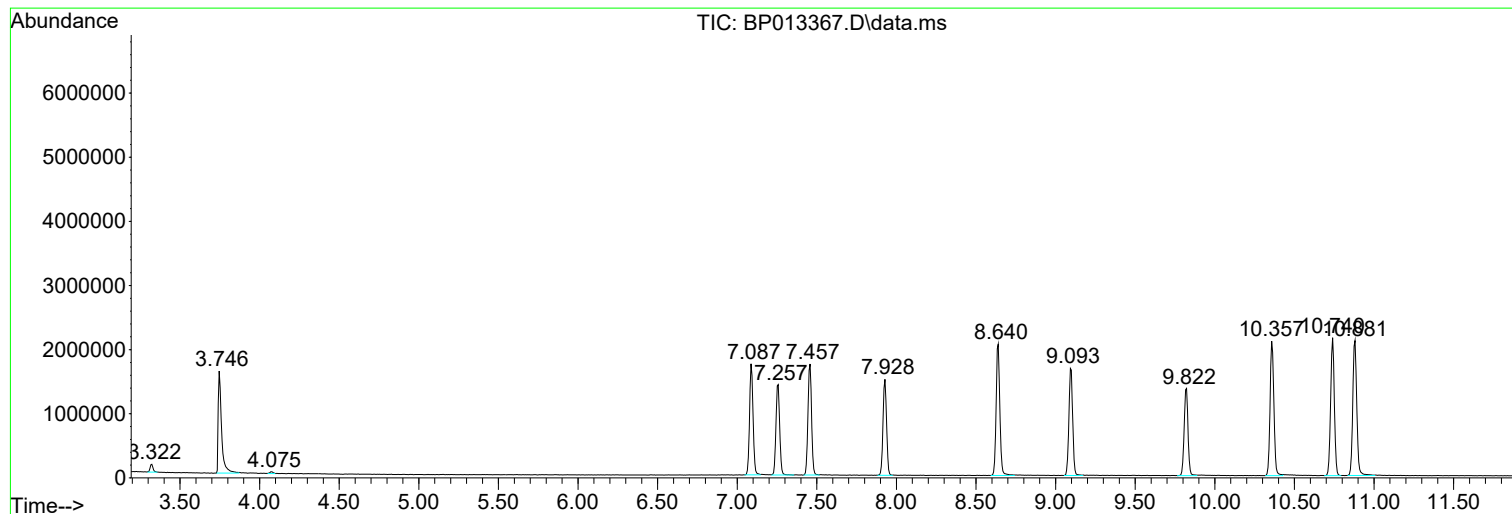

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
Data File : BP013367.D
Acq On : 30 Dec 2022 12:04
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
Data File : BP013367.D
Acq On : 30 Dec 2022 12:04
Operator : CG/JU
Sample : PB149944BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK944

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc