

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
 Data File : BP013372.D
 Acq On : 30 Dec 2022 15:06
 Operator : CG/JU
 Sample : PB149947BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK947

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.322	19	23	33	rVB	154010	214864	2.23%	0.191%
2	3.746	92	95	119	rBV	1842007	2722114	28.21%	2.414%
3	4.075	147	151	156	rVB2	32865	50594	0.52%	0.045%
4	7.010	646	650	655	rBV8	4156	10086	0.10%	0.009%
5	7.087	657	663	674	rVV	2012587	3109121	32.22%	2.758%
6	7.257	685	692	702	rVB	1673214	2574964	26.68%	2.284%
7	7.457	719	726	737	rBV	2069089	3198798	33.14%	2.837%
8	7.928	799	806	815	rBV	1758042	2692450	27.90%	2.388%
9	8.640	919	927	946	rBV	2328692	3791502	39.29%	3.363%
10	9.099	997	1005	1023	rBV	1902216	3139466	32.53%	2.785%
11	9.822	1119	1128	1139	rBV	1568743	2571427	26.64%	2.281%
12	10.357	1211	1219	1230	rBV	2386476	3893136	40.34%	3.453%
13	10.740	1273	1284	1293	rBV	2364681	3919147	40.61%	3.476%
14	10.881	1299	1308	1323	rBV	2370483	4043422	41.90%	3.586%
15	12.328	1546	1554	1562	rBV2	41167	75475	0.78%	0.067%
16	13.534	1755	1759	1765	rBV7	6672	12355	0.13%	0.011%
17	13.981	1825	1835	1848	rBV	4178647	5764915	59.73%	5.113%
18	14.087	1851	1853	1857	rVB4	10380	13082	0.14%	0.012%
19	14.263	1875	1883	1901	rBV	4690432	6985955	72.39%	6.196%
20	14.569	1929	1935	1947	rBV	3558802	5282057	54.73%	4.685%
21	14.769	1963	1969	1992	rBV	1376396	2357071	24.42%	2.091%
22	14.981	2003	2005	2011	rVB7	10898	12969	0.13%	0.012%
23	15.563	2097	2104	2119	rBV	5996331	8728499	90.44%	7.742%
24	15.686	2119	2125	2139	rVV	1761428	2357283	24.43%	2.091%
25	15.804	2141	2145	2154	rVB4	29049	49548	0.51%	0.044%
26	16.998	2346	2348	2357	rVB10	8329	15623	0.16%	0.014%
27	17.328	2396	2404	2414	rBV	4231075	5907756	61.21%	5.240%
28	17.428	2414	2421	2441	rVV	6244557	8720950	90.36%	7.735%
29	17.710	2464	2469	2470	rBV5	8297	10395	0.11%	0.009%
30	19.239	2725	2729	2733	rBV3	68239	86225	0.89%	0.076%
31	19.304	2737	2740	2744	rVB	60377	76842	0.80%	0.068%
32	19.663	2795	2801	2813	rBV	7101521	9470069	98.12%	8.400%
33	21.416	3094	3099	3108	rBV	4155162	5403925	55.99%	4.793%
34	23.721	3484	3491	3504	rVB2	4640062	9651052	100.00%	8.560%
35	23.880	3511	3518	3526	rVB2	2807195	5829908	60.41%	5.171%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
Data File : BP013372.D
Acq On : 30 Dec 2022 15:06
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 112743045

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
Data File : BP013372.D
Acq On : 30 Dec 2022 15:06
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

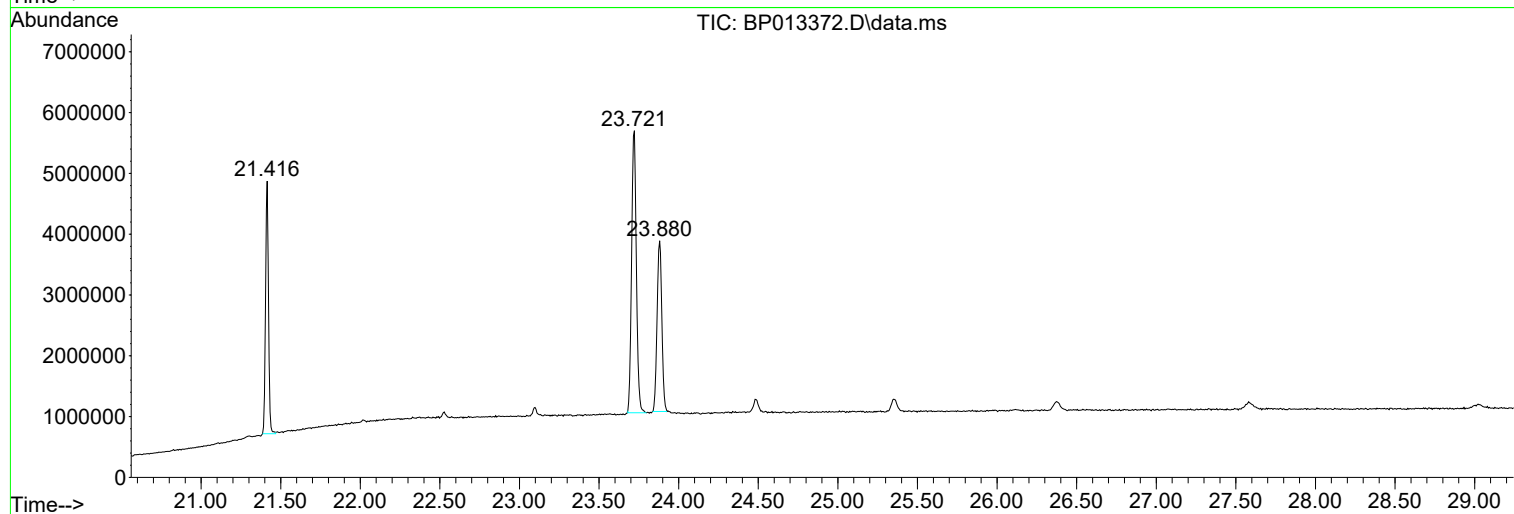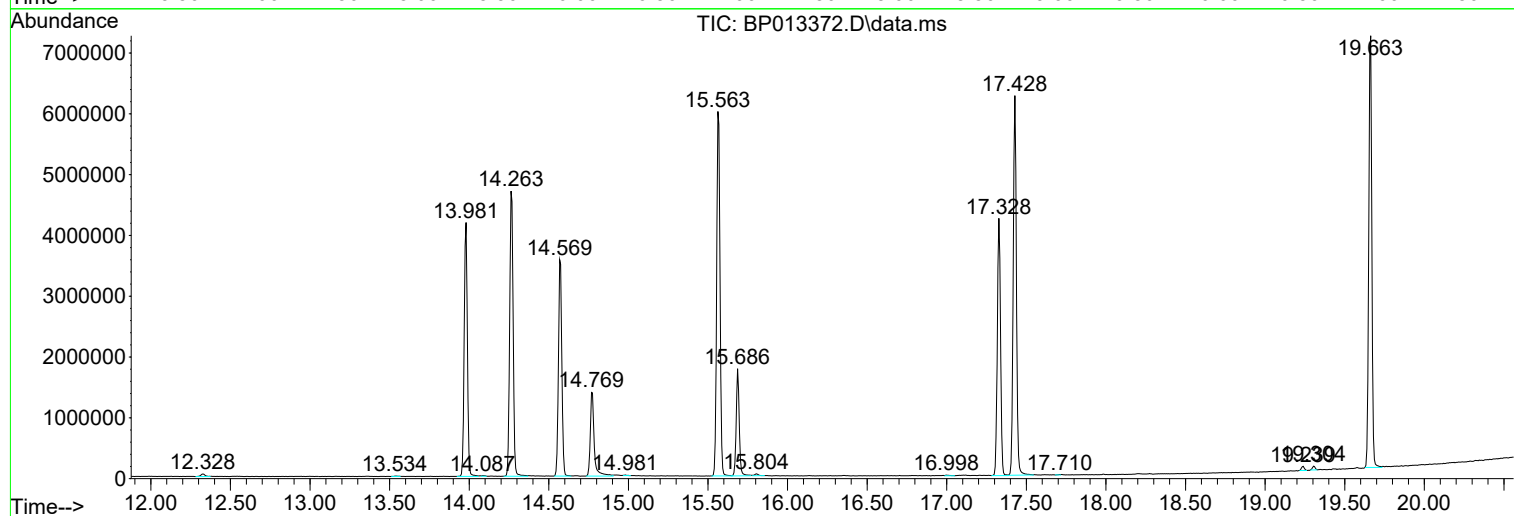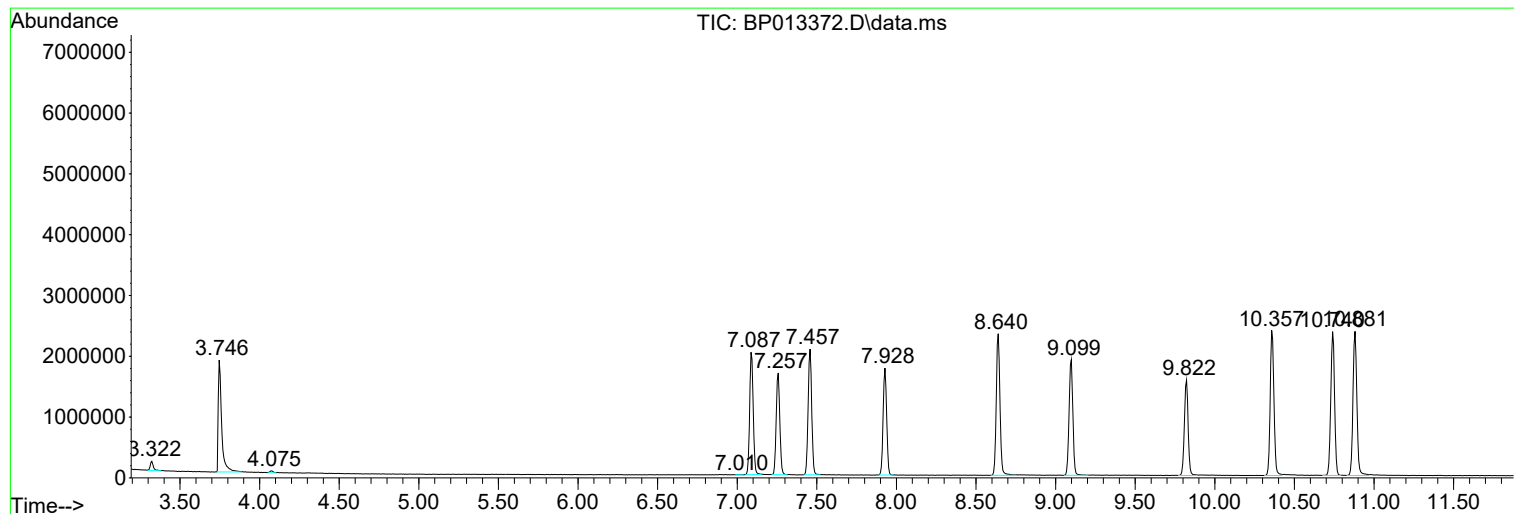

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
Data File : BP013372.D
Acq On : 30 Dec 2022 15:06
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123022\
Data File : BP013372.D
Acq On : 30 Dec 2022 15:06
Operator : CG/JU
Sample : PB149947BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc