
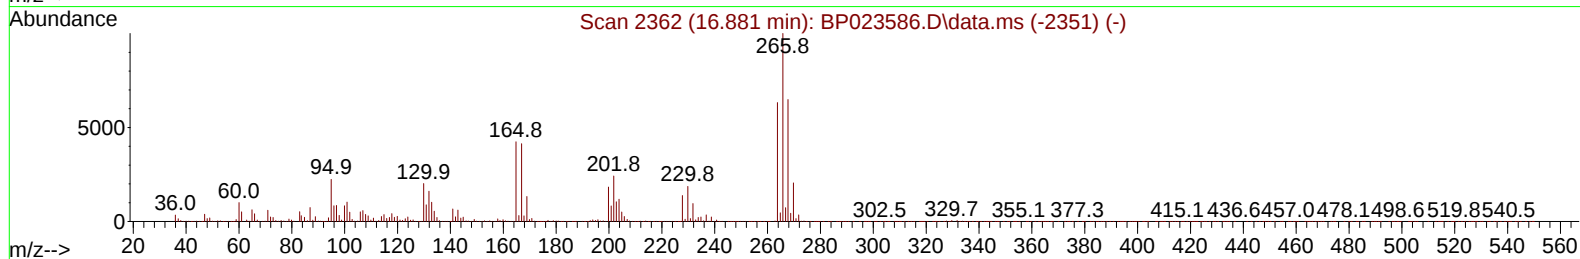
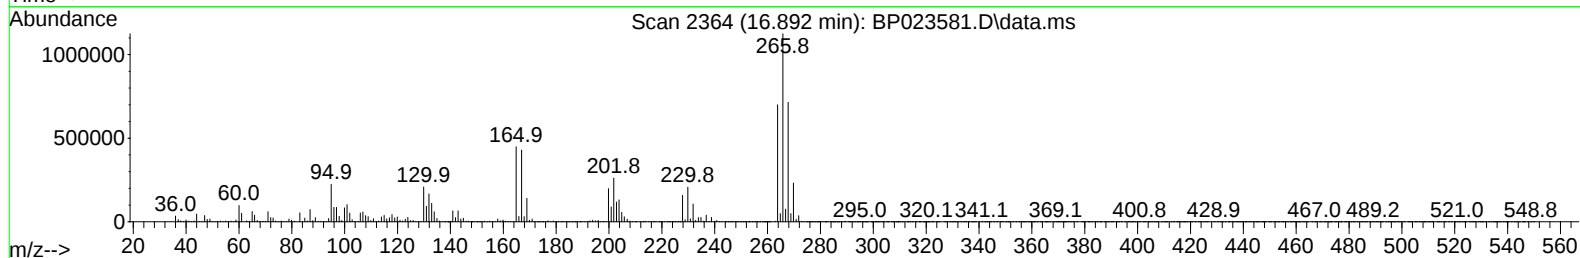


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123024\
Data File : BP023581.D
Acq On : 30 Dec 2024 09:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 16:18:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP123024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 30 16:18:08 2024
Response via : Initial Calibration

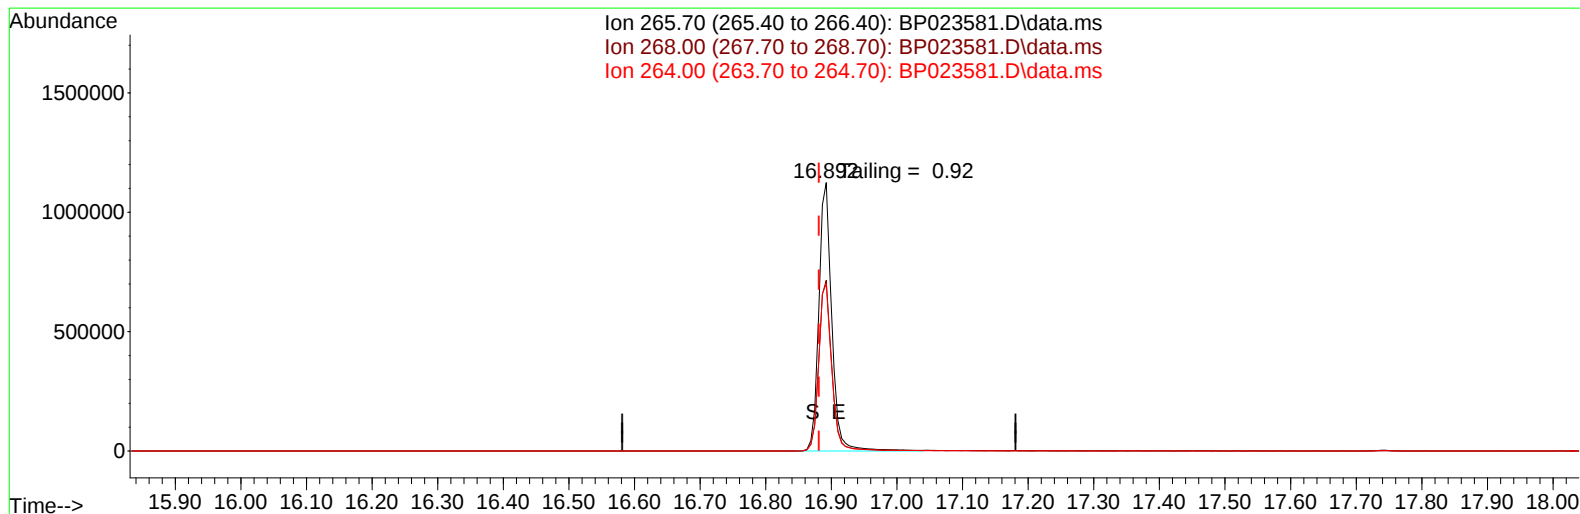

TIC: BP023581.D\data.ms

(70) Pentachlorophenol (C)




16.892min (+ 0.011) 1761437.55 ng

response 1537688

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	63.60
264.00	63.30	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123024\
Data File : BP023581.D
Acq On : 30 Dec 2024 09:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 16:18:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP123024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 30 16:18:08 2024
Response via : Initial Calibration

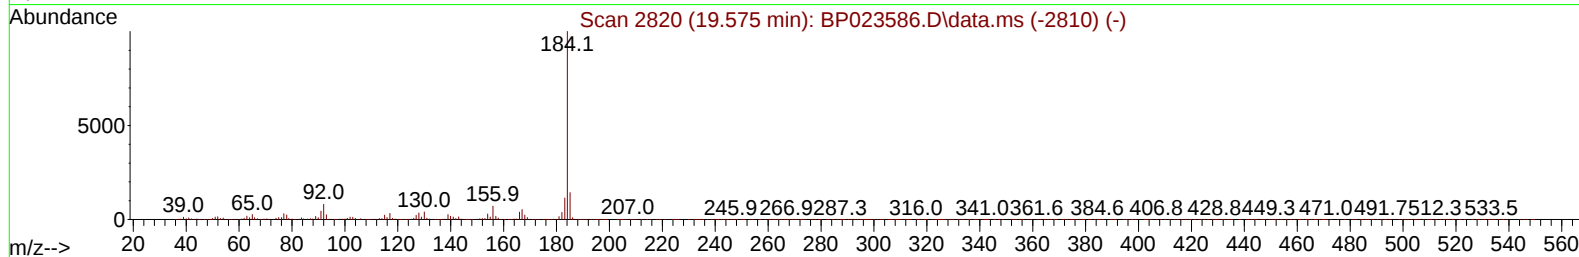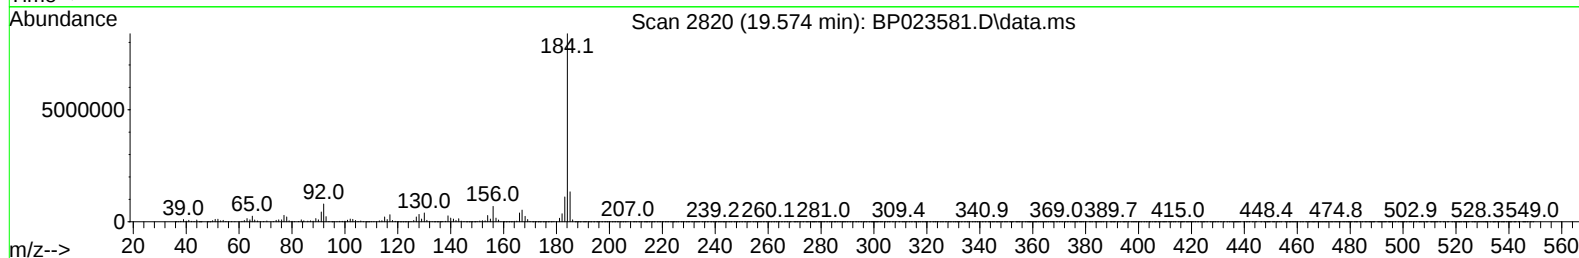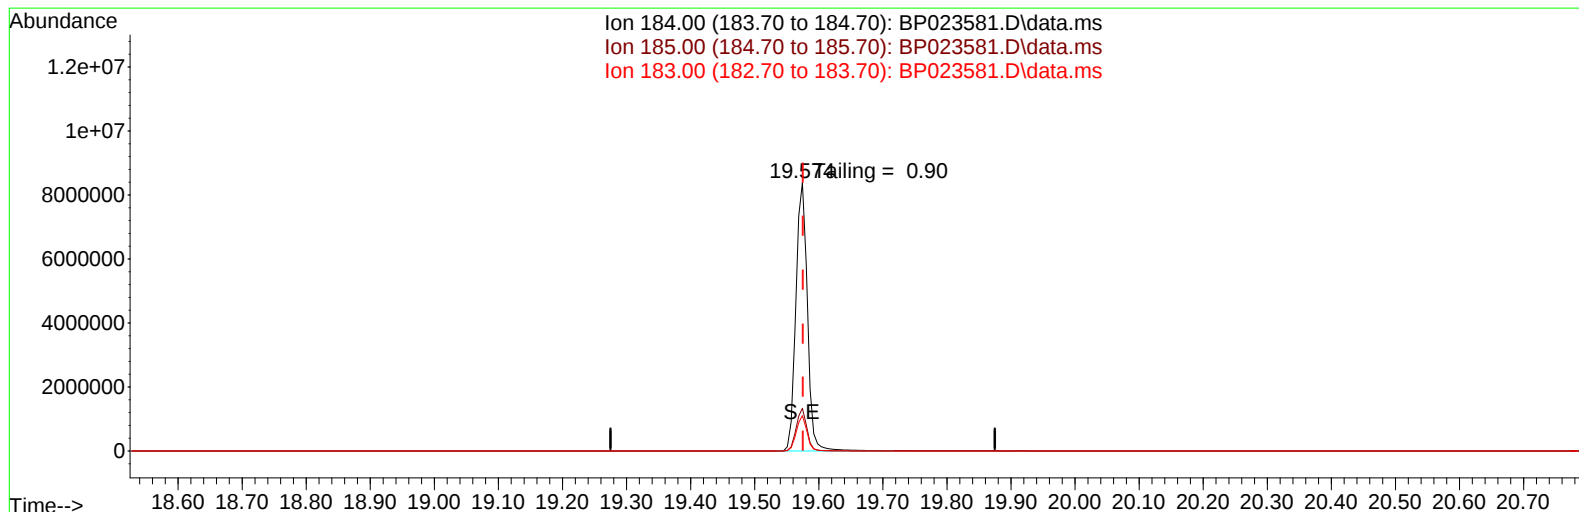

TIC: BP023581.D\data.ms

(77) Benzidine**19.574min (-0.001) 3682561.03 ng****response 10538723**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.96
183.00	11.40	13.17
0.00	0.00	0.00