
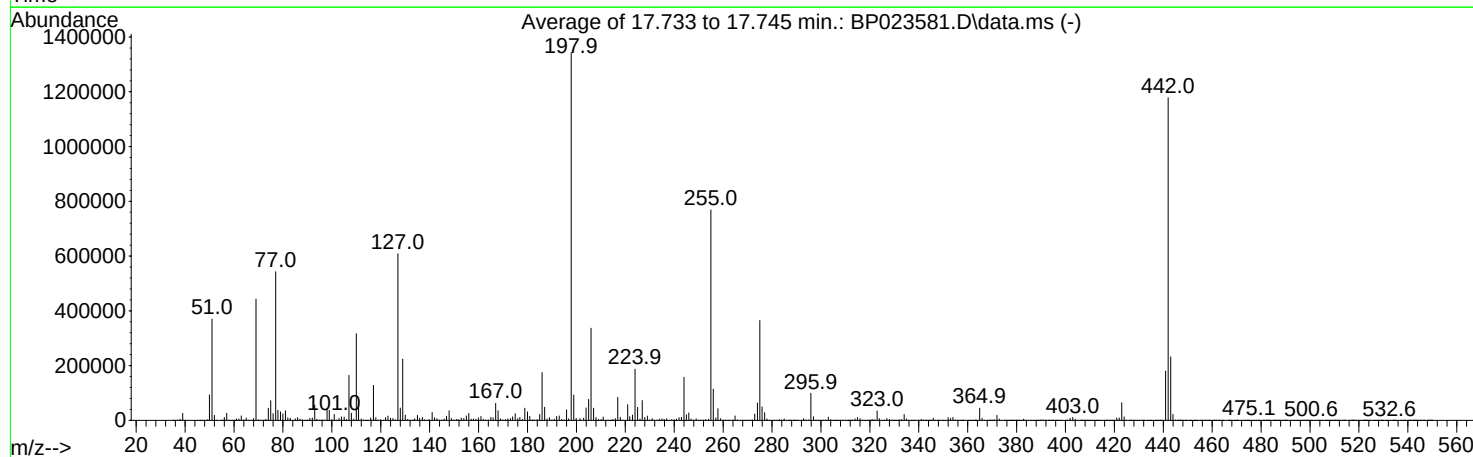


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123024\
Data File : BP023581.D
Acq On : 30 Dec 2024 09:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP123024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 30 16:39:09 2024

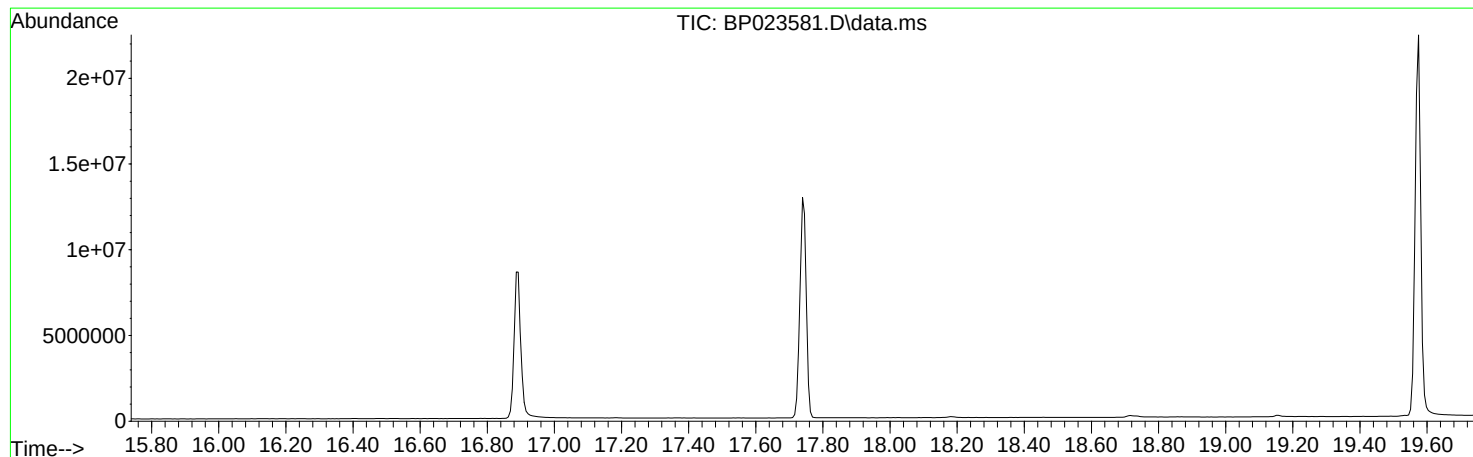

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2498

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.5	369672	PASS
68	69	0.00	2	1.5	6731	PASS
69	198	0.00	100	33.0	443087	PASS
70	69	0.00	2	0.5	2172	PASS
127	198	10	80	45.3	608533	PASS
197	198	0.00	2	0.5	6054	PASS
198	198	100	100	100.0	1343460	PASS
199	198	5	9	6.9	92263	PASS
275	198	10	60	27.1	364459	PASS
365	198	1	100	3.3	44239	PASS
441	198	0.01	100	13.4	179761	PASS
442	442	100	100	100.0	1178449	PASS
443	442	15	24	19.7	232197	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/30/2024	BNA_P	<u>BP023581.D</u>
Compound Name	Response	Retention Time
DDT	4137687	20.886
DDD	37222	20.474
DDE	1431	19.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38653	4176340	0.93

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123024\
 Data File : BP023581.D
 Acq On : 30 Dec 2024 09:34
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 30 16:18:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP123024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 30 16:18:08 2024
 Response via : Initial Calibration

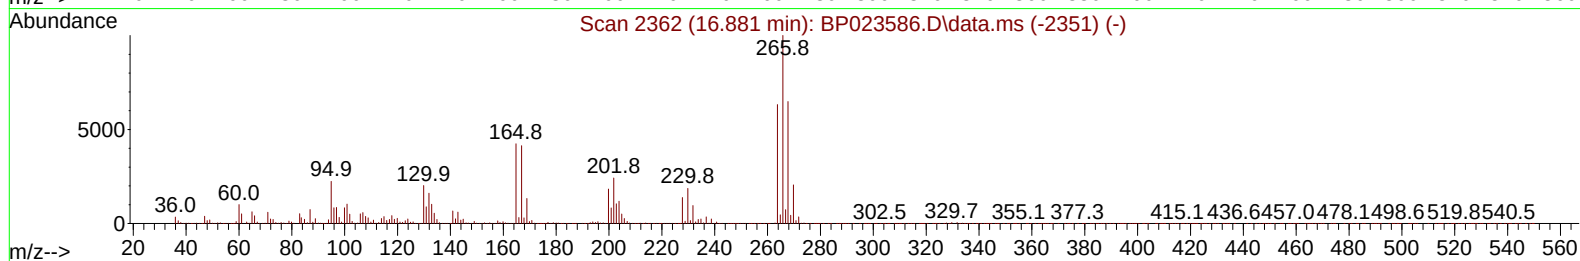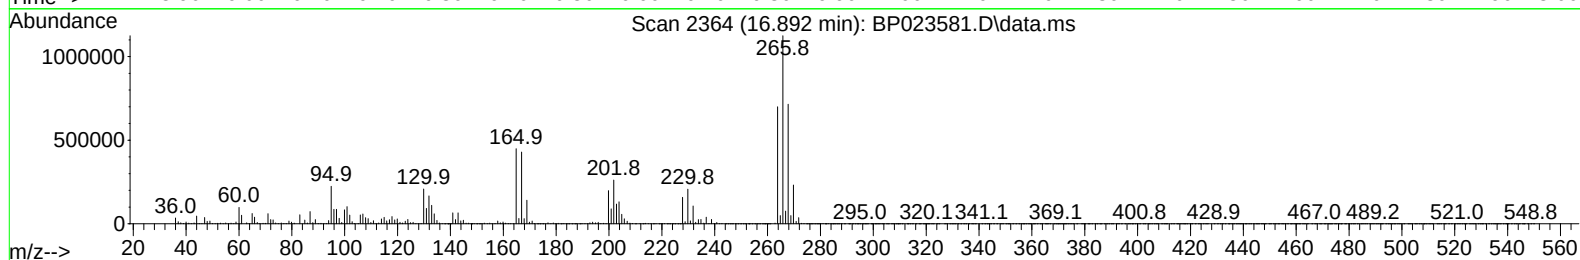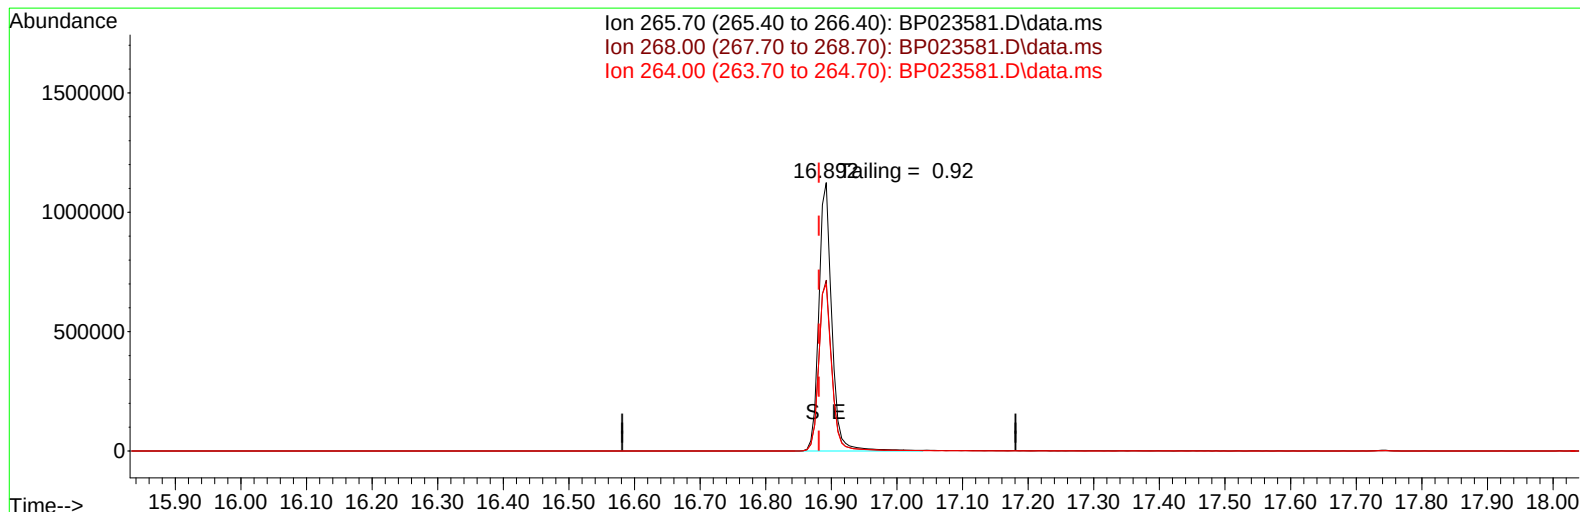

TIC: BP023581.D\data.ms

(70) Pentachlorophenol (C)

16.892min (+ 0.011) 1761437.55 ng




response 1537688

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	63.60
264.00	63.30	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP123024\
 Data File : BP023581.D
 Acq On : 30 Dec 2024 09:34
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 30 16:18:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP123024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 30 16:18:08 2024
 Response via : Initial Calibration

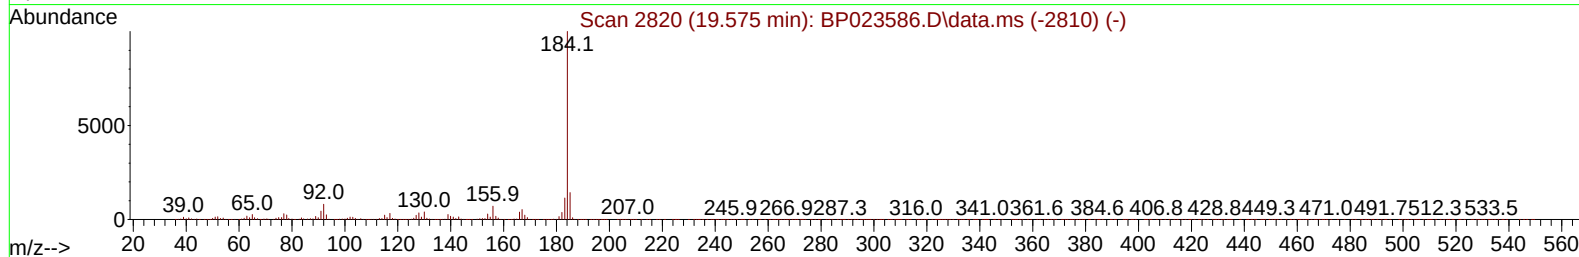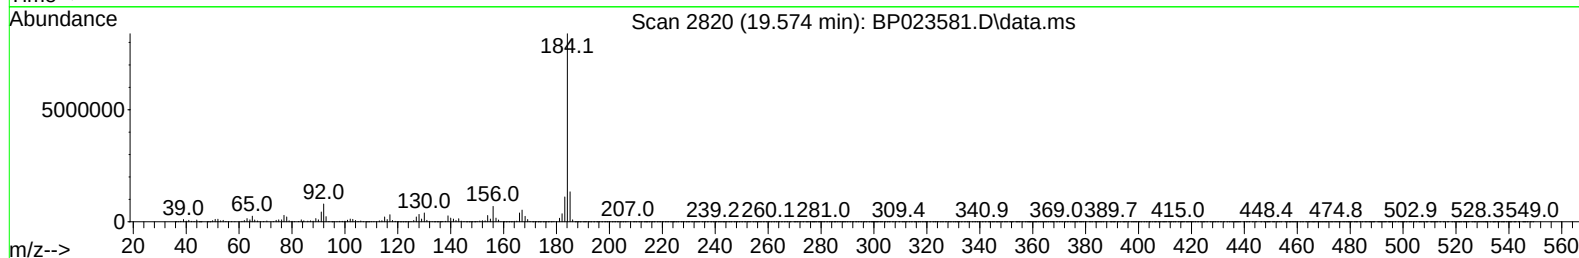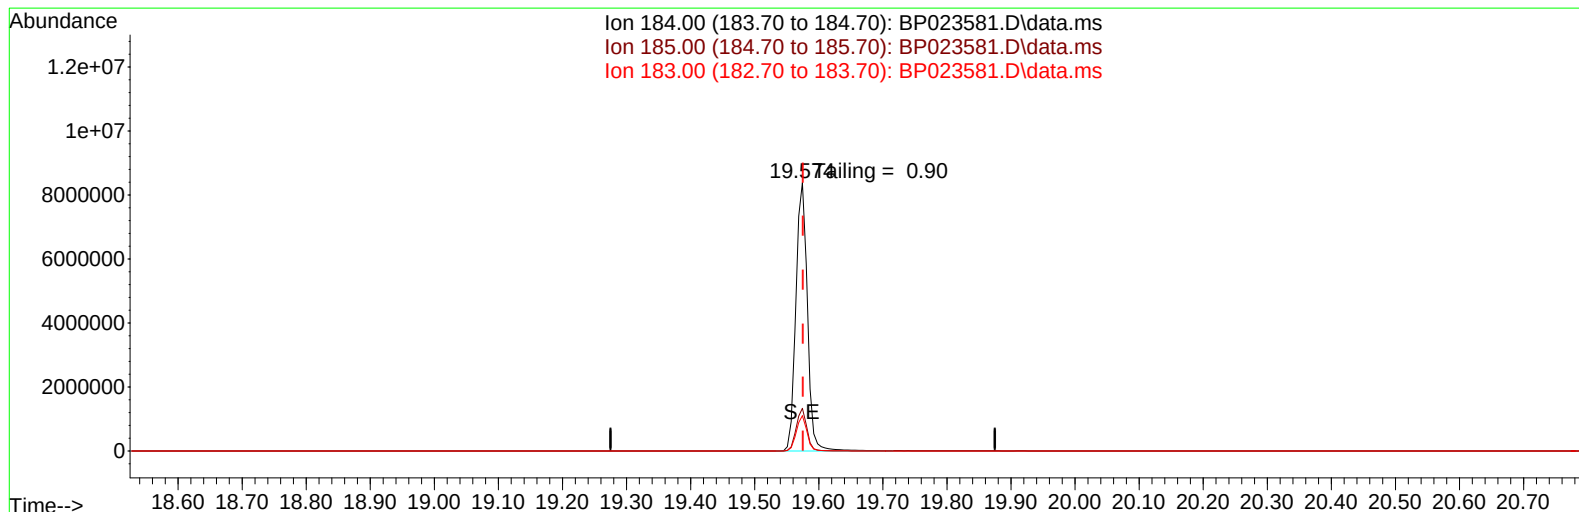

TIC: BP023581.D\data.ms

(77) Benzidine

19.574min (-0.001) 3682561.03 ng

response 10538723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.96
183.00	11.40	13.17
0.00	0.00	0.00