
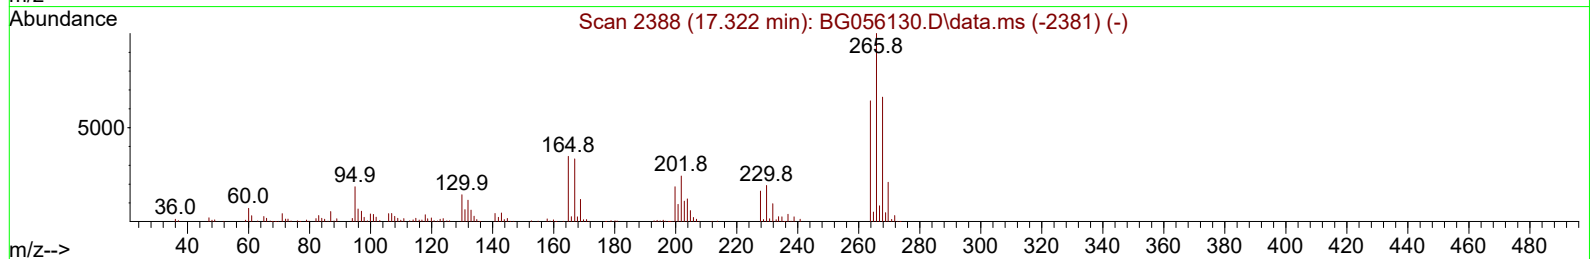
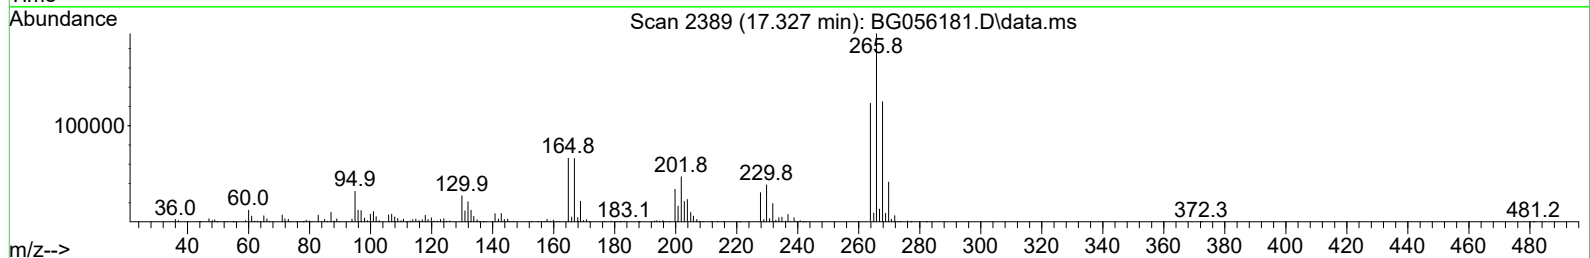


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010323\  
Data File : BG056181.D  
Acq On : 3 Jan 2023 11:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 16:25:42 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 28 05:20:14 2022  
Response via : Initial Calibration

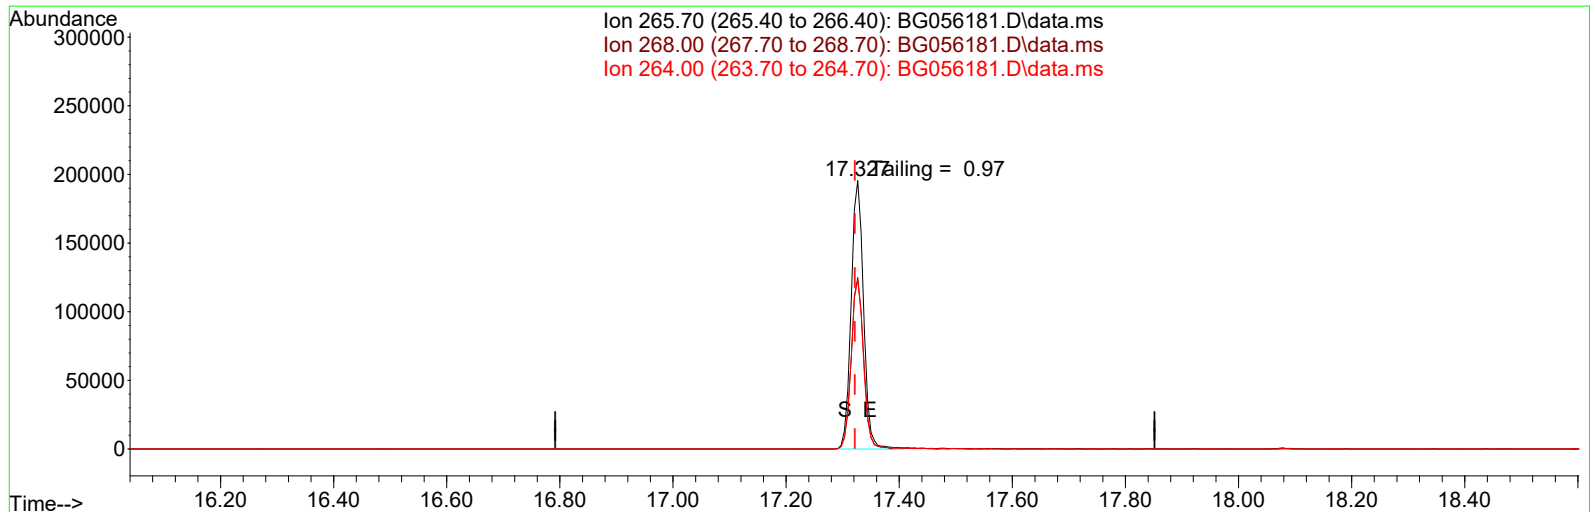

TIC: BG056181.D\data.ms

**(70) Pentachlorophenol (C)**




17.327min (+ 0.005) 251320.48 ng

response 298170

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.20  | 63.86  |
| 264.00 | 64.30  | 63.03  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010323\  
Data File : BG056181.D  
Acq On : 3 Jan 2023 11:04  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 16:25:42 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 28 05:20:14 2022  
Response via : Initial Calibration

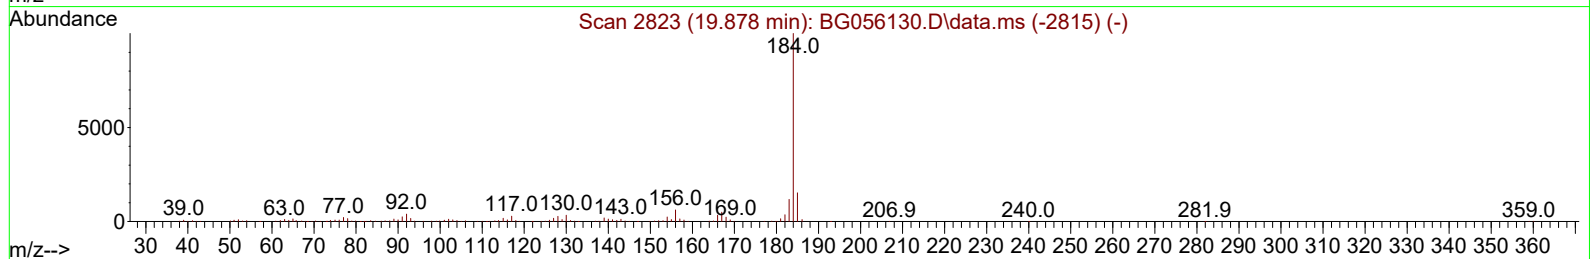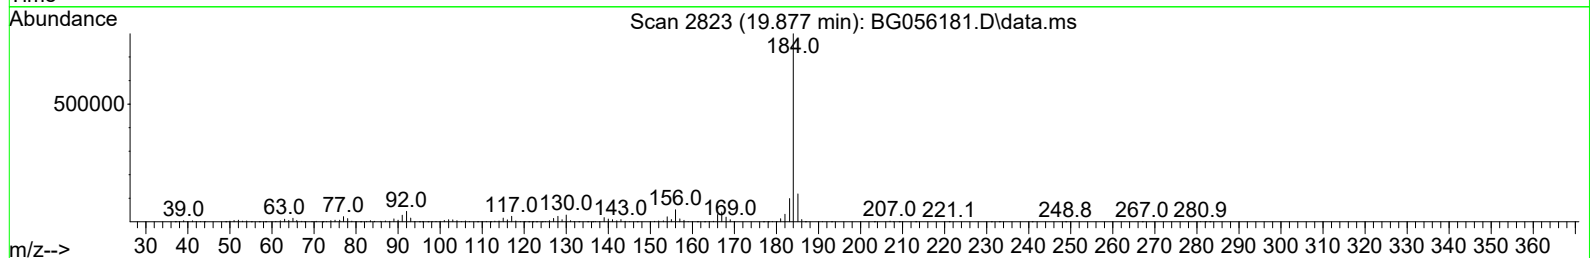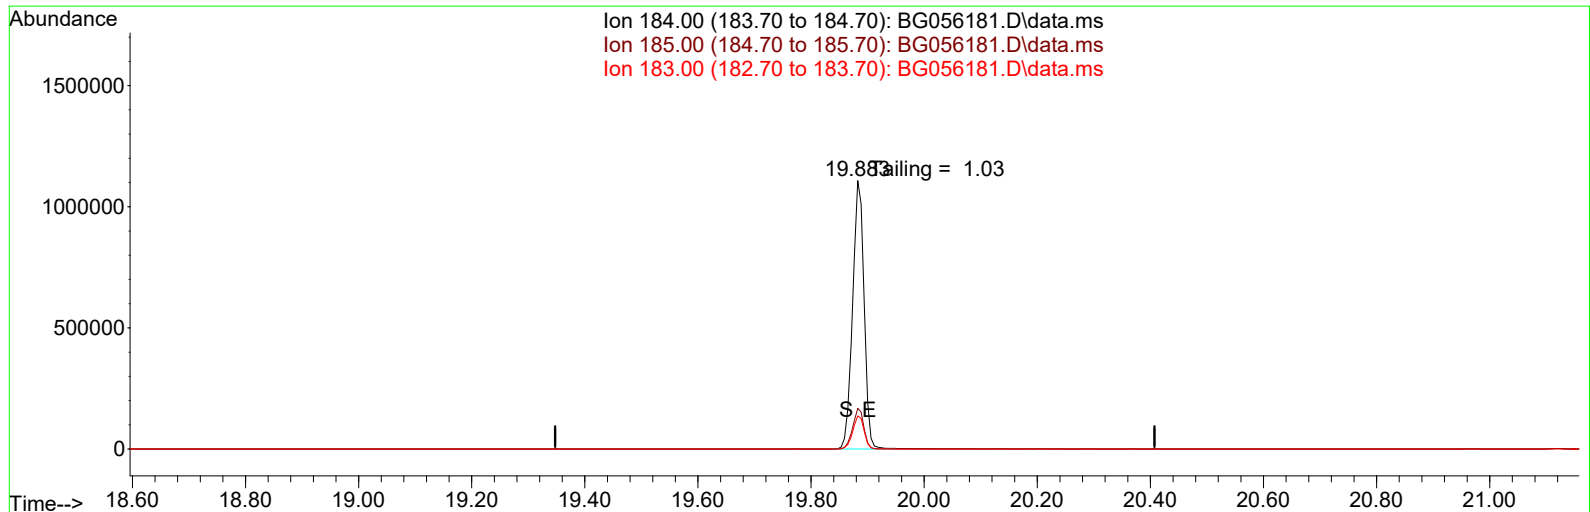

TIC: BG056181.D\data.ms

**(77) Benzidine**

19.878min (-19.878) 0.00 ng

response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 184.00 | 100.00 | 0.00  |
| 185.00 | 15.20  | 0.00# |
| 183.00 | 11.70  | 0.00# |
| 0.00   | 0.00   | 0.00  |