
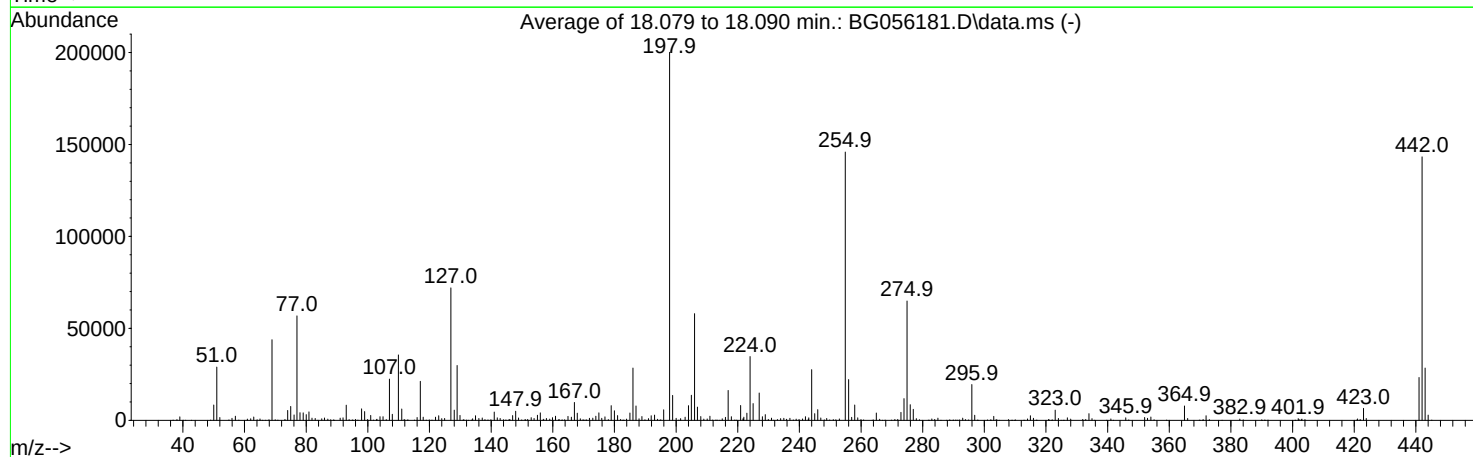


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010323\
Data File : BG056181.D
Acq On : 3 Jan 2023 11:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 04 02:08:15 2023

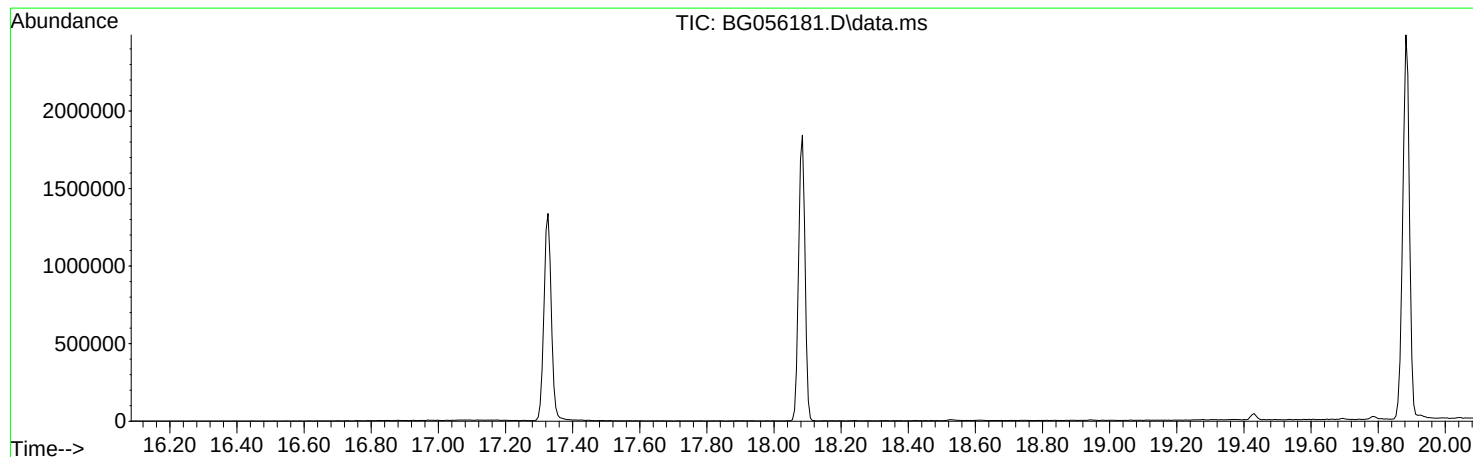


AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.5	28976	PASS
68	69	0.00	2	0.8	340	PASS
69	198	0.00	100	21.9	43829	PASS
70	69	0.00	2	0.7	299	PASS
127	198	10	80	36.0	72035	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	200064	PASS
199	198	5	9	6.8	13568	PASS
275	198	10	60	32.4	64917	PASS
365	198	1	100	3.9	7783	PASS
441	198	0.01	100	11.6	23296	PASS
442	442	50	100	100.0	143285	PASS
443	442	15	24	19.8	28429	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010323\
 Data File : BG056181.D
 Acq On : 3 Jan 2023 11:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 03 16:25:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 05:20:14 2022
 Response via : Initial Calibration

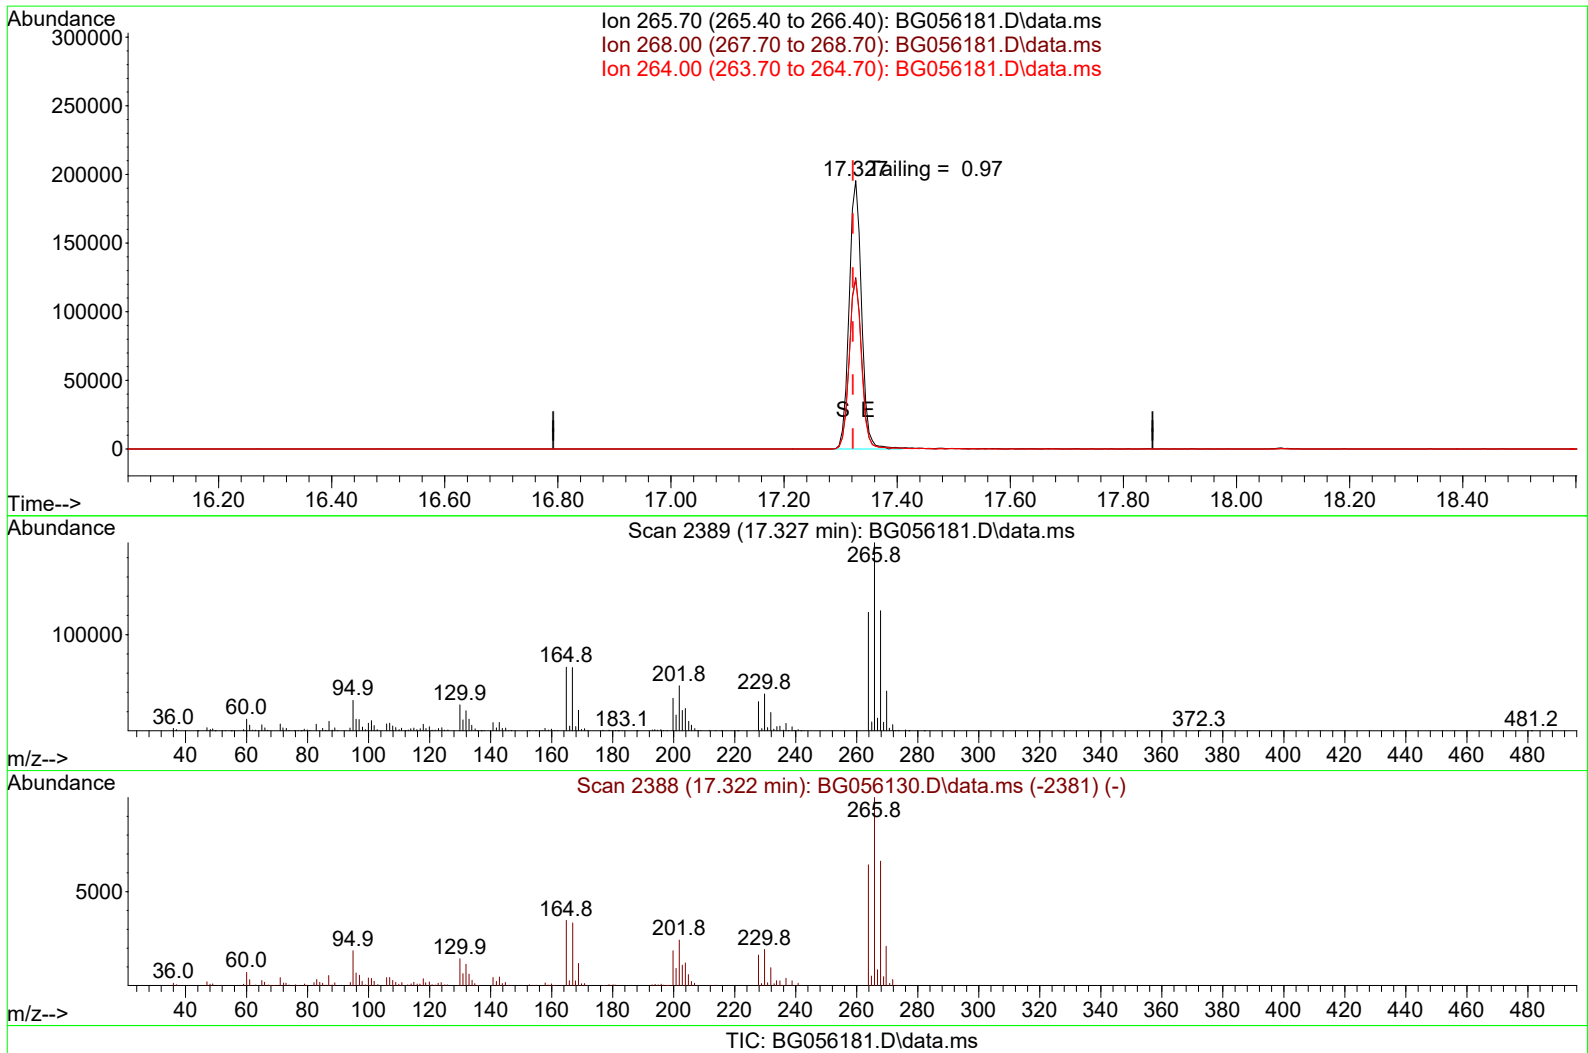

(70) Pentachlorophenol (C)

17.327min (+ 0.005) 251320.48 ng




response 298170

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	63.86
264.00	64.30	63.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010323\
 Data File : BG056181.D
 Acq On : 3 Jan 2023 11:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 03 16:25:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 28 05:20:14 2022
 Response via : Initial Calibration

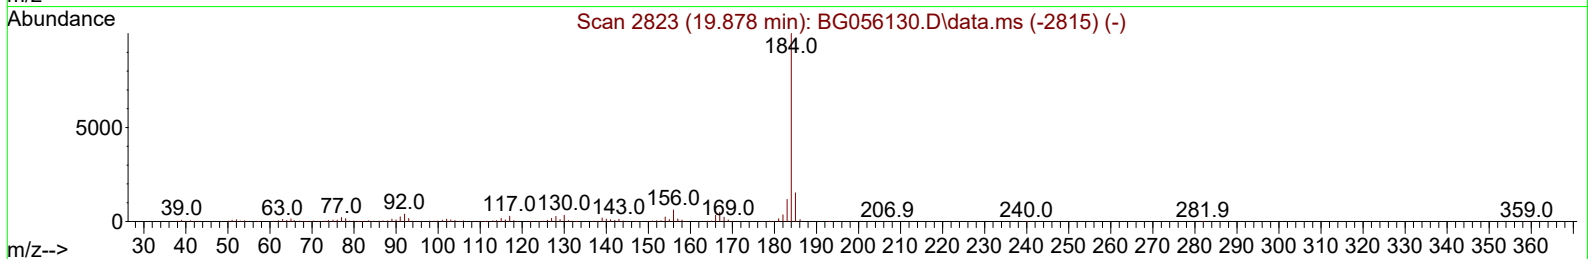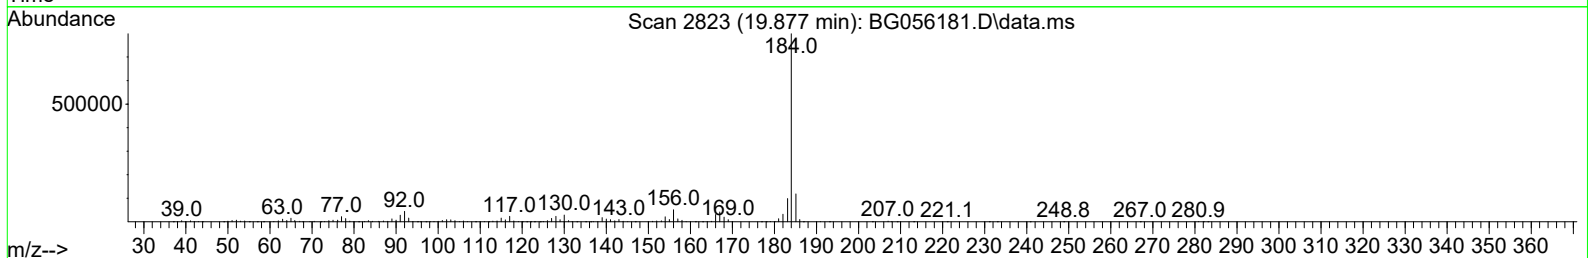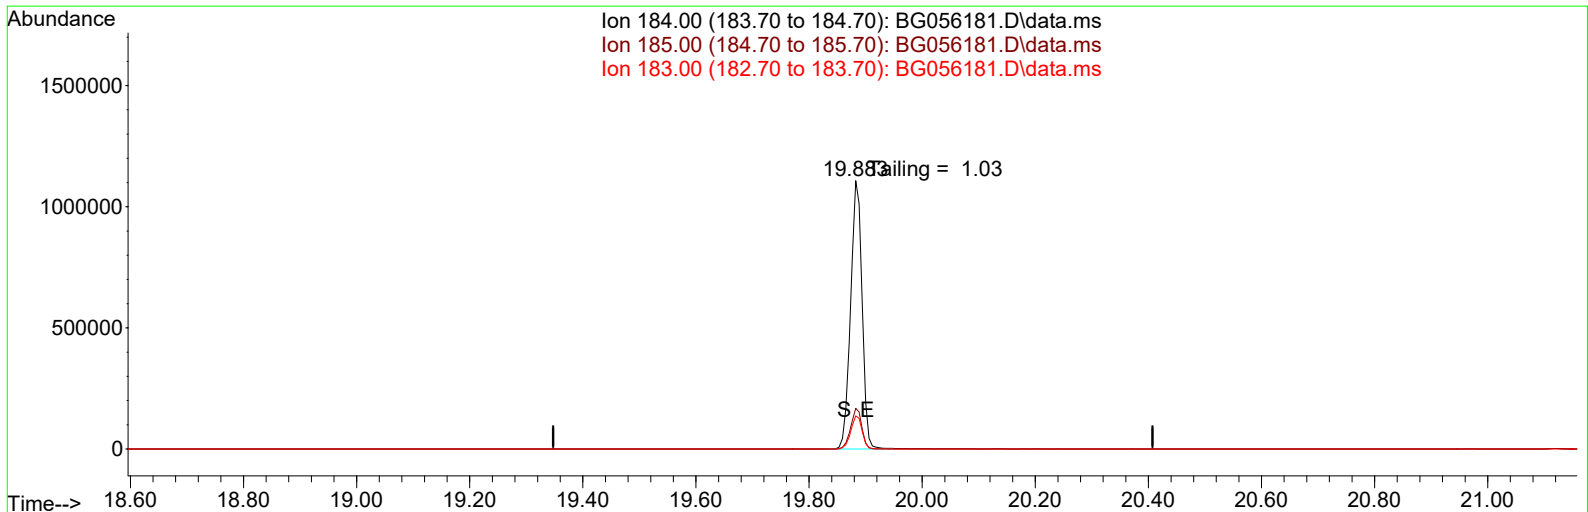

TIC: BG056181.D\data.ms

(77) Benzidine

19.878min (-19.878) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.20	0.00#
183.00	11.70	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/3/2022	BNA_G	BG056181.D
Compound Name	Response	Retention Time
DDT	729208	21.122
DDD	15217	20.717
DDE	53	19.994
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15270	744478	2.05

Instrument :
BNA_G
ClientSampleId :
DFTPP