
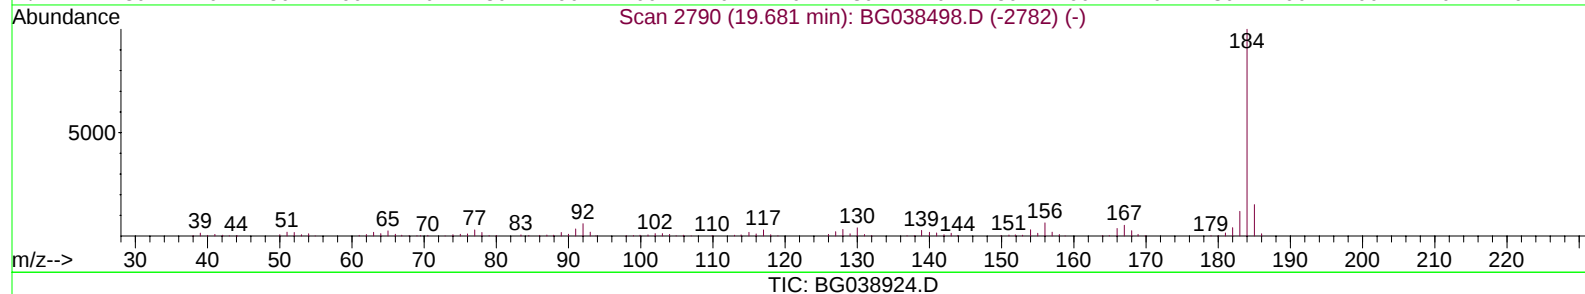
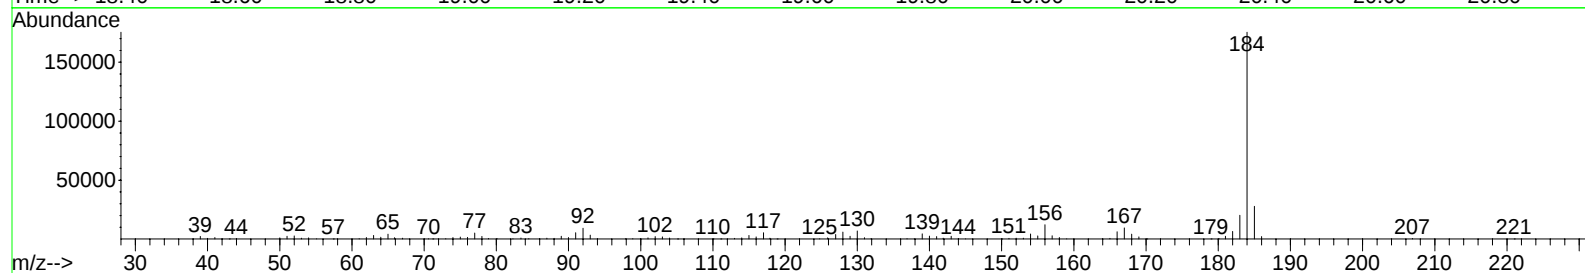


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010419\
Data File : BG038924.D
Acq On : 4 Jan 2019 9:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 16:04:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

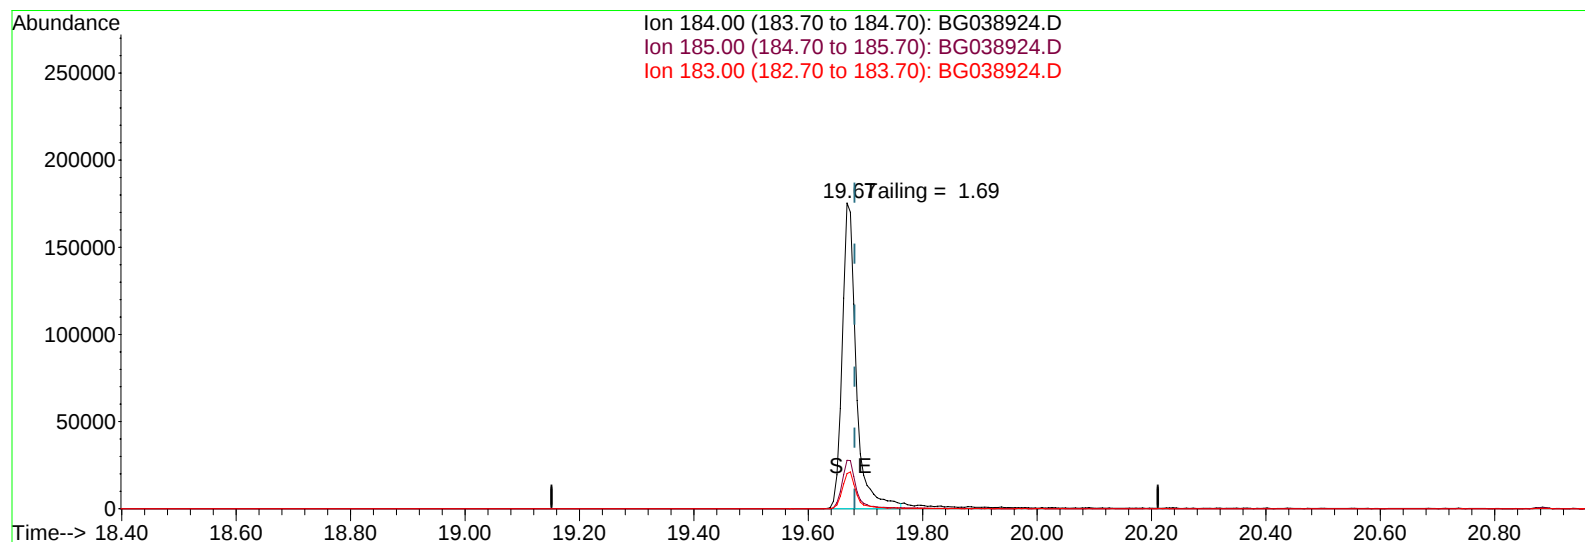

(77) Benzidine




19.668min (-0.014) 51658.34ng

response 302494

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.87
183.00	12.00	11.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010419\
Data File : BG038924.D
Acq On : 4 Jan 2019 9:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 16:04:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

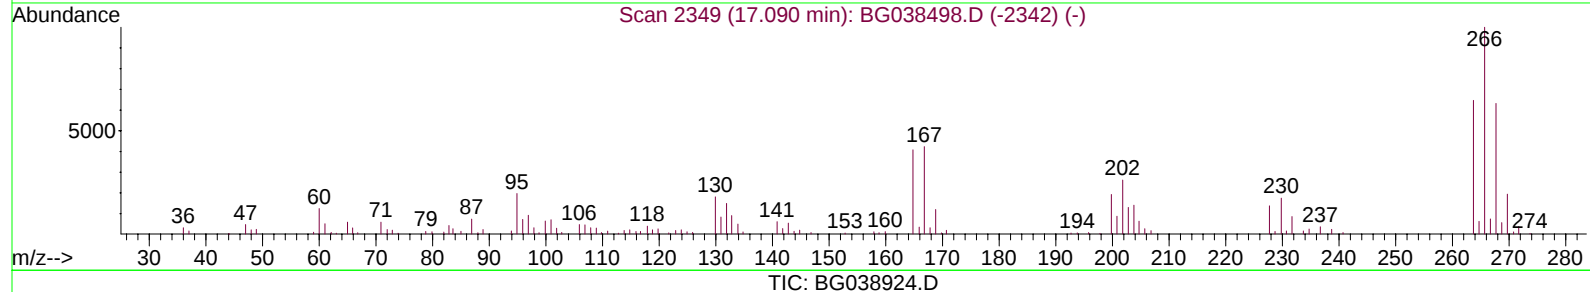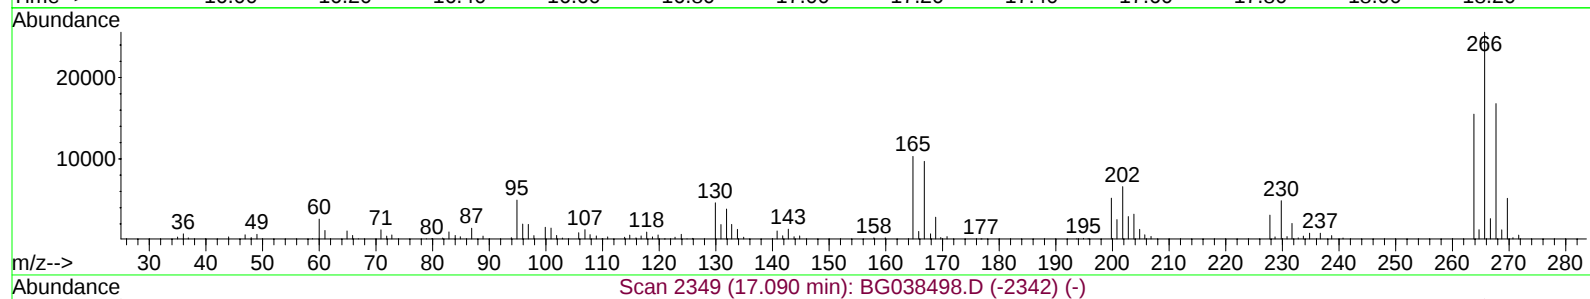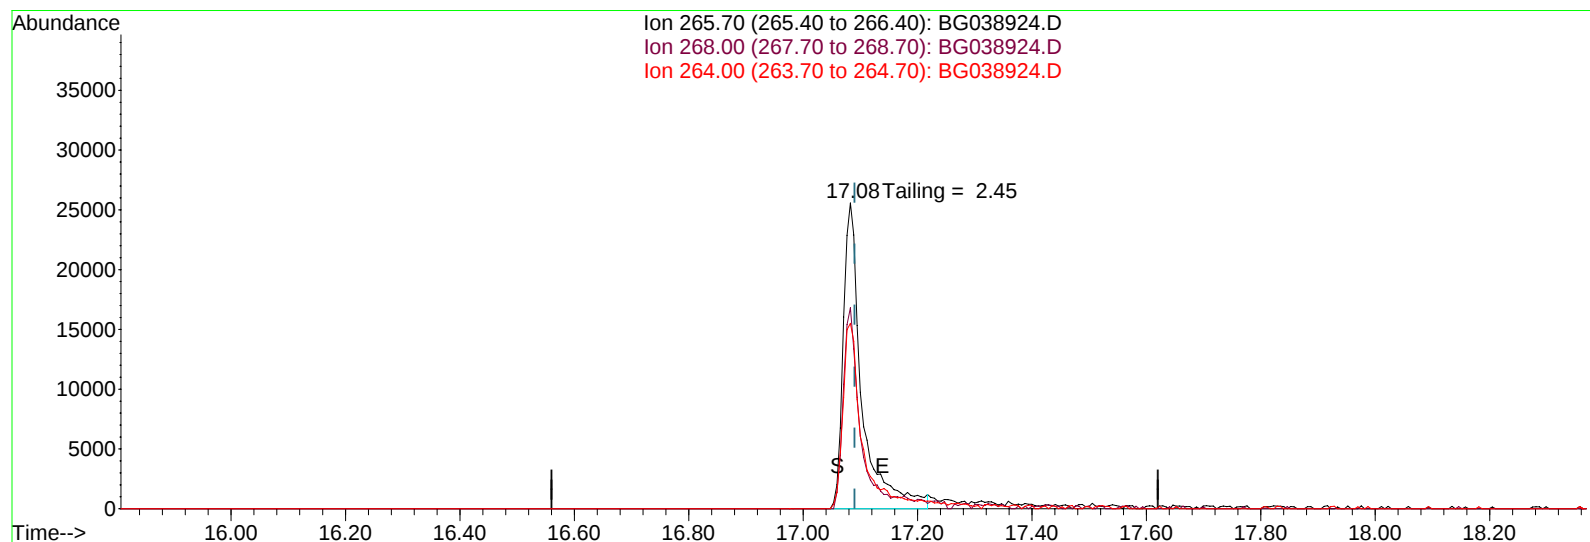

(70) Pentachlorophenol (C)

17.082min (-0.008) 63429.59ng

response 58422

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	70.72
264.00	70.90	65.75
0.00	0.00	0.00