
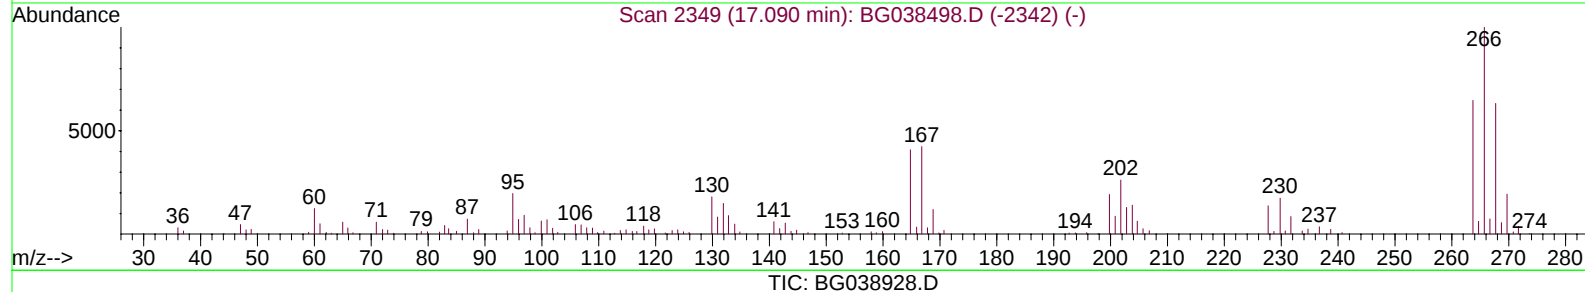
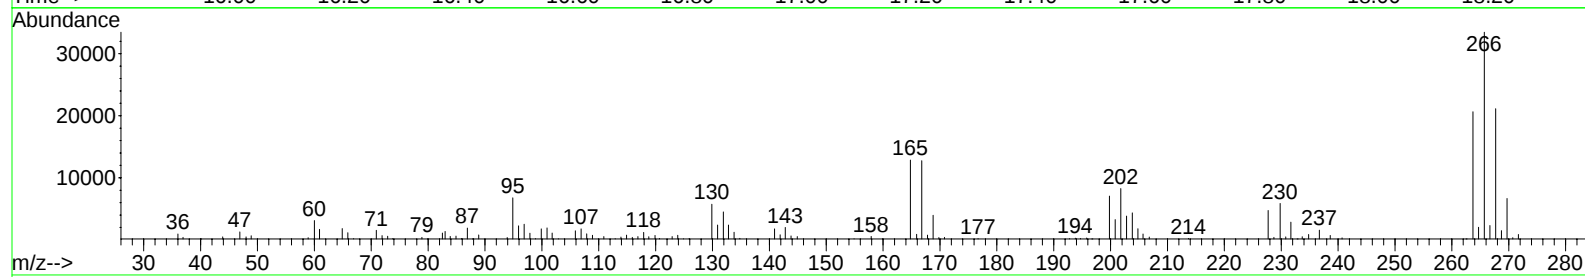


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010419\
Data File : BG038928.D
Acq On : 4 Jan 2019 13:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 15:56:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

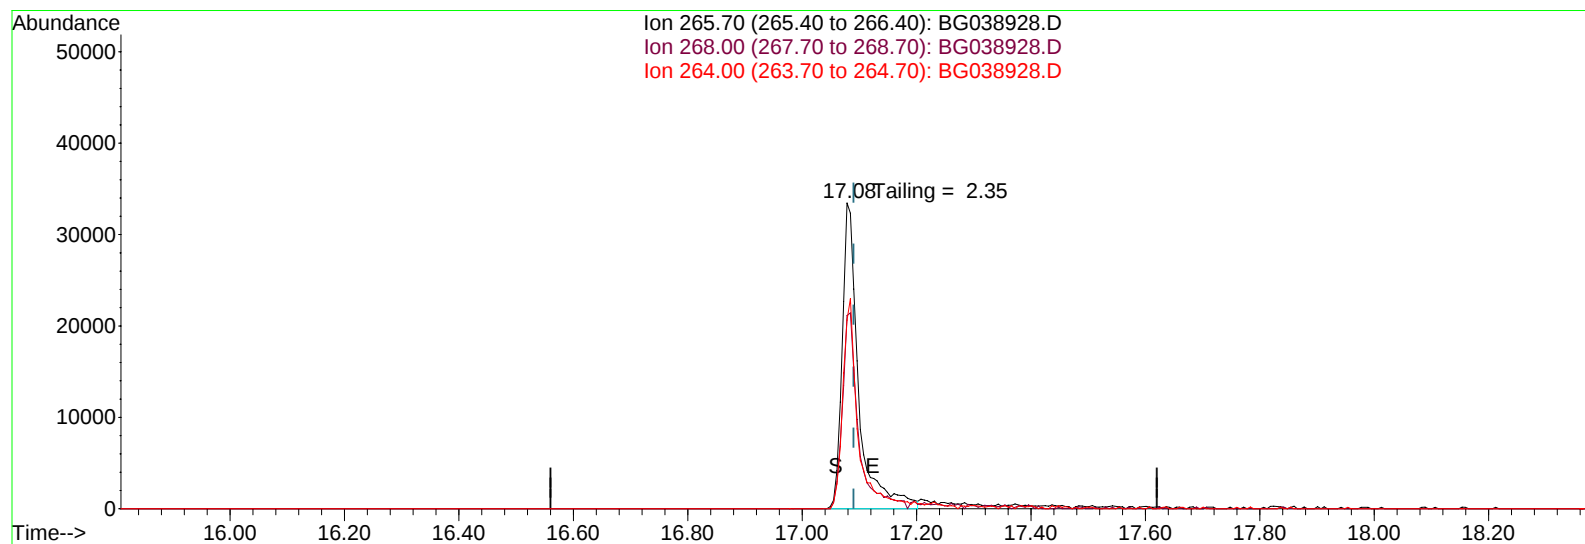

(70) Pentachlorophenol (C)




17.078min (-0.012) 22501.44ng

response 64197

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.68
264.00	70.90	67.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010419\
Data File : BG038928.D
Acq On : 4 Jan 2019 13:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 15:56:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

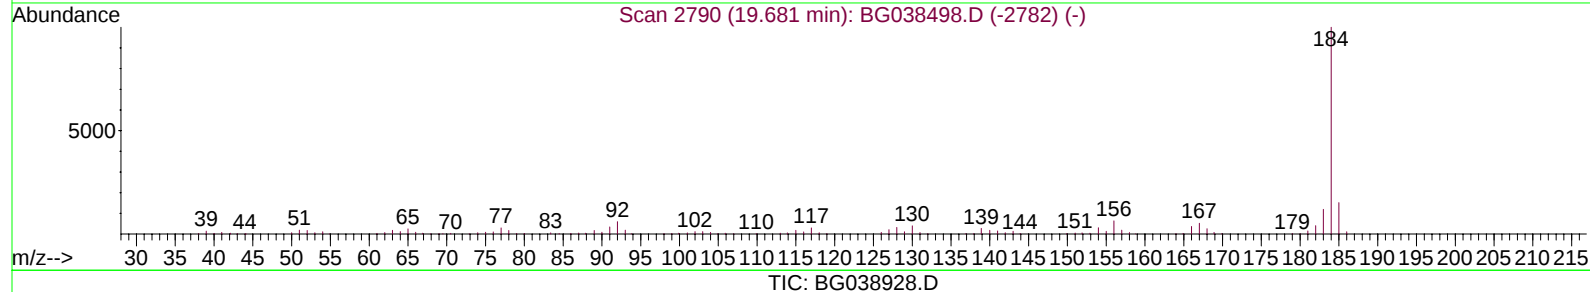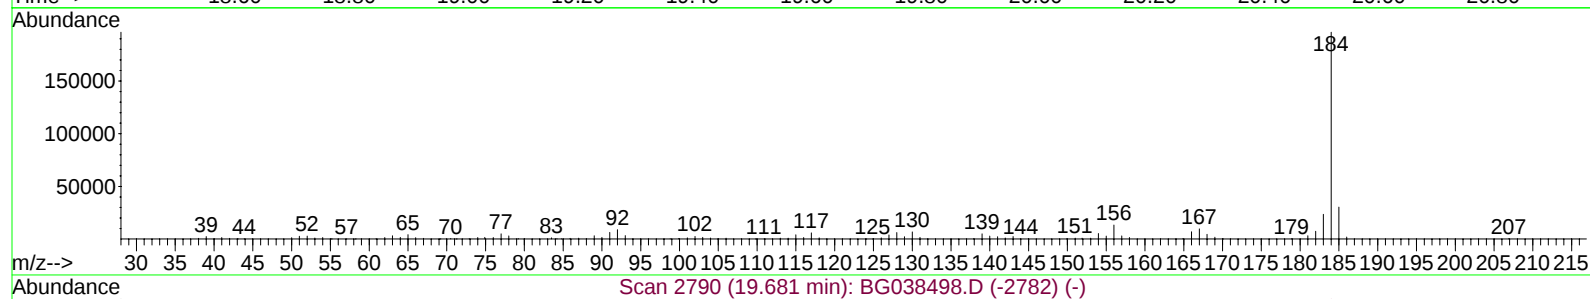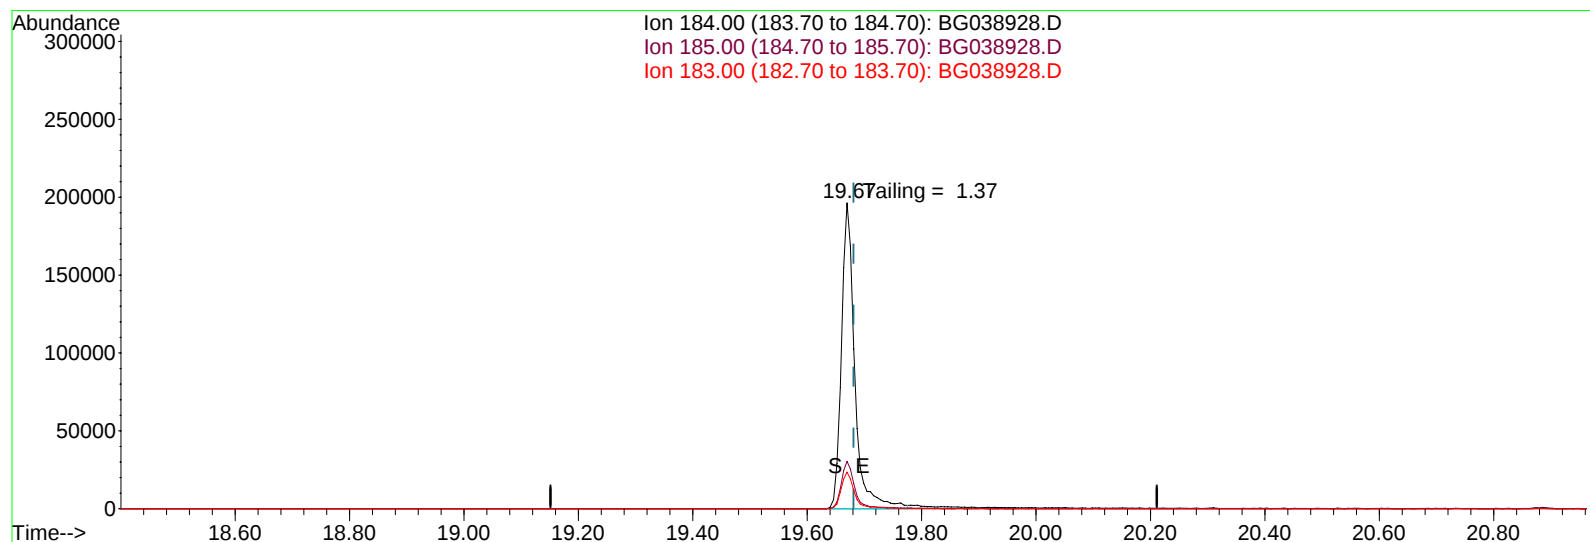

(77) Benzidine

19.669min (-0.012) 68830.65ng

response 317554

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.50
183.00	12.00	11.99
0.00	0.00	0.00