

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010419\
 Data File : BG038947.D
 Acq On : 5 Jan 2019 3:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1


Instrument :
 BNA_G
 ClientSampleID :
 SSTDCCC040

Manual Integrations
 APPROVED

Sohil
 1/7/2019 12:48:00 PM

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

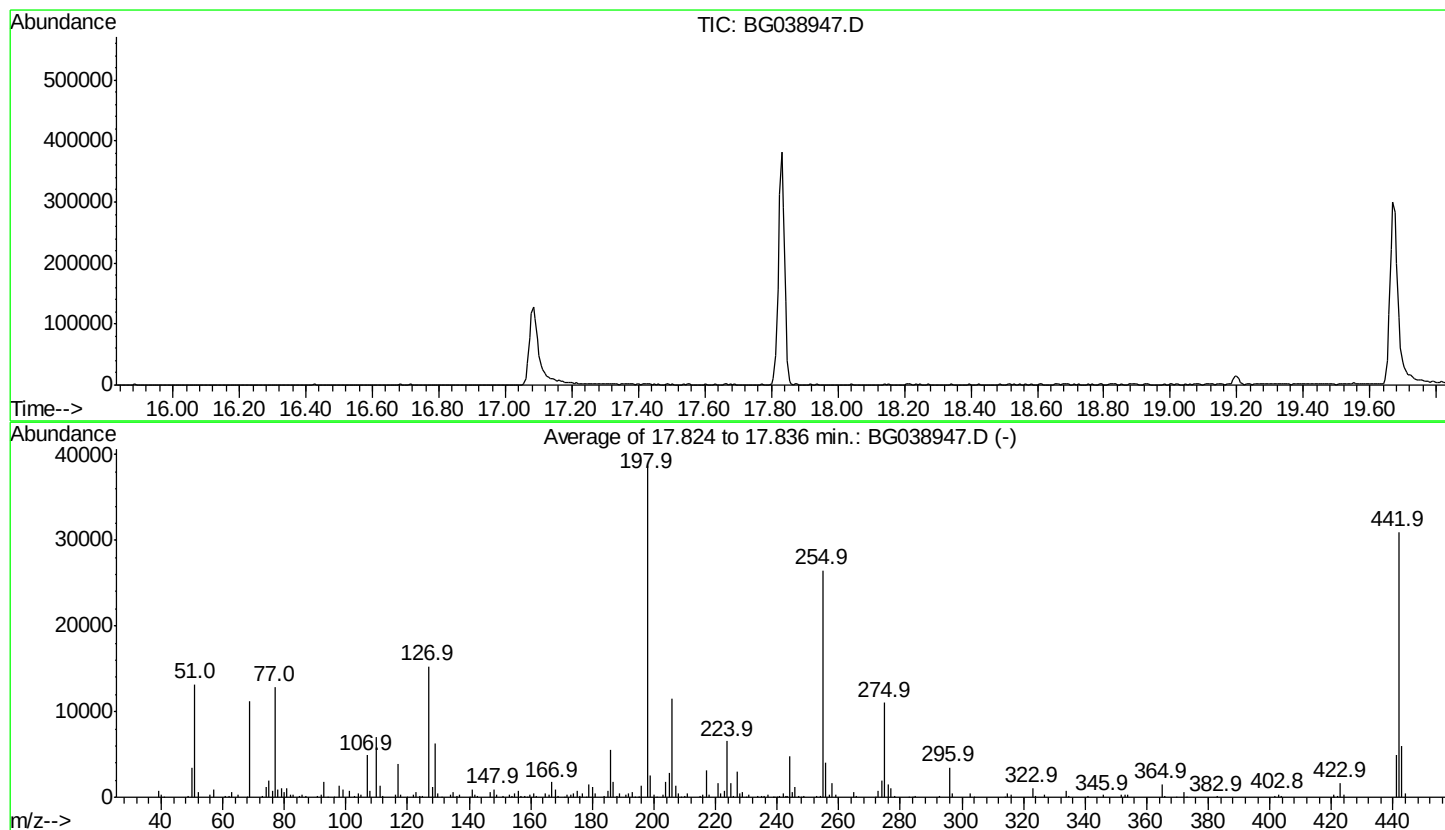

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	13185	PASS
68	69	0.00	2	0.5	55	PASS
69	198	0.00	100	28.9	11201	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.4	15252	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38725	PASS
199	198	5	9	6.6	2575	PASS
275	198	10	60	28.5	11030	PASS
365	198	1	100	3.9	1524	PASS
441	198	0.01	100	12.9	4996	PASS
442	198	50	100	80.0	30978	PASS
443	442	15	24	19.3	5968	PASS