

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010419\
 Data File : BG038957.D
 Acq On : 5 Jan 2019 10:12
 Operator : JU/SJ
 Sample : K1036-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 13-L

Quant Time: Jan 06 23:09:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	26619	20.00	ng	-0.01
21) Naphthalene-d8	10.87	136	107933	20.00	ng	-0.01
39) Acenaphthene-d10	14.69	164	73170	20.00	ng	-0.01
64) Phenanthrene-d10	17.43	188	160003	20.00	ng	0.00
76) Chrysene-d12	21.72	240	153683	20.00	ng	0.00
87) Perylene-d12	25.01	264	166218	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	127747	85.12	ng	0.00
7) Phenol-d6	7.21	99	181871	88.27	ng	0.00
23) Nitrobenzene-d5	9.23	82	117362	55.55	ng	-0.01
42) 2,4,6-Tribromophenol	16.18	330	97947	97.13	ng	-0.01
45) 2-Fluorobiphenyl	13.30	172	334541	62.72	ng	-0.01
79) Terphenyl-d14	20.04	244	502251	71.12	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010419\
Data File : BG038957.D
Acq On : 5 Jan 2019 10:12
Operator : JU/SJ
Sample : K1036-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
13-L

Quant Time: Jan 06 23:09:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

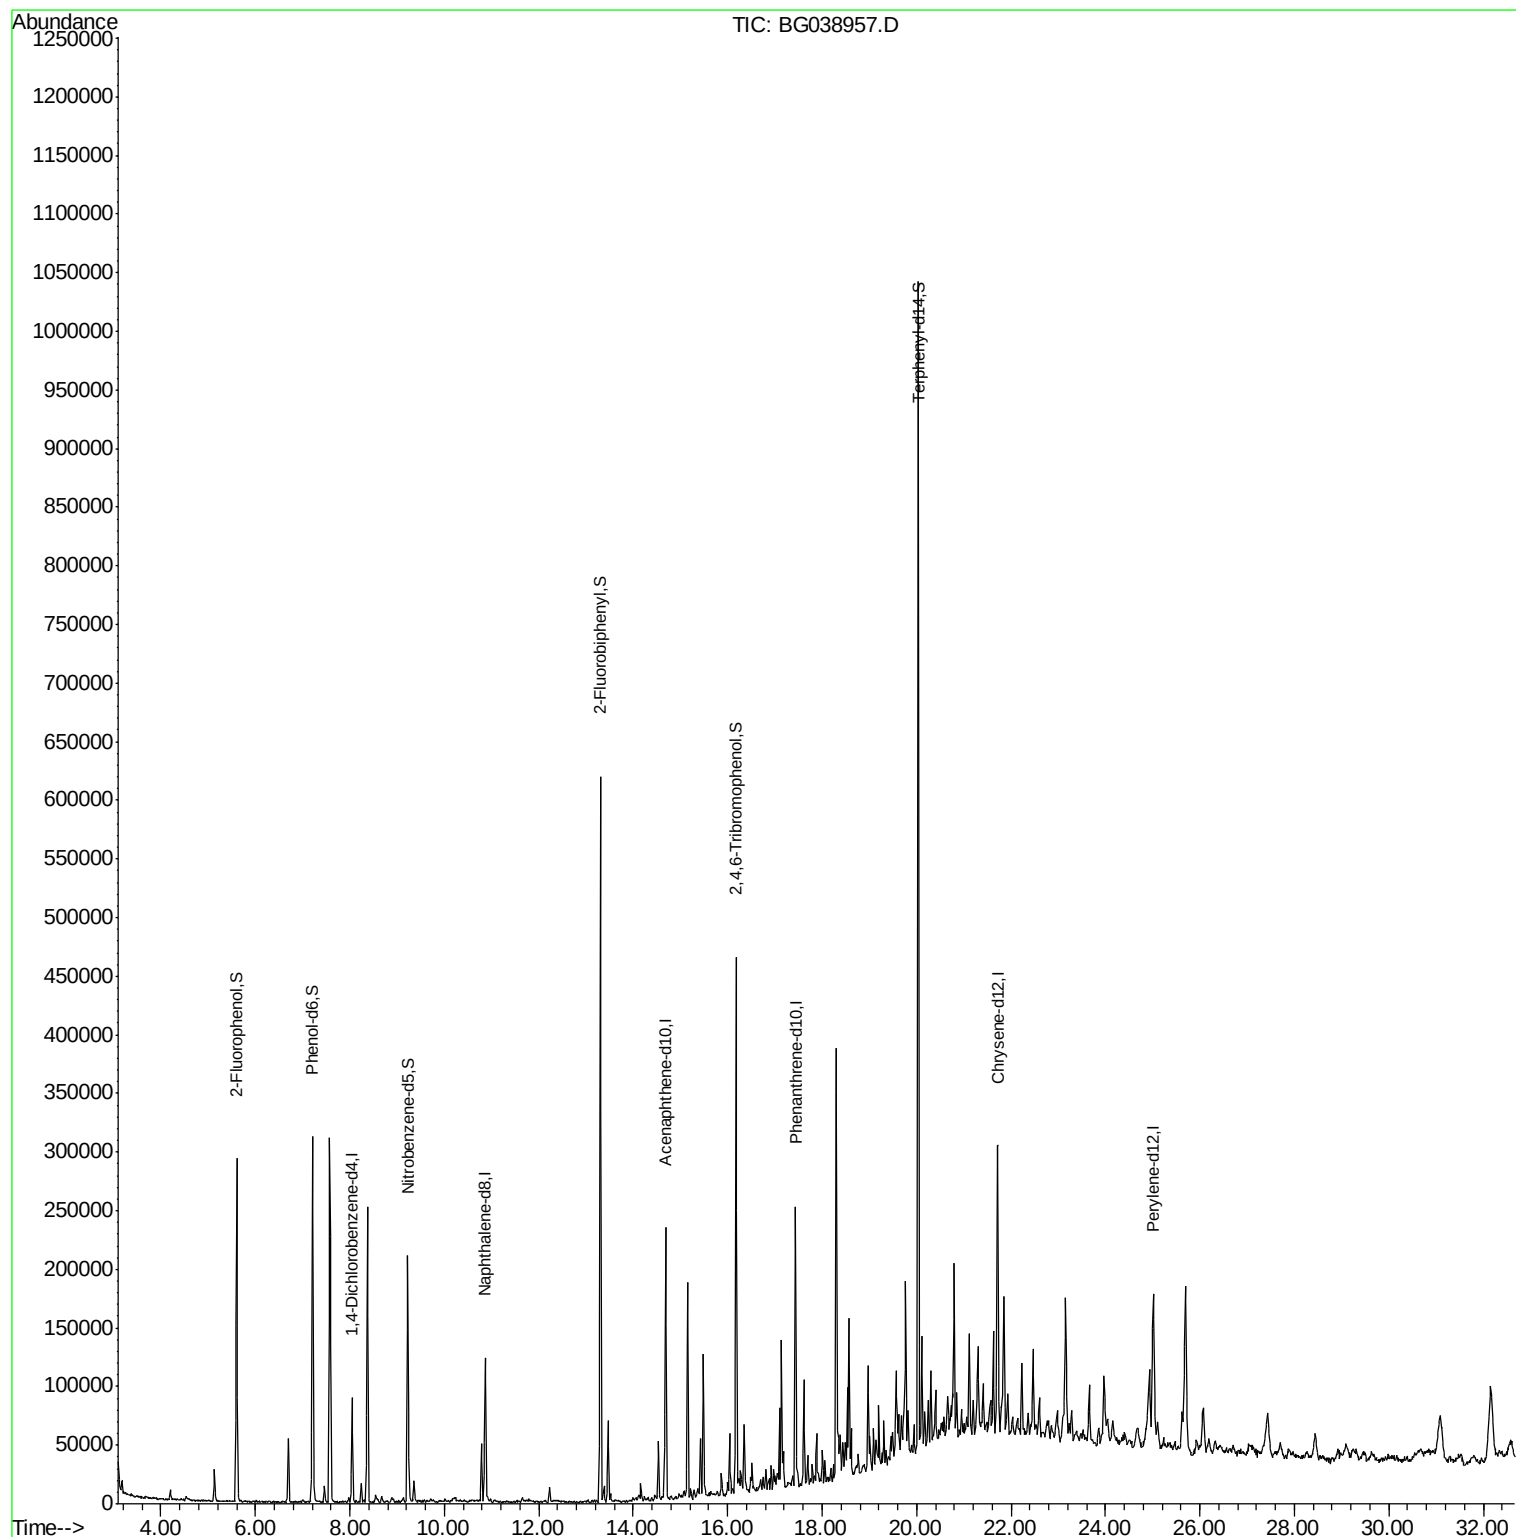

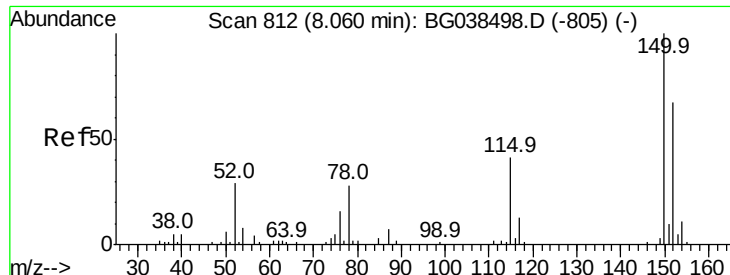


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.01 min
Lab File: BG038957.D
Acq: 5 Jan 2019 10:12

Instrument :
BNA_G
ClientSampleId :
13-L

Tot Ion:152 Resp: 26619
Ion Ratio Lower Upper
152 100
150 157.2 119.5 179.3
115 59.3 49.6 74.4

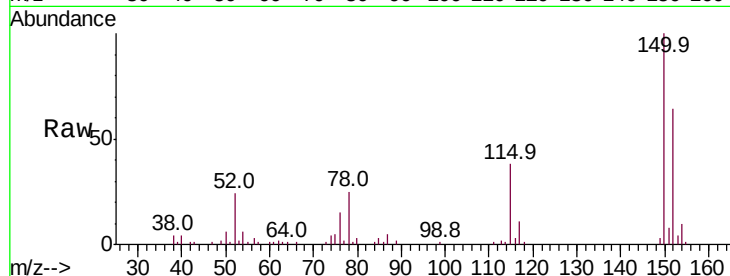


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

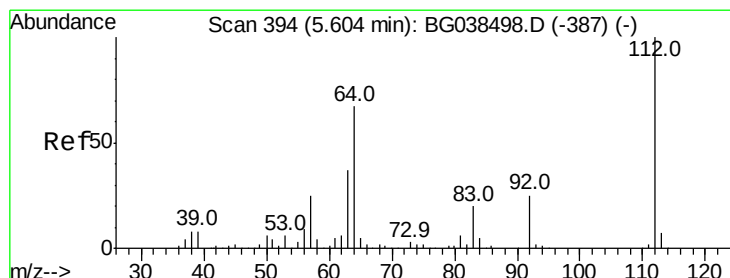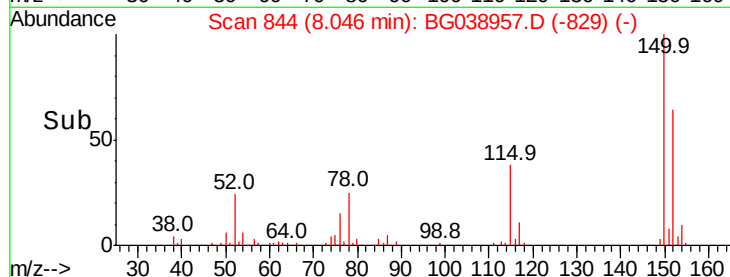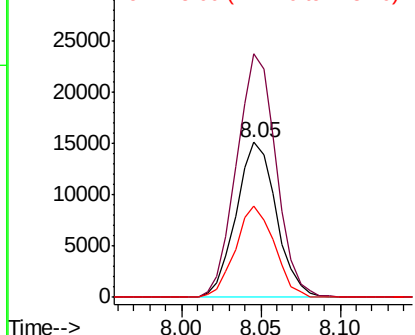



#5


2-Fluorophenol
Concen: 85.119 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.00 min
Lab File: BG038957.D
Acq: 5 Jan 2019 10:12

Tgt Ion:112 Resp: 127747
Ion Ratio Lower Upper
112 100
64 64.4 53.4 80.2
63 36.5 29.3 43.9

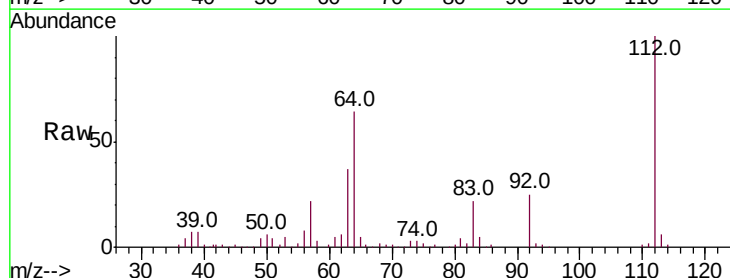

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

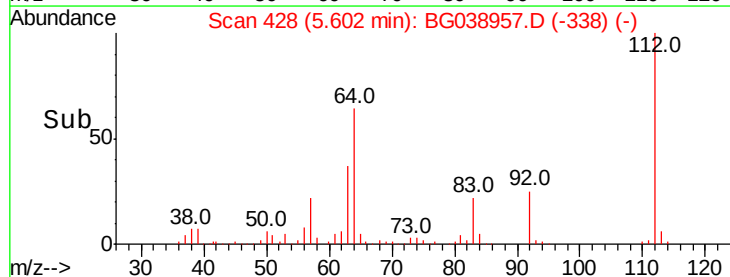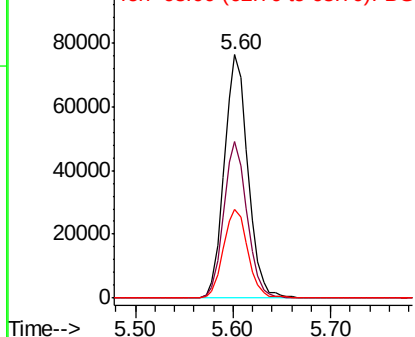

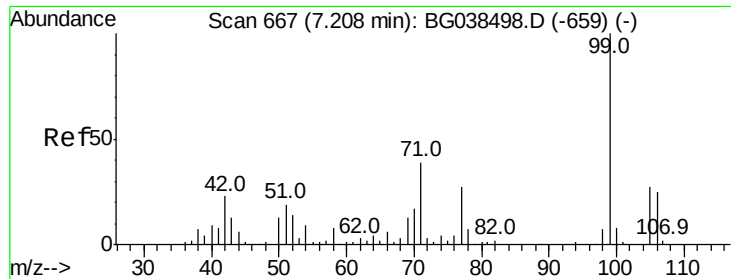

#7

Phenol-d6

Concen: 88.274 ng

RT: 7.21 min Scan# 702

Delta R.T. 0.00 min

Lab File: BG038957.D

Acq: 5 Jan 2019 10:12

Instrument :

BNA_G

ClientSampled :

13-L


Tot Ion: 99 Resp: 181871

Ion Ratio Lower Upper




99 100

42 22.0 18.5 27.7

71 38.3 31.1 46.7

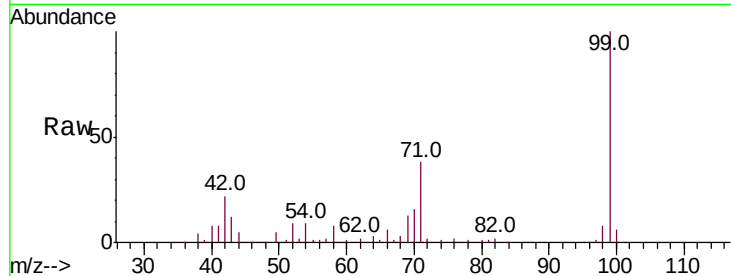

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

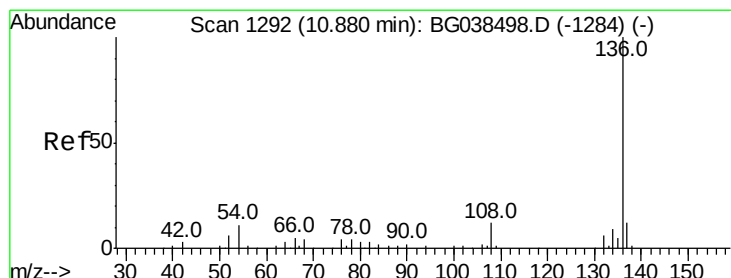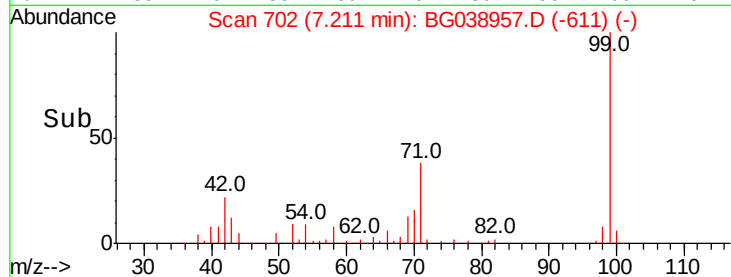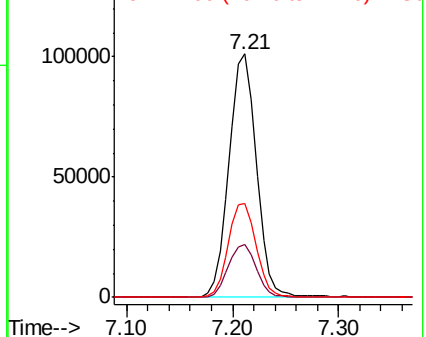

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1324

Delta R.T. -0.01 min

Lab File: BG038957.D

Acq: 5 Jan 2019 10:12

Tgt Ion: 136 Resp: 107933


Ion Ratio Lower Upper

136 100



137 11.1 9.3 13.9


54 9.4 8.5 12.7

68 4.0 3.5 5.3

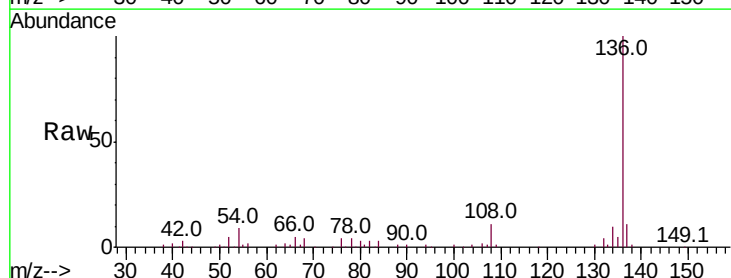

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

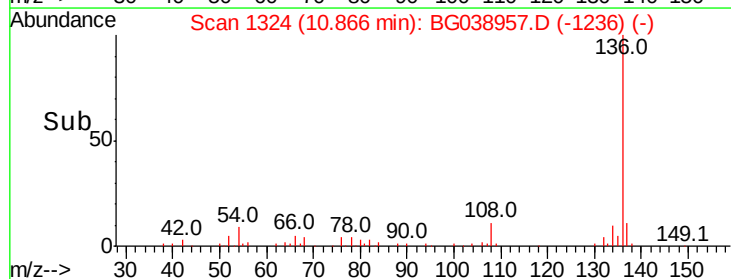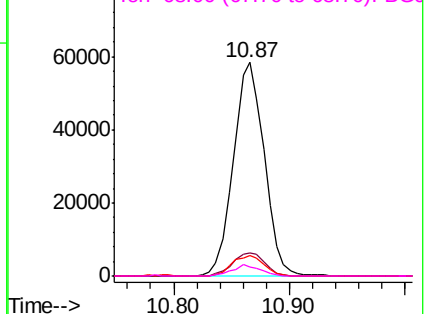


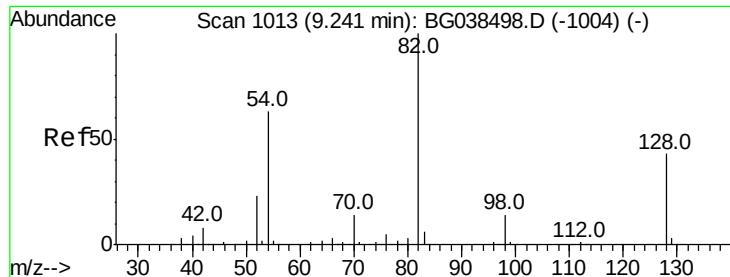




#23
Nitrobenzene-d5
Concen: 55.550 ng
RT: 9.23 min Scan# 1045
Delta R.T. -0.01 min
Lab File: BG038957.D
Acq: 5 Jan 2019 10:12

Instrument :
BNA_G
ClientSampleId :
13-L

Tot Ion: 82 Resp: 117362
Ion Ratio Lower Upper
82 100
128 44.4 34.6 52.0
54 61.7 50.6 76.0

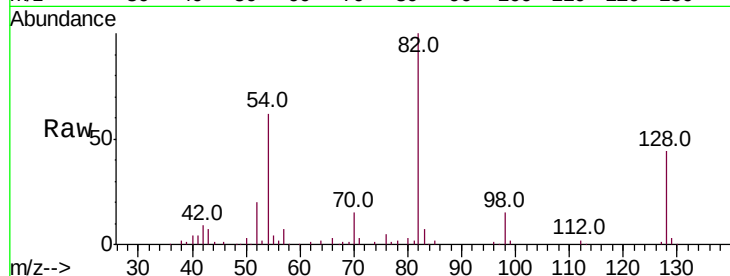


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

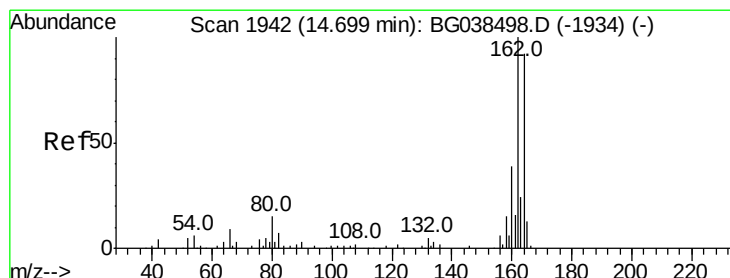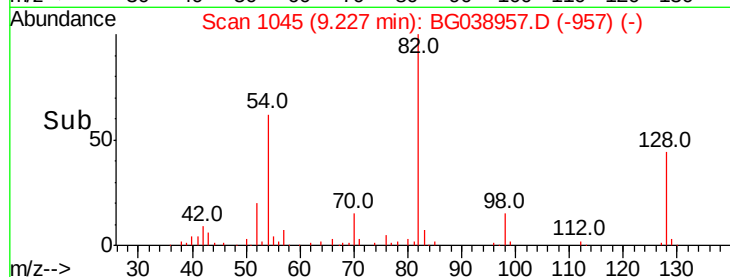
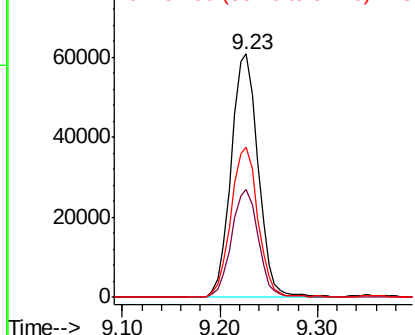



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.69 min Scan# 1974
Delta R.T. -0.01 min
Lab File: BG038957.D
Acq: 5 Jan 2019 10:12

Tgt Ion:164 Resp: 73170
Ion Ratio Lower Upper
164 100
162 103.4 86.6 130.0
160 43.8 34.2 51.2

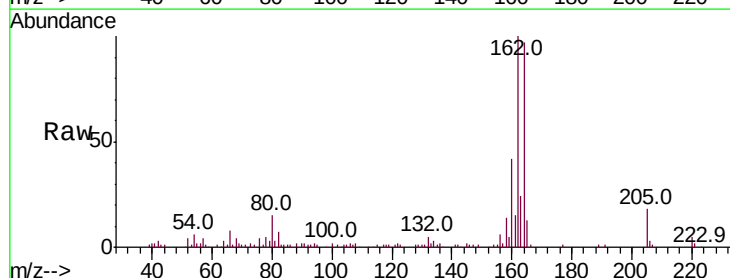

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

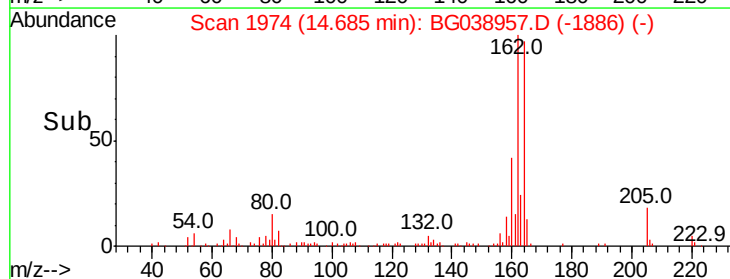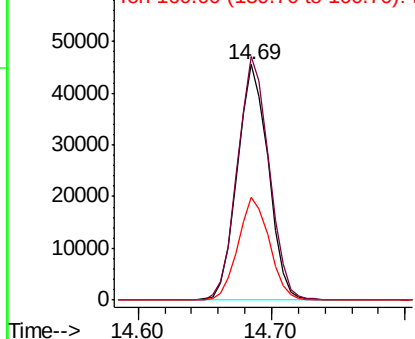

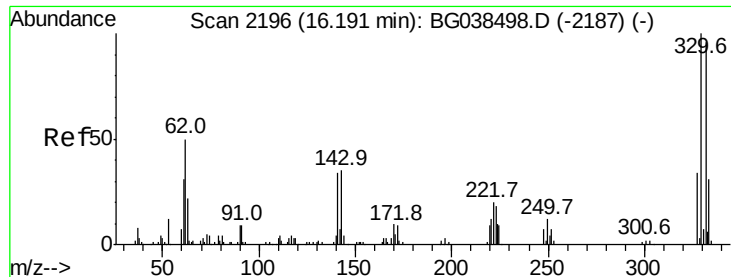

#42

2,4,6-Tribromophenol

Concen: 97.130 ng

RT: 16.18 min Scan# 2228

Delta R.T. -0.01 min

Lab File: BG038957.D

Acq: 5 Jan 2019 10:12

Instrument :

BNA_G

ClientSampleId :

13-L


Tot Ion:330 Resp: 97947

Ion Ratio Lower Upper




330 100

332 93.5 76.9 115.3

141 32.2 28.8 43.2

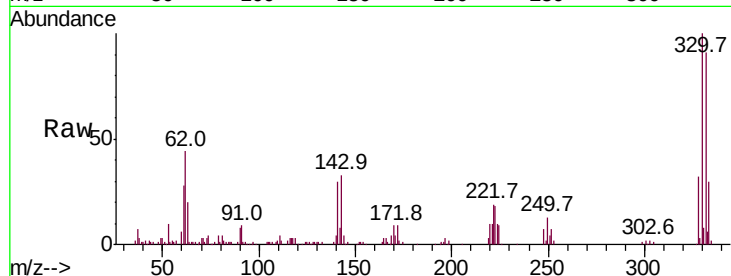

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

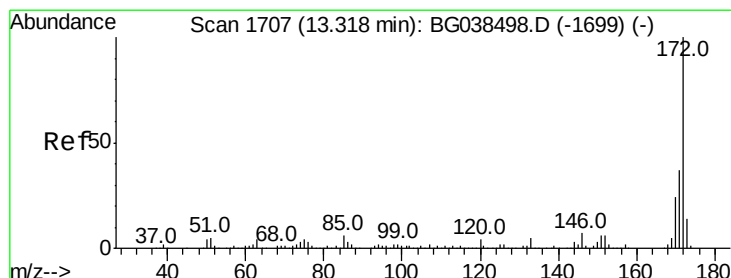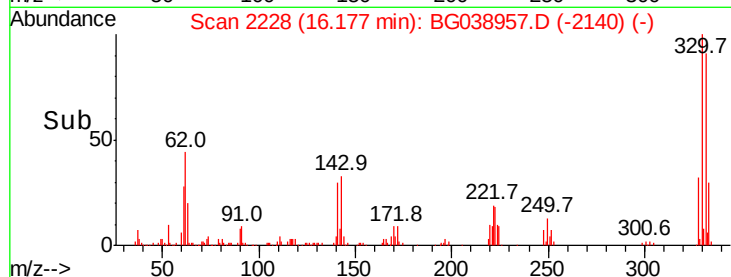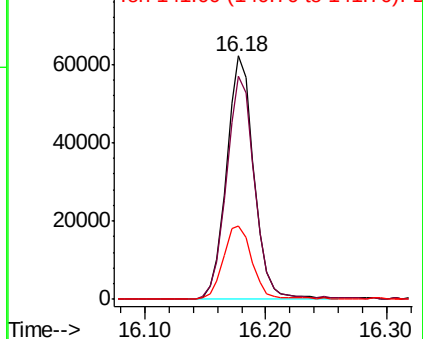

#45

2-Fluorobiphenyl

Concen: 62.722 ng

RT: 13.30 min Scan# 1739

Delta R.T. -0.01 min

Lab File: BG038957.D

Acq: 5 Jan 2019 10:12


Tgt Ion:172 Resp: 334541

Ion Ratio Lower Upper



172 100


171 36.5 29.8 44.6

170 24.1 19.5 29.3

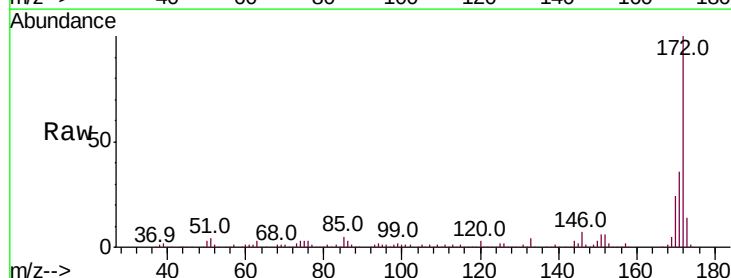

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

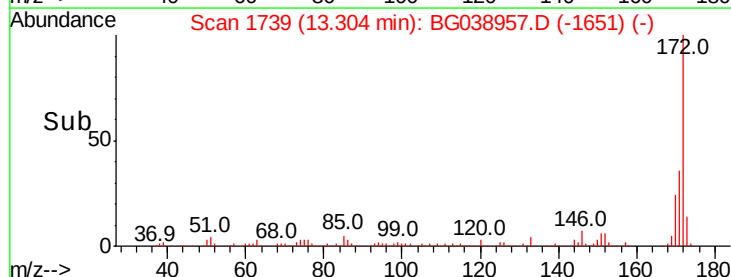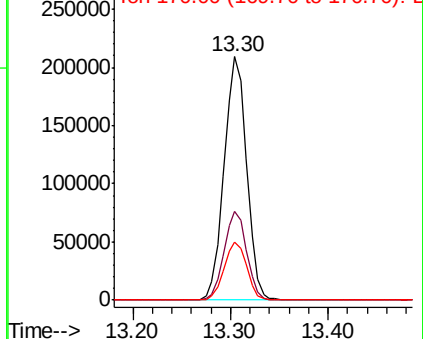


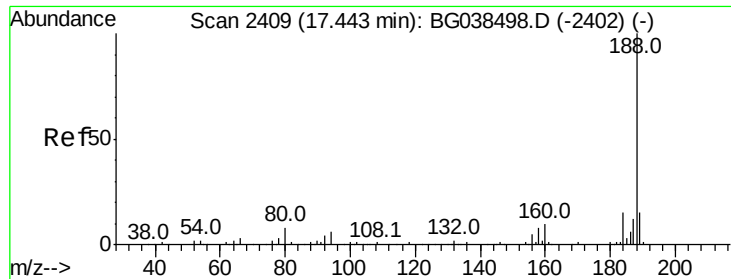




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2442
Delta R.T. -0.01 min
Lab File: BG038957.D
Acq: 5 Jan 2019 10:12

Instrument :
BNA_G
ClientSampled :
13-L

Tot Ion:188 Resp: 160003
Ion Ratio Lower Upper
188 100
94 5.3 5.1 7.7
80 6.2 6.1 9.1

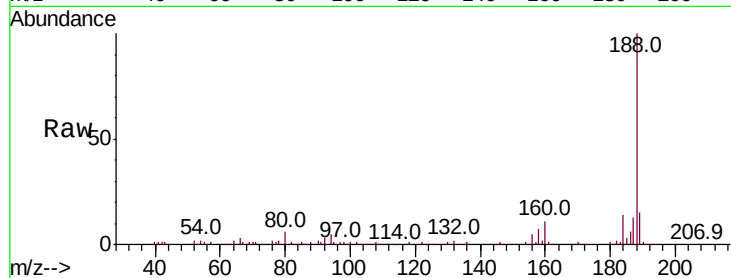


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

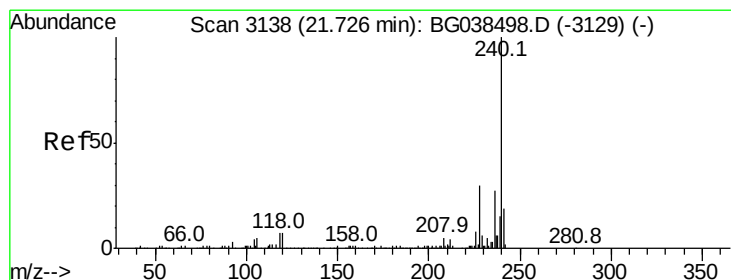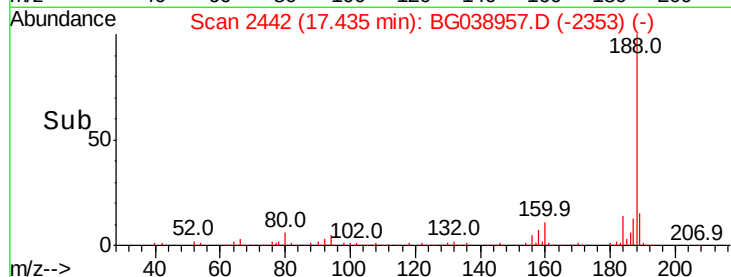
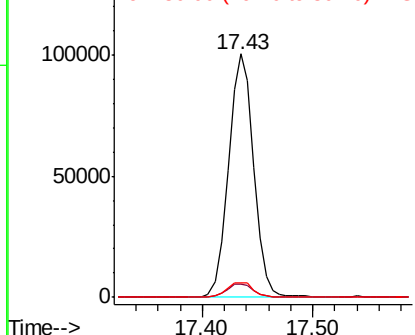



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.72 min Scan# 3171
Delta R.T. -0.01 min
Lab File: BG038957.D
Acq: 5 Jan 2019 10:12

Tgt Ion:240 Resp: 153683
Ion Ratio Lower Upper
240 100
120 5.6 5.3 7.9
236 25.5 21.4 32.2

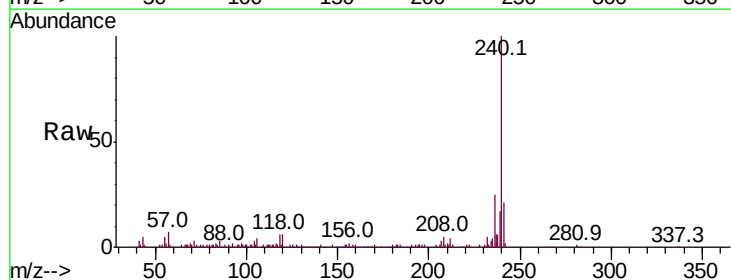

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

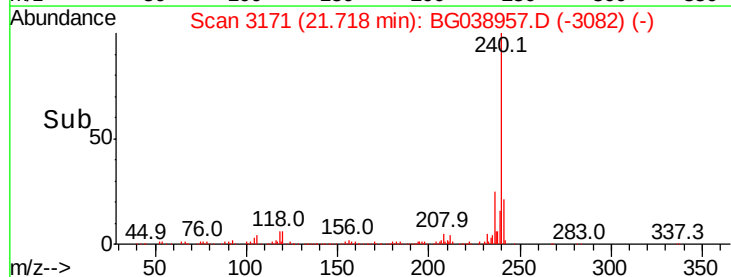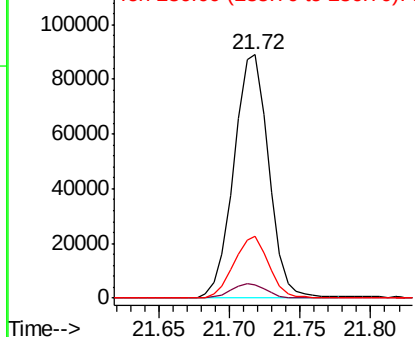

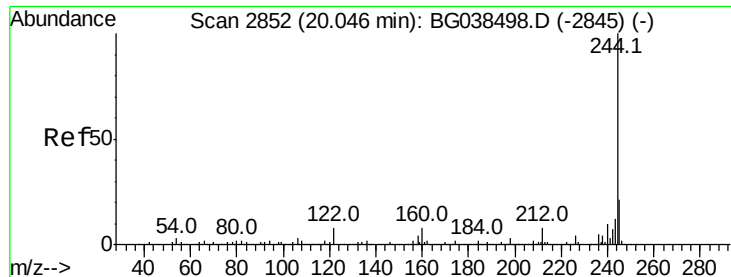

#79

Terphenyl-d14

Concen: 71.125 ng

RT: 20.04 min Scan# 2885

Delta R.T. -0.01 min

Lab File: BG038957.D

Acq: 5 Jan 2019 10:12

Instrument :

BNA_G

ClientSampleId :

13-L


Tot Ion:244 Resp: 502251

Ion Ratio Lower Upper

244 100

212 7.4 6.2 9.2




122 6.2 6.3 9.5#

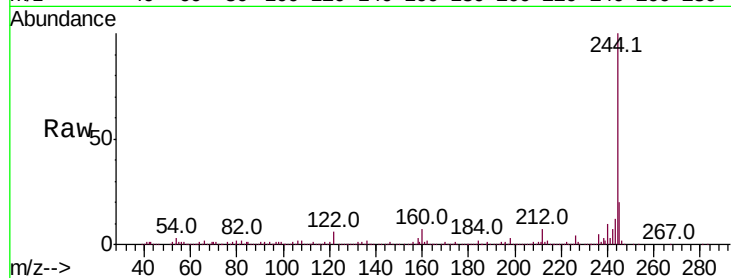

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

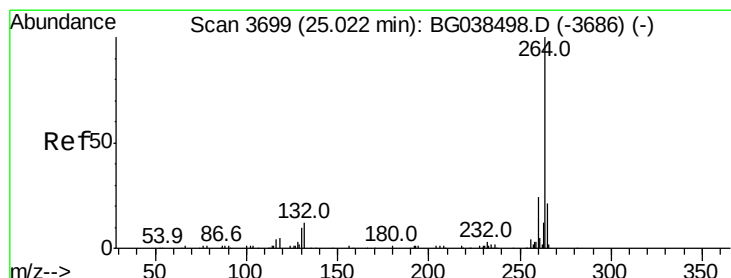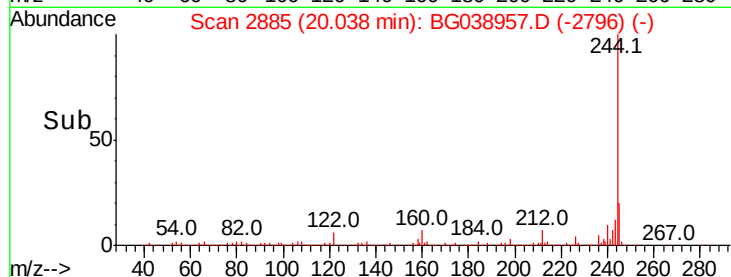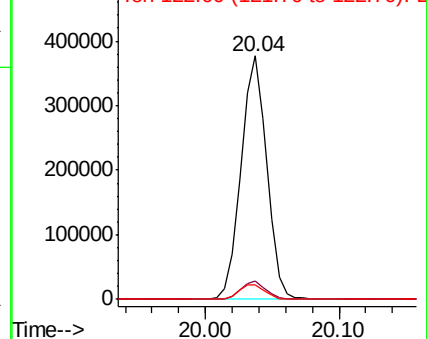

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.01 min Scan# 3732

Delta R.T. -0.01 min

Lab File: BG038957.D

Acq: 5 Jan 2019 10:12


Tgt Ion:264 Resp: 166218

Ion Ratio Lower Upper

264 100

260 22.5 18.9 28.3

265 20.7 17.0 25.4

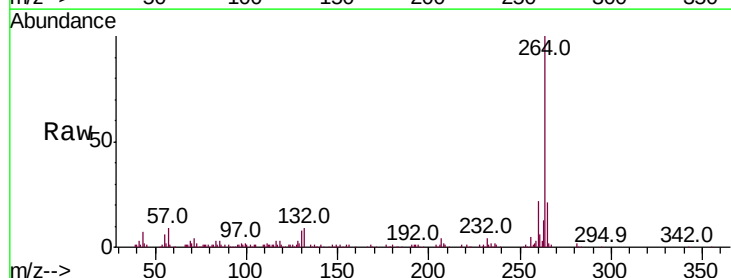

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

