


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010419\
 Data File : BG038924.D
 Acq On : 4 Jan 2019 9:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

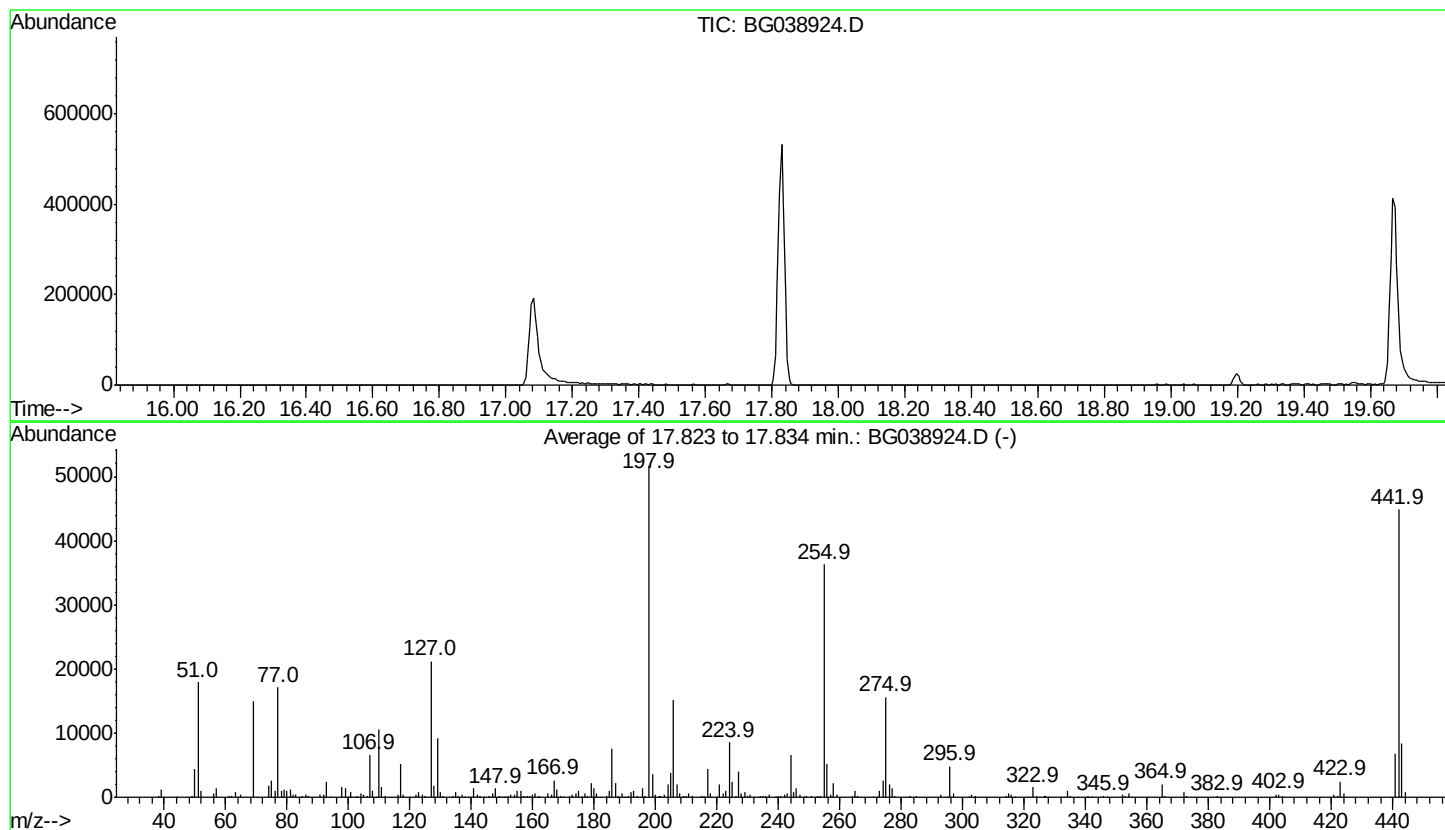

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	17922	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.0	14990	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	21216	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51704	PASS
199	198	5	9	6.8	3512	PASS
275	198	10	60	30.2	15626	PASS
365	198	1	100	4.0	2088	PASS
441	198	0.01	100	13.3	6876	PASS
442	198	50	100	86.8	44880	PASS
443	442	15	24	18.8	8445	PASS