


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010419\
 Data File : BG038928.D
 Acq On : 4 Jan 2019 13:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

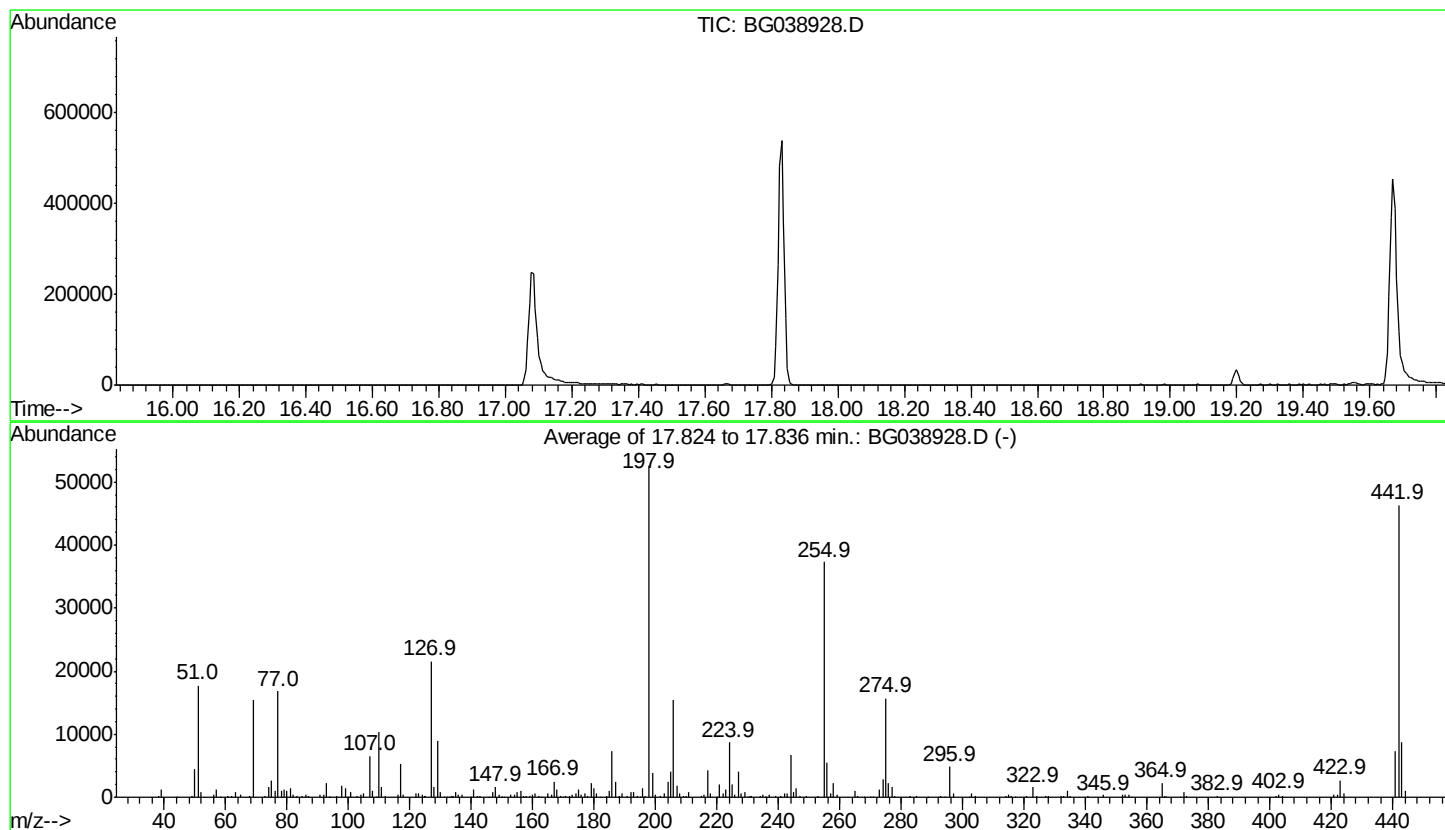

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	17766	PASS
68	69	0.00	2	1.2	180	PASS
69	198	0.00	100	29.5	15496	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	21529	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52584	PASS
199	198	5	9	7.2	3803	PASS
275	198	10	60	29.9	15723	PASS
365	198	1	100	4.3	2259	PASS
441	198	0.01	100	13.8	7251	PASS
442	198	50	100	88.1	46309	PASS
443	442	15	24	19.0	8779	PASS