
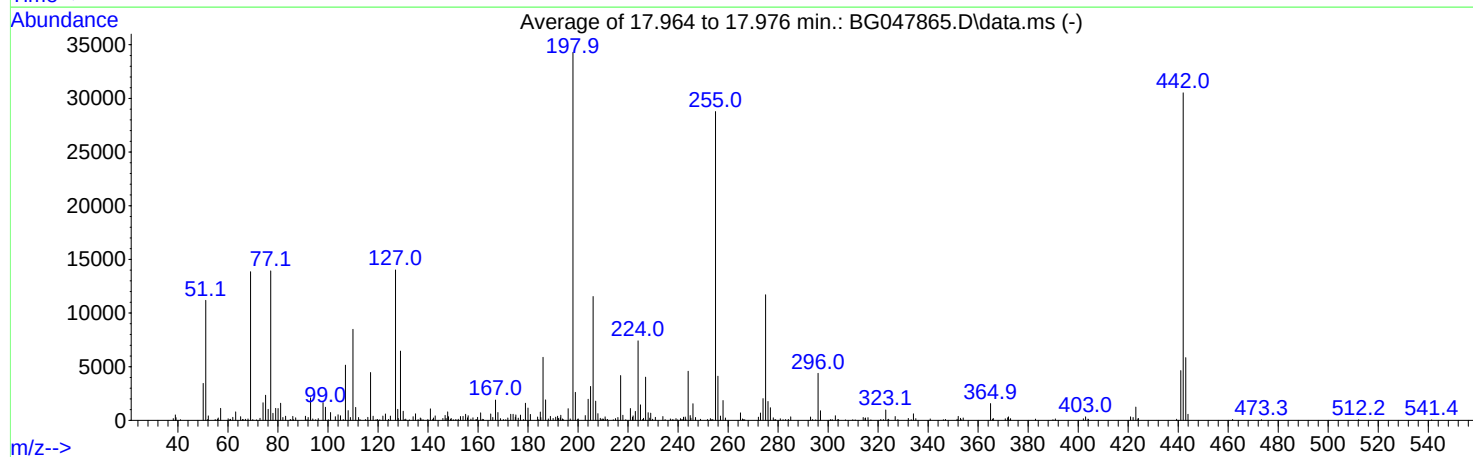


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010521\
 Data File : BG047865.D
 Acq On : 5 Jan 2021 13:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 15:55:16 2020

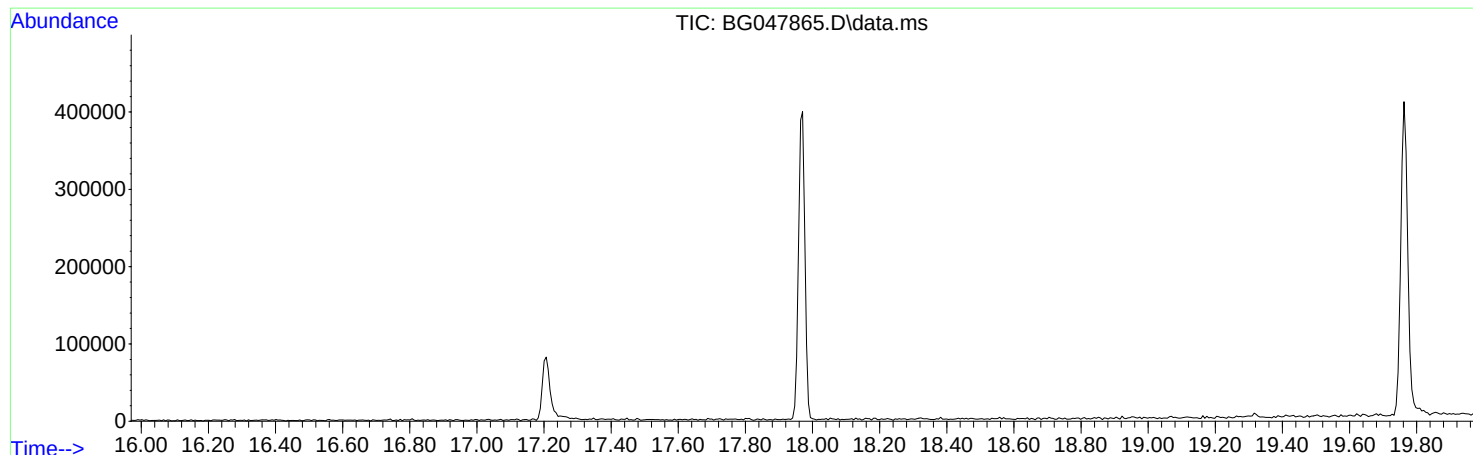

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	11178	PASS
68	69	0.00	2	1.0	139	PASS
69	198	0.00	100	40.4	13859	PASS
70	69	0.00	2	0.5	71	PASS
127	198	10	80	40.9	14018	PASS
197	198	0.00	2	0.4	138	PASS
198	198	100	100	100.0	34277	PASS
199	198	5	9	7.6	2605	PASS
275	198	10	60	34.1	11705	PASS
365	198	1	100	4.6	1570	PASS
441	198	0.01	100	13.5	4632	PASS
442	198	50	100	89.0	30515	PASS
443	442	15	24	19.1	5842	PASS