
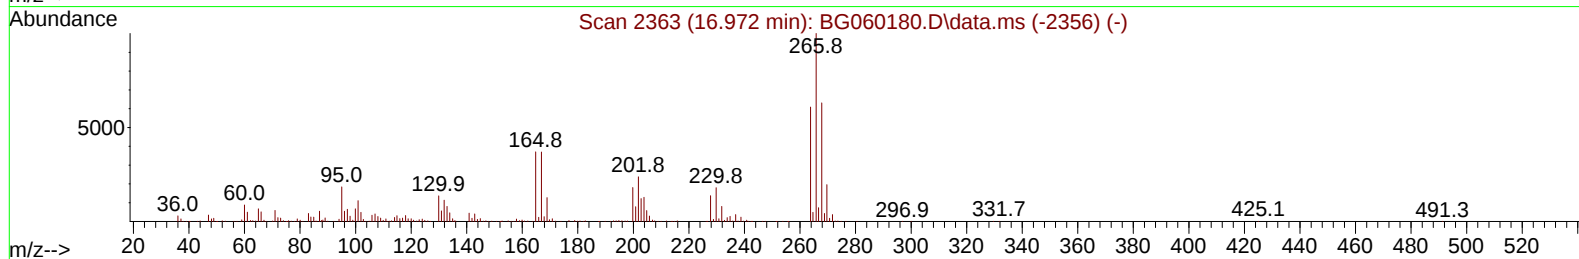
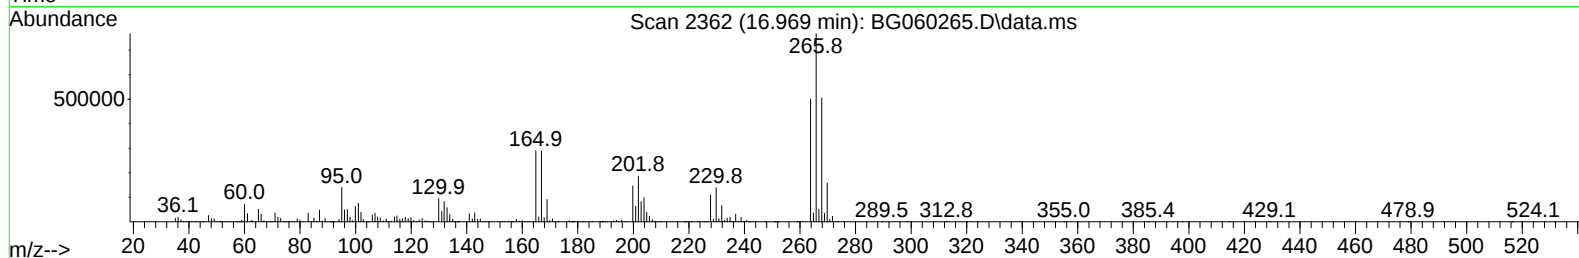


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\  
Data File : BG060265.D  
Acq On    : 5 Jan 2024 10:26  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Jan 05 12:04:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

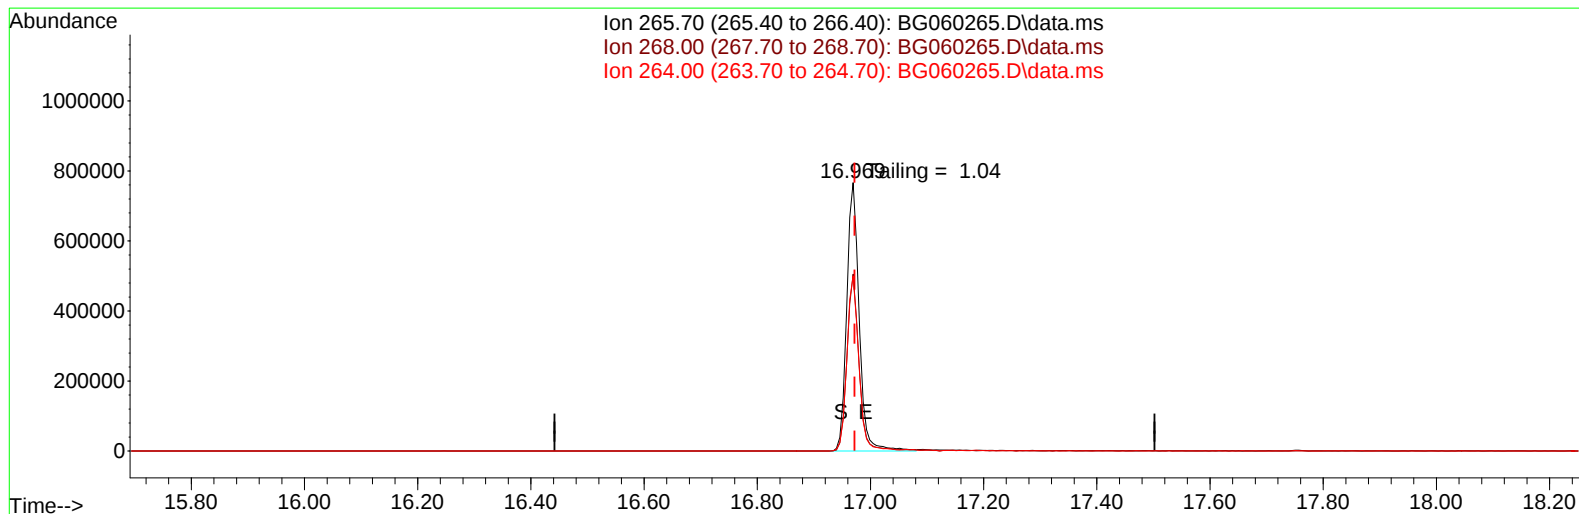

TIC: BG060265.D\data.ms

(70) **Pentachlorophenol (C)**




16.969min (-0.002) 311613.12 ng

response **1170365**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.87
264.00	65.80	65.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060265.D
Acq On : 5 Jan 2024 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 12:04:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

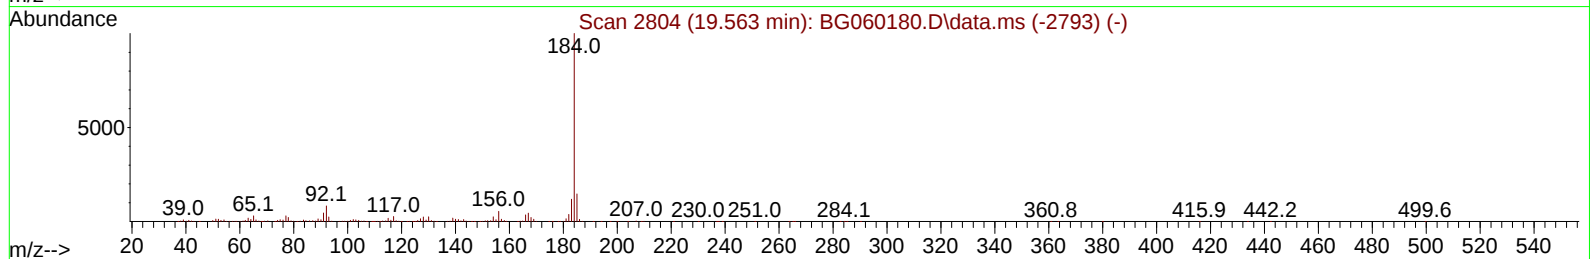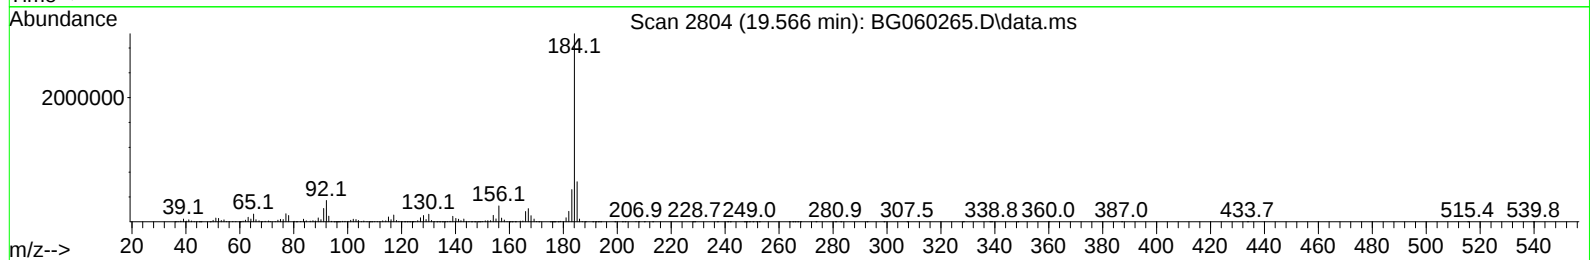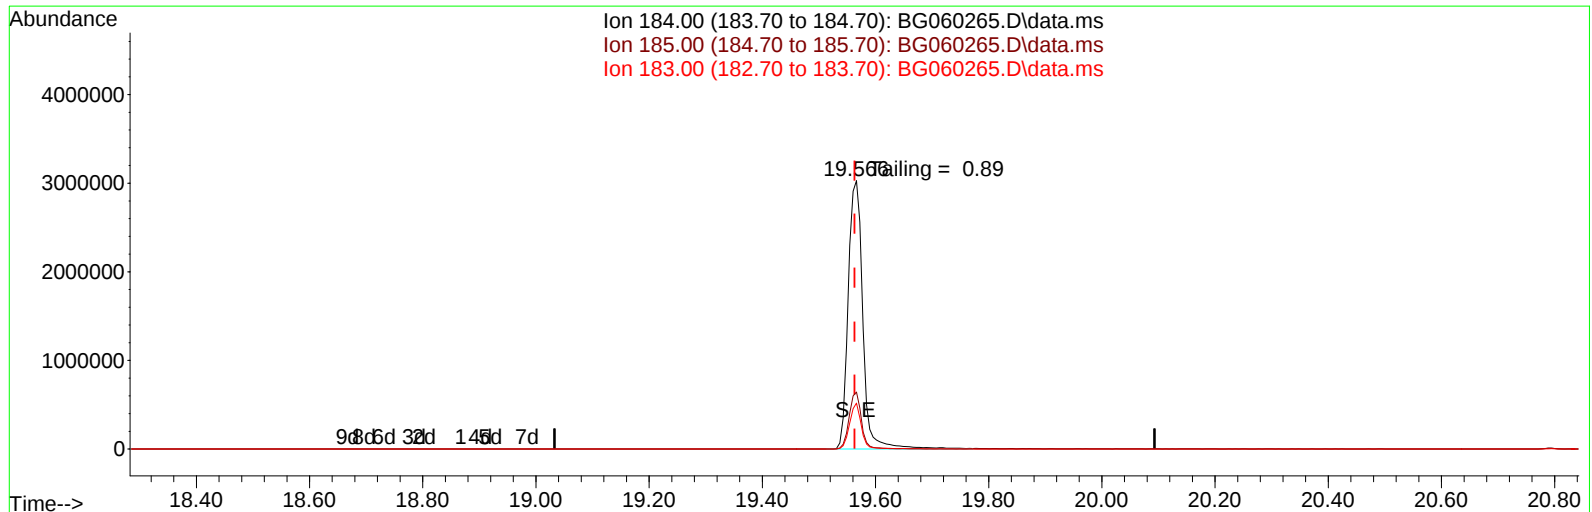

TIC: BG060265.D\data.ms

(77) Benzidine

19.566min (+ 0.004) 4116.38 ng m

response 5426139

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	21.26#
183.00	11.80	17.14#
0.00	0.00	0.00