

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
 Data File : BG060267.D
 Acq On : 5 Jan 2024 12:32
 Operator : MA/JU
 Sample : PB158174BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB158174BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.507	405	412	426	rBV	5372761	8552675	35.95%	8.690%
2	7.100	675	683	702	rBV	5252550	9230431	38.80%	9.379%
3	7.934	817	825	834	rBV	875621	1497051	6.29%	1.521%
4	9.097	1015	1023	1038	rBV	3174375	5669778	23.83%	5.761%
5	10.737	1291	1302	1318	rBV	1192493	2160464	9.08%	2.195%
6	13.193	1713	1720	1734	rBV	8592176	13975500	58.75%	14.200%
7	14.573	1947	1955	1965	rBV	2161653	3403790	14.31%	3.458%
8	16.060	2201	2208	2225	rBV	7233944	11484992	48.28%	11.669%
9	17.317	2415	2422	2434	rBV	3063395	4872048	20.48%	4.950%
10	19.943	2862	2869	2885	rBV	16656990	23788520	100.00%	24.170%
11	21.583	3141	3148	3160	rBV2	3186416	5536008	23.27%	5.625%
12	23.052	3392	3398	3405	rVB4	147561	275584	1.16%	0.280%
13	23.845	3526	3533	3541	rBV3	178722	389805	1.64%	0.396%
14	24.761	3677	3689	3706	rBV	2095879	6357634	26.73%	6.460%
15	25.884	3872	3880	3893	rBV3	207104	624134	2.62%	0.634%
16	27.229	4100	4109	4119	rVB5	181407	602614	2.53%	0.612%




Sum of corrected areas: 98421028

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060267.D
Acq On : 5 Jan 2024 12:32
Operator : MA/JU
Sample : PB158174BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

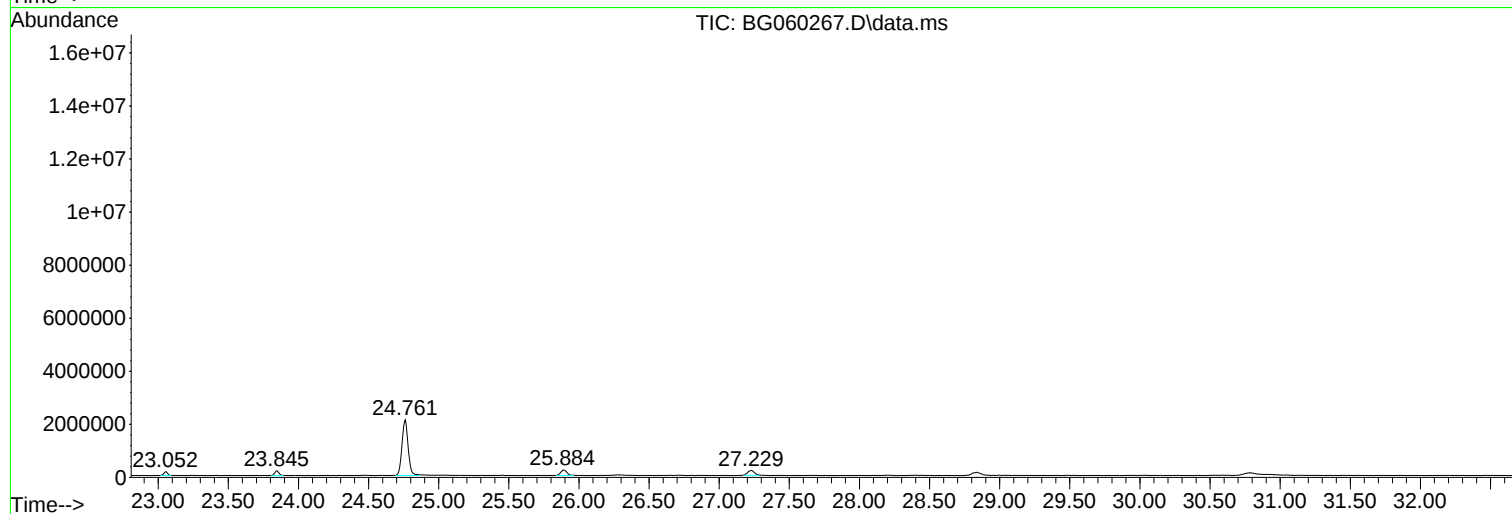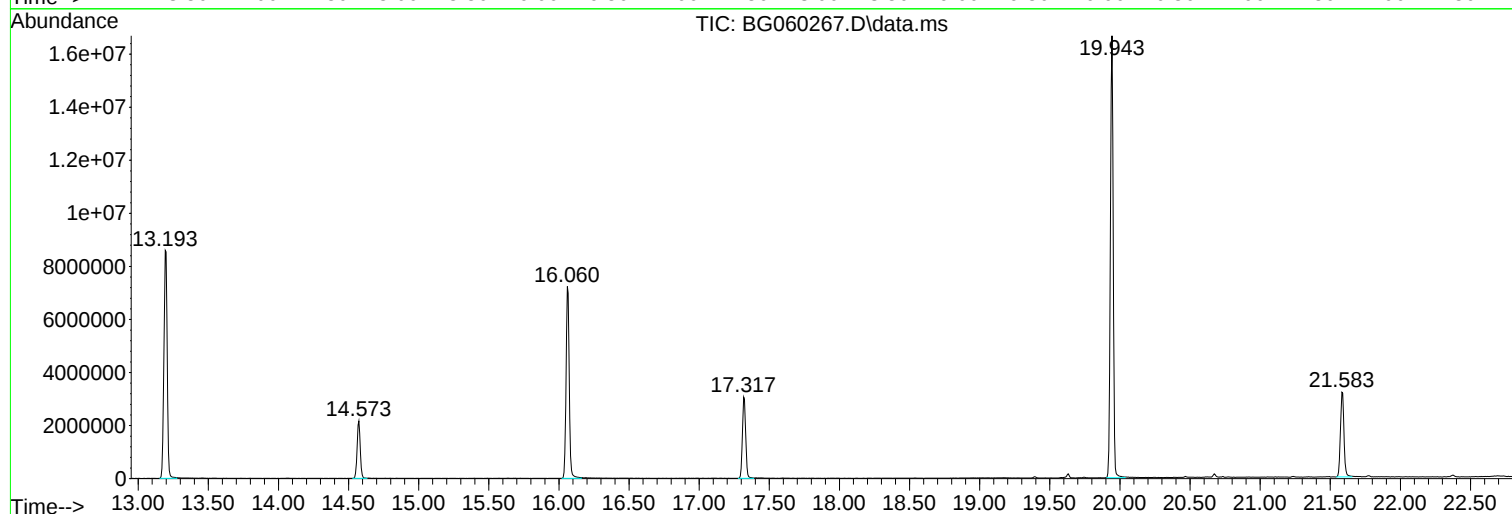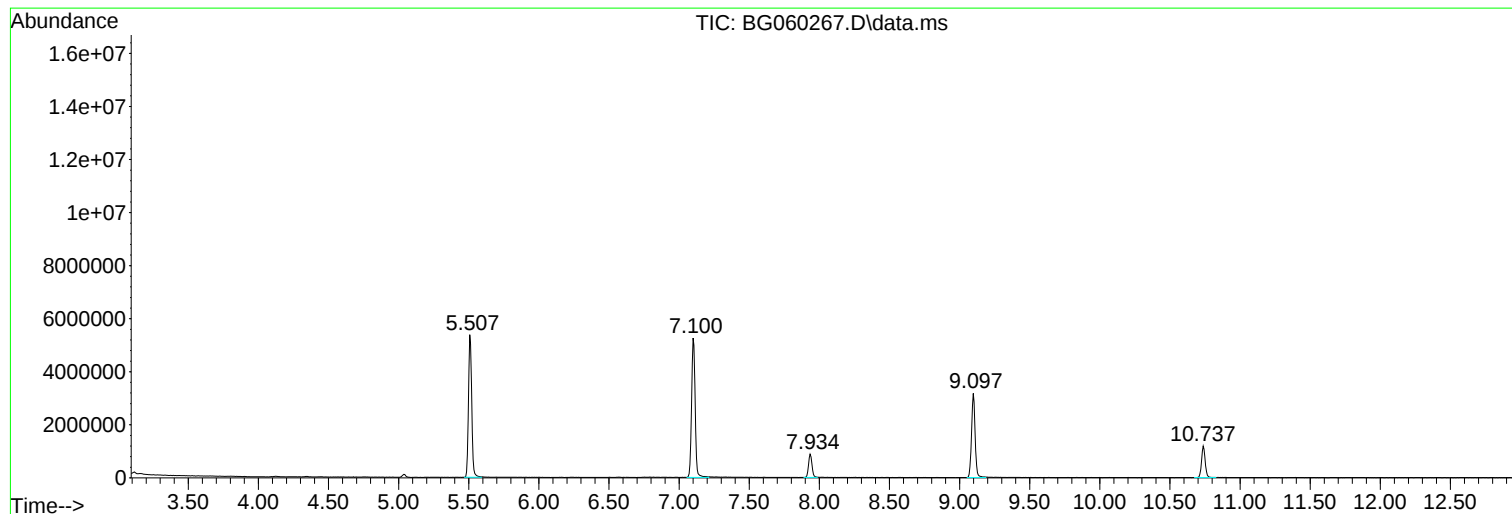

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060267.D
Acq On : 5 Jan 2024 12:32
Operator : MA/JU
Sample : PB158174BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060267.D
Acq On : 5 Jan 2024 12:32
Operator : MA/JU
Sample : PB158174BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------