

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
 Data File : BG060273.D
 Acq On : 5 Jan 2024 16:37
 Operator : MA/JU
 Sample : 05965-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COMA0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.114	3	4	22	rVB	1244555	1704055	10.02%	2.611%
2	5.506	404	411	427	rBV	1681871	2821532	16.59%	4.323%
3	7.092	672	681	692	rBV	935895	1715974	10.09%	2.629%
4	7.932	817	824	831	rBV	757965	1265461	7.44%	1.939%
5	9.096	1013	1022	1036	rBV	2530498	4498165	26.44%	6.892%
6	10.735	1293	1301	1309	rBV	962959	1725778	10.14%	2.644%
7	13.191	1711	1719	1735	rBV	6444731	10114270	59.45%	15.496%
8	14.571	1946	1954	1963	rBV	1647325	2594778	15.25%	3.975%
9	16.058	2198	2207	2224	rBV	5346508	8301549	48.80%	12.719%
10	17.321	2412	2422	2427	rBV	2264840	3549282	20.86%	5.438%
11	19.942	2861	2868	2883	rBV	12117507	17012044	100.00%	26.064%
12	21.228	3082	3087	3095	rBV	277400	412371	2.42%	0.632%
13	21.581	3141	3147	3164	rVB	2671220	4417054	25.96%	6.767%
14	23.244	3424	3430	3438	rVB2	111552	214599	1.26%	0.329%
15	24.195	3585	3592	3605	rBV4	111204	314601	1.85%	0.482%
16	24.754	3677	3687	3704	rVB	1658724	4607734	27.09%	7.060%




Sum of corrected areas: 65269247

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060273.D
Acq On : 5 Jan 2024 16:37
Operator : MA/JU
Sample : 05965-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

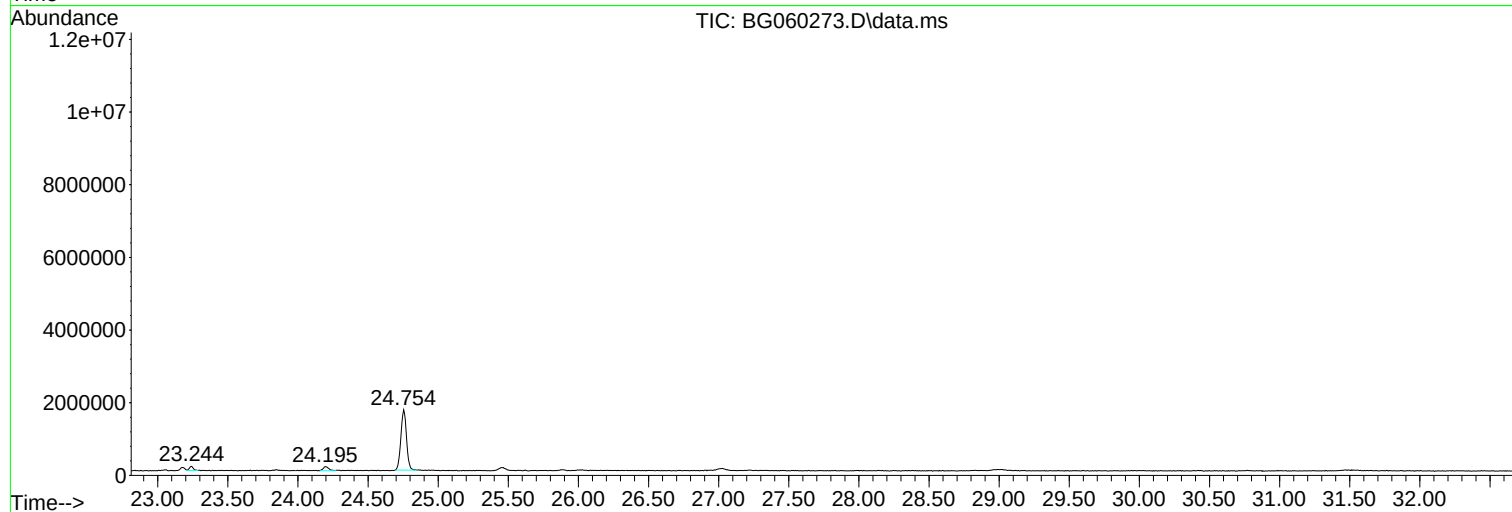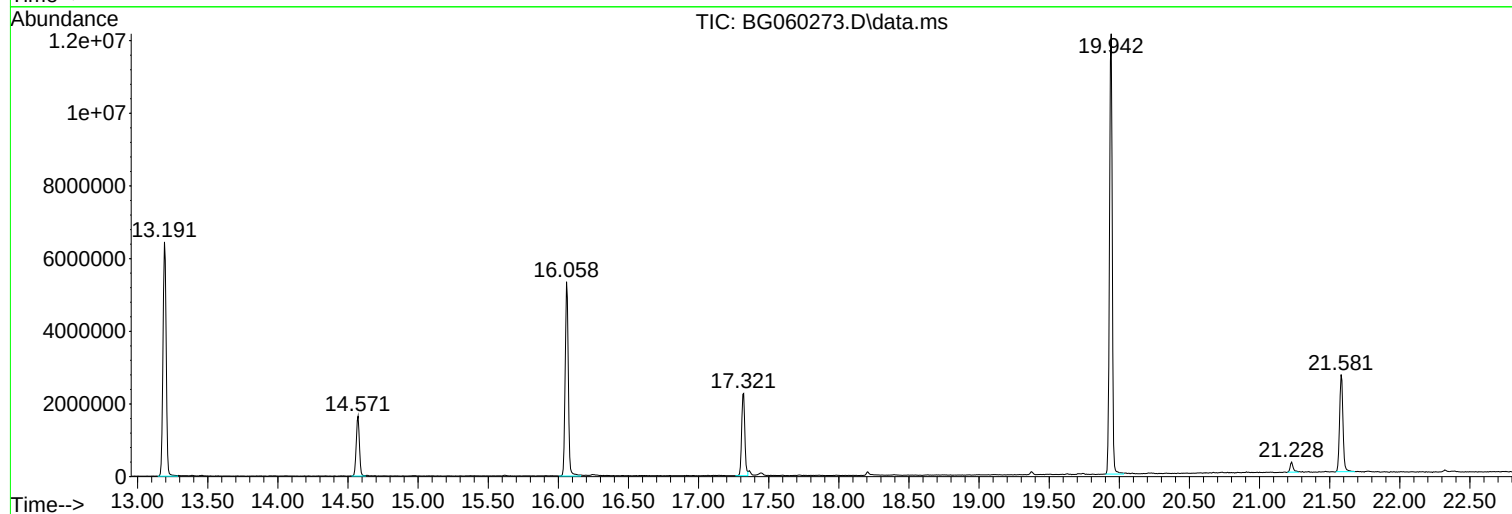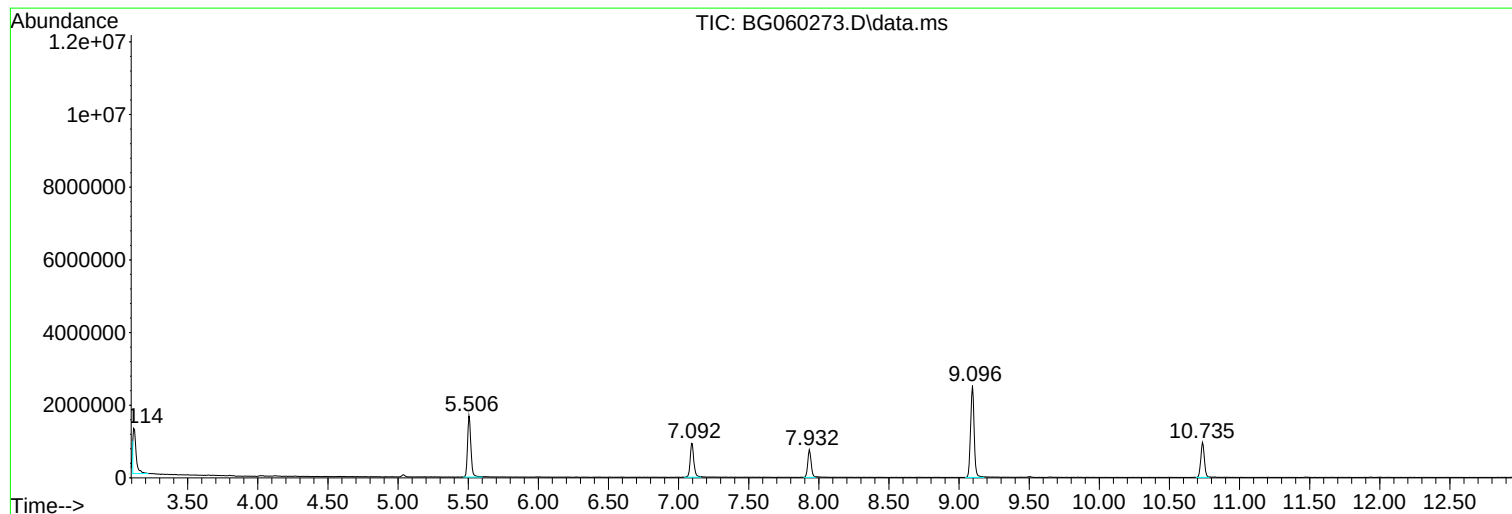

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060273.D
Acq On : 5 Jan 2024 16:37
Operator : MA/JU
Sample : 05965-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COMA0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.114	26.93 ng	1704060	1,4-Dichlorobenzene-d4	7.932

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	56
2			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23
3			Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	9
4			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	9
5			Acetic acid, 3-[1,3]dioxolan-2-y...	174	C8H14O4	1000186-02-3	9

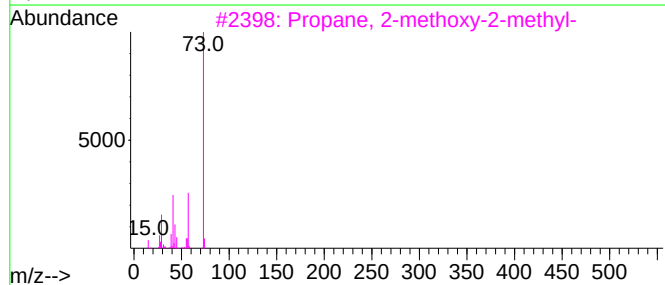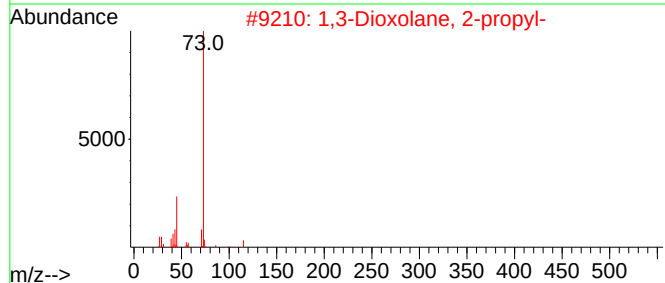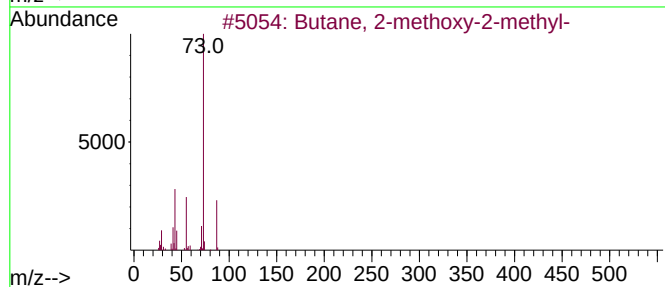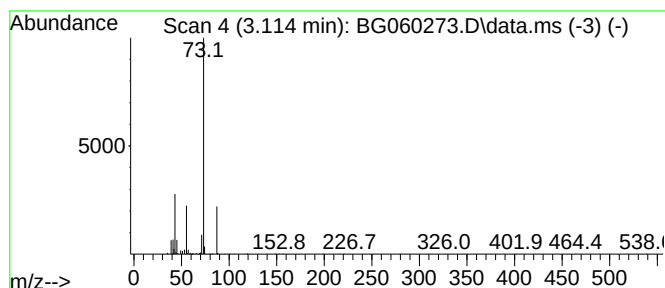

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060273.D
Acq On : 5 Jan 2024 16:37
Operator : MA/JU
Sample : 05965-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0MA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.114	26.9	ng	1704060	1	7.932	1265460	20.0