

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
 Data File : BG060276.D
 Acq On : 5 Jan 2024 18:38
 Operator : MA/JU
 Sample : 05967-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COM99

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.506	405	411	425	rBV	1368983	2250562	13.98%	3.701%
2	7.092	673	681	695	rBV	742965	1354131	8.41%	2.227%
3	7.932	815	824	833	rBV	721979	1252288	7.78%	2.059%
4	9.096	1013	1022	1034	rBV	2323110	4201709	26.10%	6.910%
5	10.735	1294	1301	1312	rBV	948352	1703967	10.58%	2.802%
6	13.191	1712	1719	1733	rBV	6435785	10051695	62.43%	16.530%
7	14.572	1946	1954	1962	rBV	1558094	2511579	15.60%	4.130%
8	14.783	1988	1990	1998	rVB	1190593	1285971	7.99%	2.115%
9	16.058	2196	2207	2224	rBV	4817243	7449080	46.27%	12.250%
10	17.316	2415	2421	2433	rBV	2243836	3349647	20.80%	5.508%
11	18.203	2566	2572	2581	rBV2	113512	180226	1.12%	0.296%
12	19.936	2861	2867	2883	rBV	11297986	16100690	100.00%	26.477%
13	21.229	3083	3087	3091	rBV2	218406	309260	1.92%	0.509%
14	21.581	3140	3147	3159	rBV2	2588953	4214139	26.17%	6.930%
15	24.754	3676	3687	3699	rBV	1629574	4594504	28.54%	7.556%




Sum of corrected areas: 60809448

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060276.D
Acq On : 5 Jan 2024 18:38
Operator : MA/JU
Sample : 05967-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COM99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

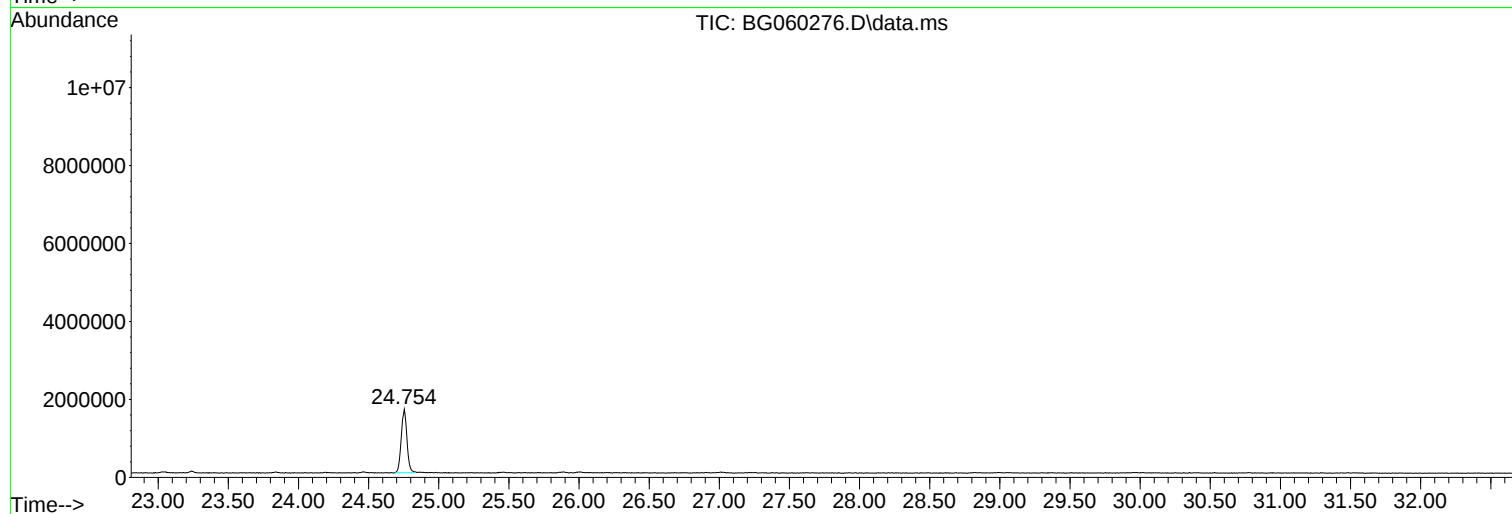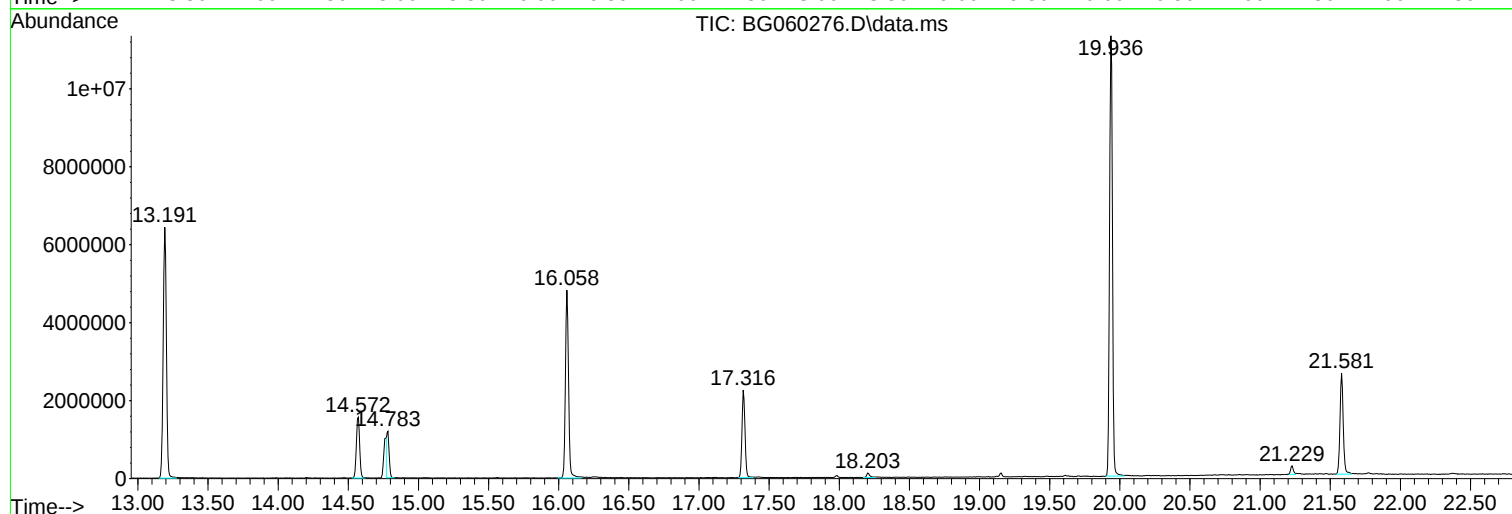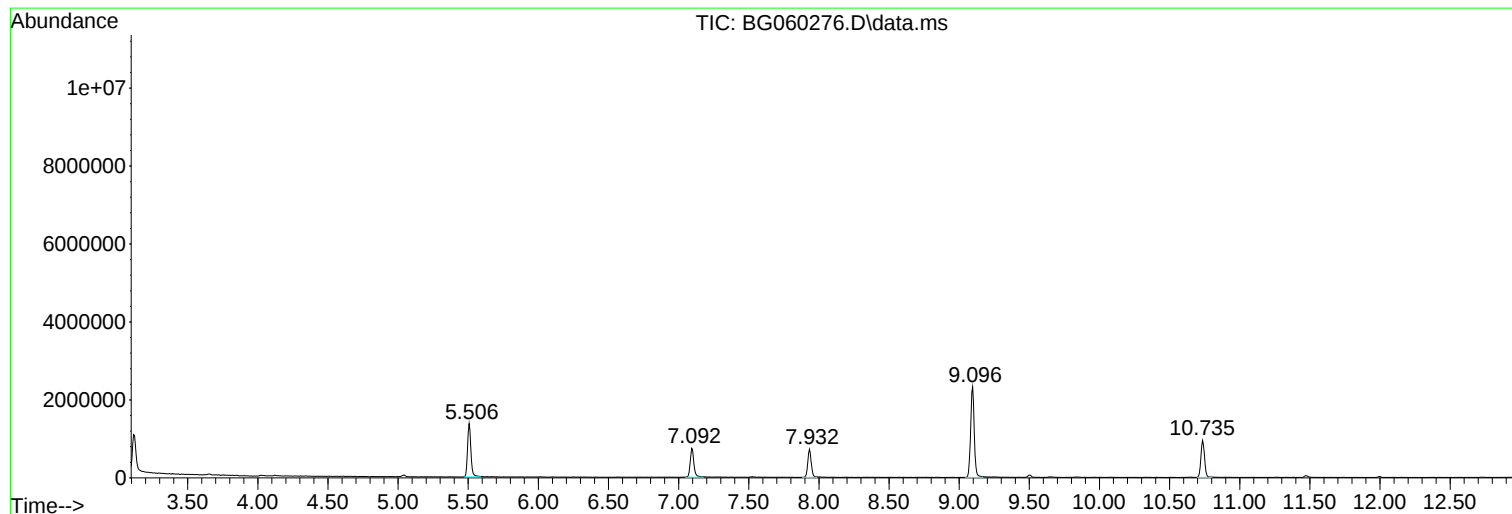

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060276.D
Acq On : 5 Jan 2024 18:38
Operator : MA/JU
Sample : 05967-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COM99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060276.D
Acq On : 5 Jan 2024 18:38
Operator : MA/JU
Sample : 05967-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COM99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc