
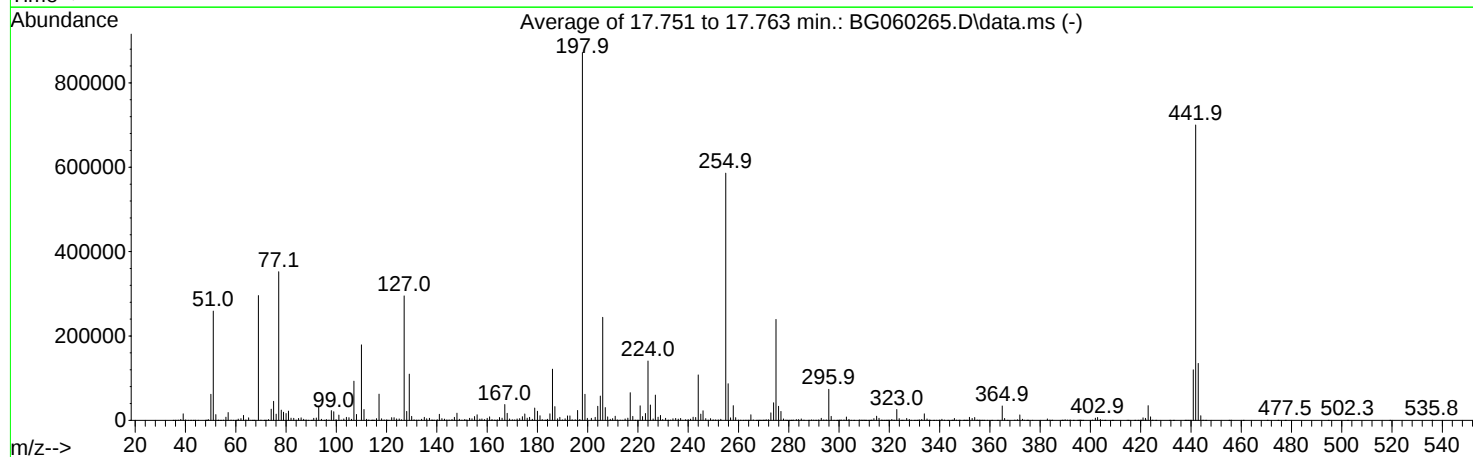


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060265.D
Acq On : 5 Jan 2024 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 30 03:14:04 2023

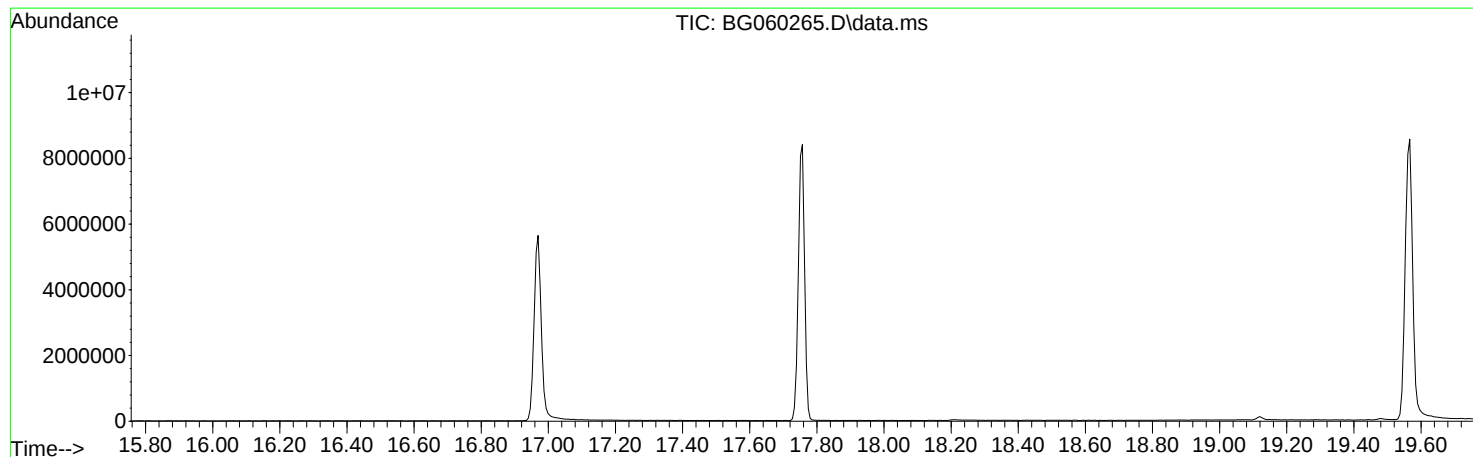

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	258974	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	295858	PASS
70	69	0.00	2	0.2	620	PASS
127	198	10	80	33.8	295061	PASS
197	198	0.00	2	0.3	2462	PASS
198	198	100	100	100.0	872021	PASS
199	198	5	9	7.1	61693	PASS
275	198	10	60	27.4	239317	PASS
365	198	1	100	3.9	34075	PASS
441	198	0.01	100	13.7	119725	PASS
442	442	50	100	100.0	700203	PASS
443	442	15	24	19.3	135136	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/5/2024	BNA_G	<u>BG060265.D</u>
Compound Name	Response	Retention Time
DDT	2914269	20.794
DDD	116000	20.348
DDE	5607	19.843
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
121607	3035876	4.01

Instrument :
BNA_G
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\  
Data File : BG060265.D  
Acq On    : 5 Jan 2024 10:26  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 05 12:04:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

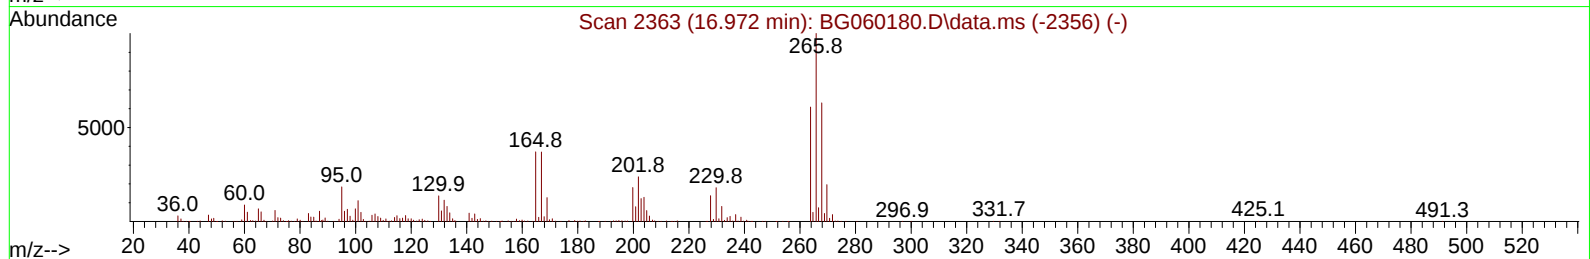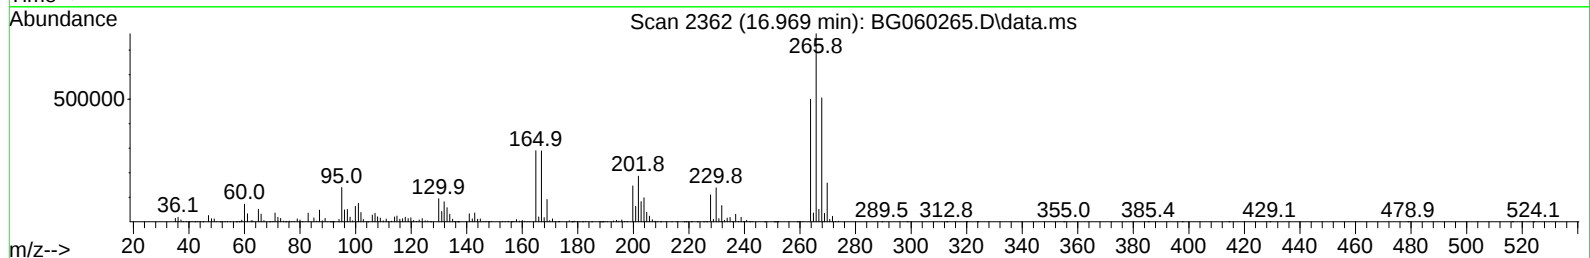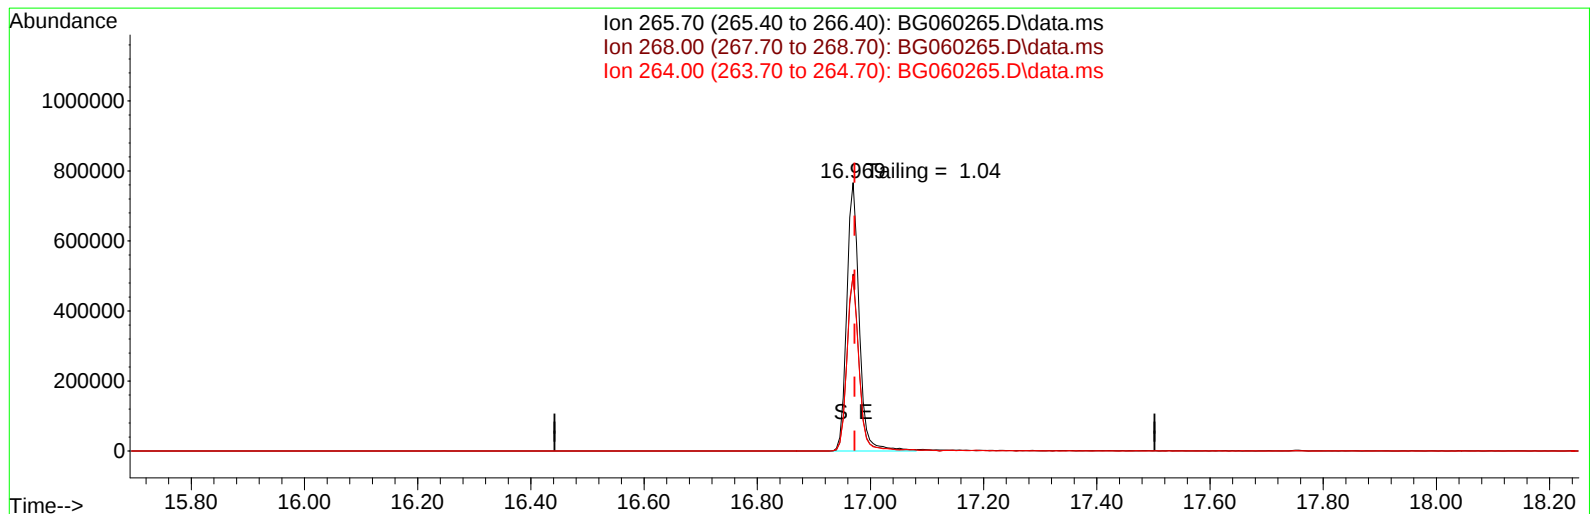

TIC: BG060265.D\data.ms

(70) Pentachlorophenol (C)

16.969min (-0.002) 311613.12 ng




response **1170365**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.87
264.00	65.80	65.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010524\
Data File : BG060265.D
Acq On : 5 Jan 2024 10:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 05 12:04:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

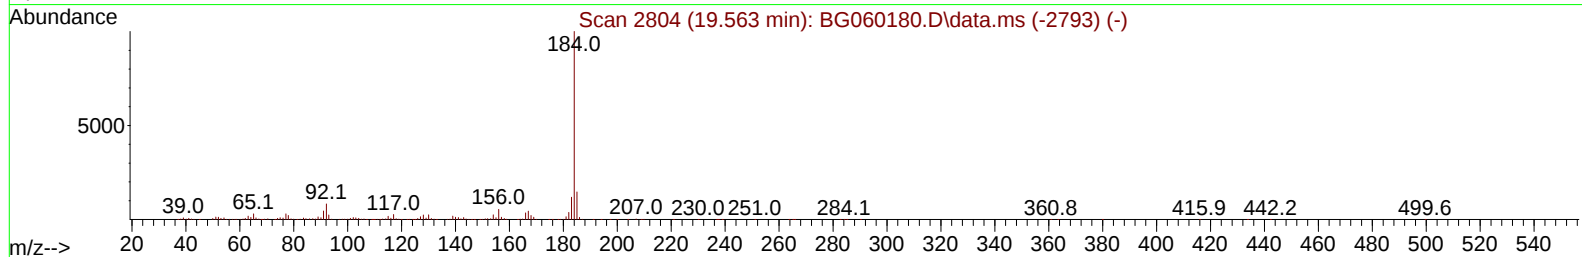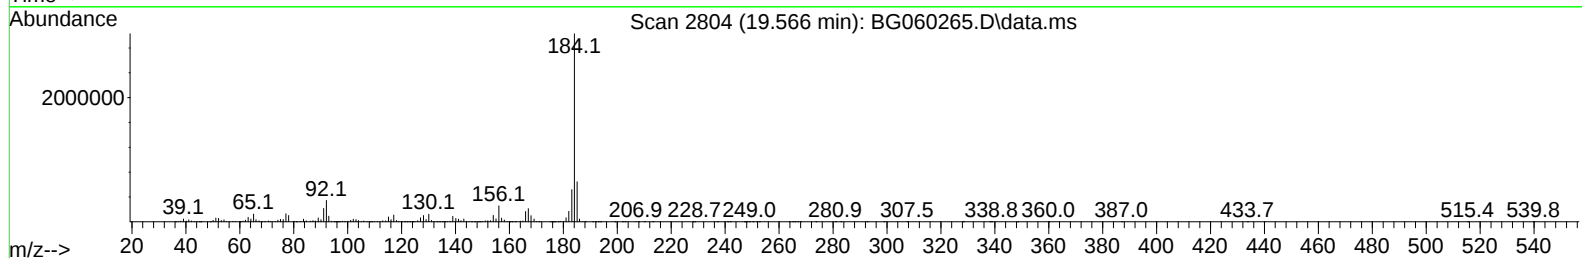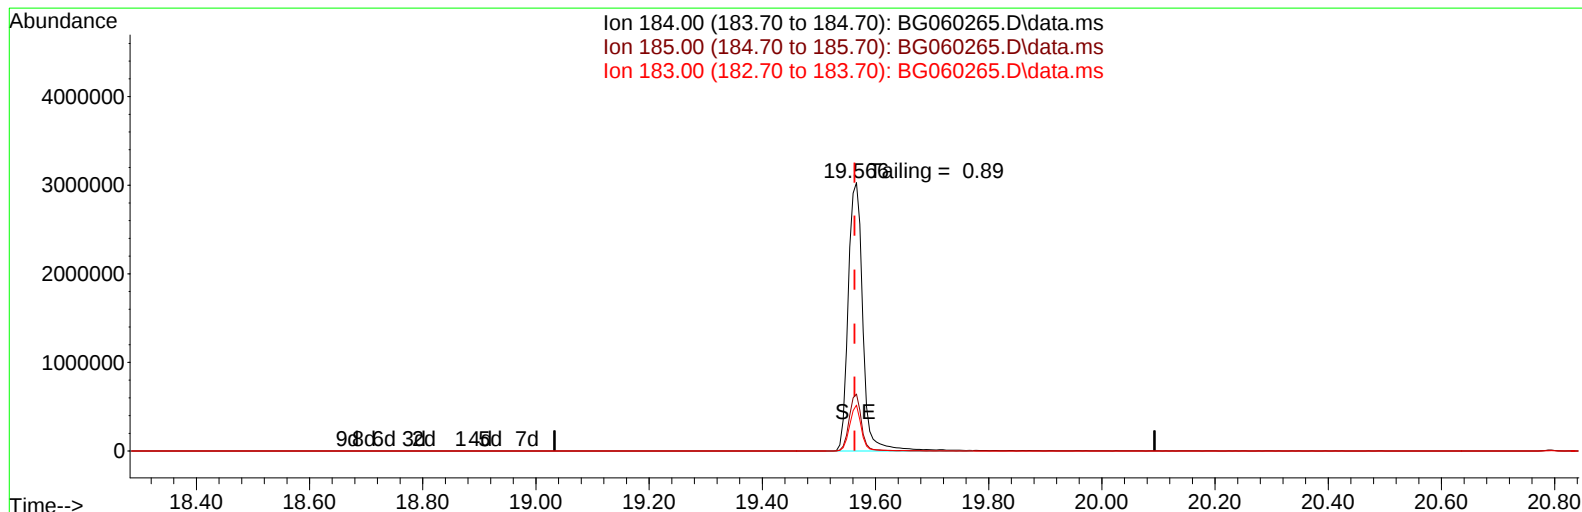

TIC: BG060265.D\data.ms

(77) Benzidine

19.566min (+ 0.004) 4116.38 ng m

response 5426139

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	21.26#
183.00	11.80	17.14#
0.00	0.00	0.00