


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010621\
 Data File : BG047876.D
 Acq On : 6 Jan 2021 15:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 15:55:16 2020

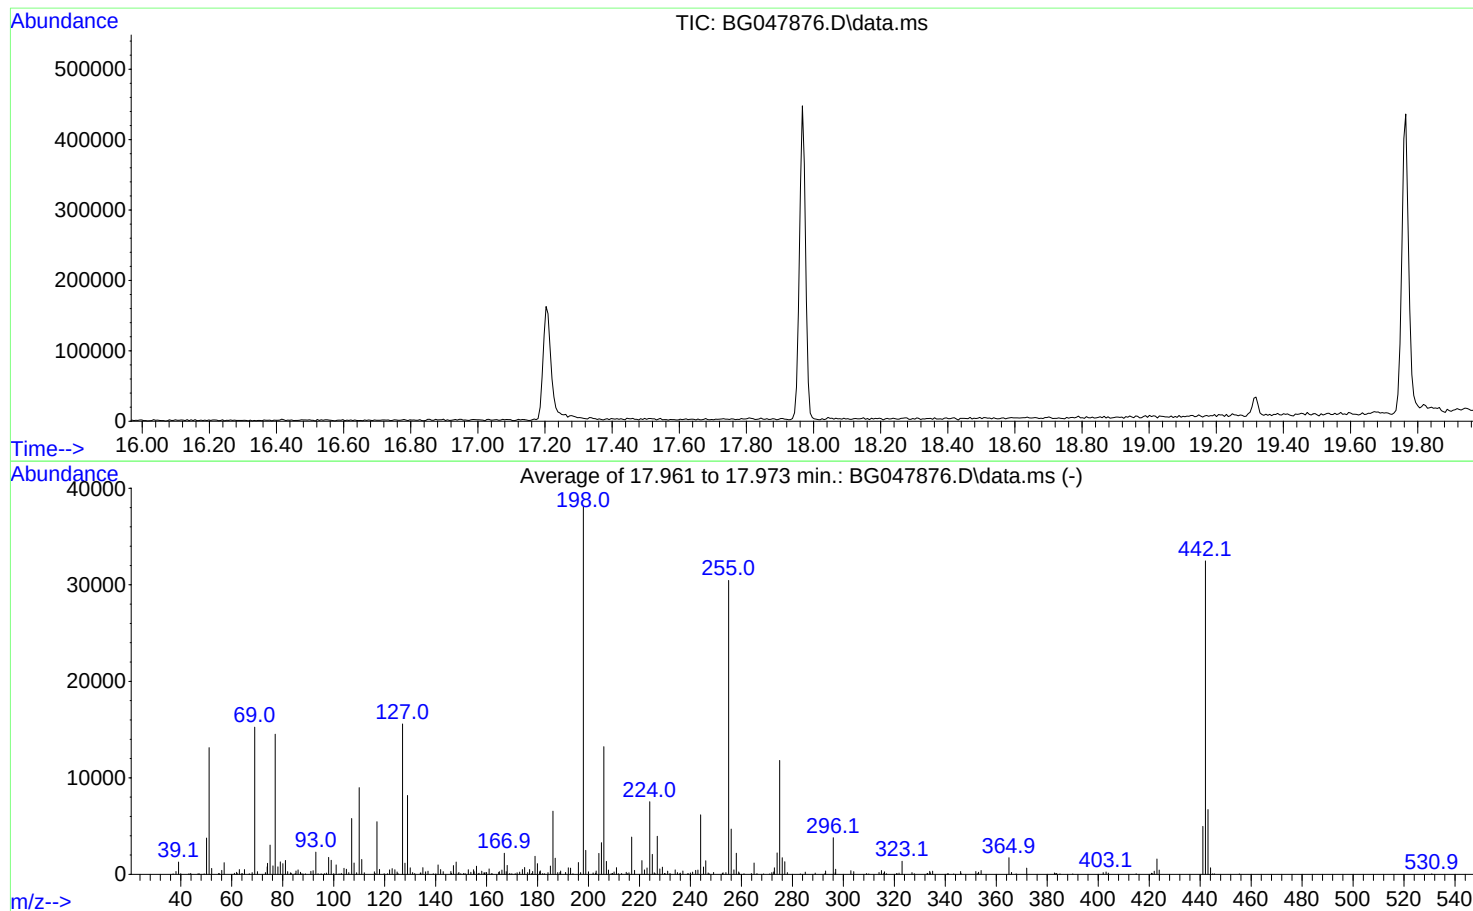

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	13130	PASS
68	69	0.00	2	1.2	178	PASS
69	198	0.00	100	40.0	15257	PASS
70	69	0.00	2	1.9	284	PASS
127	198	10	80	40.9	15579	PASS
197	198	0.00	2	0.5	182	PASS
198	198	100	100	100.0	38112	PASS
199	198	5	9	6.5	2493	PASS
275	198	10	60	31.0	11801	PASS
365	198	1	100	4.5	1727	PASS
441	198	0.01	100	13.0	4973	PASS
442	198	50	100	85.2	32472	PASS
443	442	15	24	20.7	6721	PASS