

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010623\
 Data File : BG056219.D
 Acq On : 6 Jan 2023 10:14
 Operator : CG/JU
 Sample : PB149983BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK983

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.356	8	11	16	rVB2	8641	12531	0.83%	0.094%
2	3.632	54	58	66	rVB2	9919	16132	1.07%	0.120%
3	4.066	128	132	146	rBV	92525	159647	10.60%	1.191%
4	4.372	180	184	186	rVB2	1271	1514	0.10%	0.011%
5	4.431	190	194	196	rVB2	2057	2882	0.19%	0.022%
6	4.525	206	210	214	rBV2	1128	1957	0.13%	0.015%
7	7.462	702	710	721	rBV	139846	238059	15.81%	1.776%
8	7.639	733	740	748	rVB	117480	188817	12.54%	1.409%
9	7.856	770	777	786	rVB	143020	240534	15.98%	1.795%
10	8.332	850	858	866	rBB	129984	217625	14.45%	1.624%
11	9.019	967	975	987	rBV	193149	338220	22.46%	2.524%
12	9.501	1050	1057	1068	rBB	128056	231816	15.40%	1.730%
13	10.230	1175	1181	1189	rBV	120470	209856	13.94%	1.566%
14	10.770	1266	1273	1281	rBV2	203379	369880	24.57%	2.760%
15	11.164	1330	1340	1348	rBV	184545	321610	21.36%	2.400%
16	11.287	1354	1361	1368	rBV	188884	329176	21.86%	2.456%
17	12.721	1600	1605	1613	rBB3	4003	6438	0.43%	0.048%
18	14.331	1873	1879	1889	rVB	445324	641189	42.59%	4.784%
19	14.642	1924	1932	1941	rBV2	472337	764864	50.80%	5.707%
20	14.942	1975	1983	1991	rBV	362673	565797	37.58%	4.222%
21	15.106	2004	2011	2028	rBV	150360	247176	16.42%	1.844%
22	15.929	2141	2151	2158	rBV	685419	1048101	69.61%	7.821%
23	16.029	2162	2168	2177	rBV	167182	241345	16.03%	1.801%
24	16.170	2187	2192	2197	rVB2	3572	3919	0.26%	0.029%
25	17.321	2386	2388	2391	rBV3	1267	1784	0.12%	0.013%
26	17.410	2402	2403	2409	rVB3	1307	1595	0.11%	0.012%
27	17.545	2421	2426	2427	rBV3	1976	1844	0.12%	0.014%
28	17.680	2442	2449	2455	rVV	495631	774713	51.45%	5.781%
29	17.780	2458	2466	2476	rVB	777325	1223835	81.28%	9.132%
30	17.886	2481	2484	2487	rBV4	1725	2386	0.16%	0.018%
31	18.032	2506	2509	2510	rVV3	2814	2937	0.20%	0.022%
32	18.074	2514	2516	2517	rBV2	3429	2891	0.19%	0.022%
33	18.314	2555	2557	2561	rVB4	3119	3209	0.21%	0.024%
34	18.397	2568	2571	2574	rBV3	2654	4418	0.29%	0.033%
35	18.497	2586	2588	2592	rVB4	2022	2282	0.15%	0.017%
36	18.585	2598	2603	2604	rBV4	2677	3813	0.25%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010623\
 Data File : BG056219.D
 Acq On : 6 Jan 2023 10:14
 Operator : CG/JU
 Sample : PB149983BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK983

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
 Title : SVOA CALIBRATION

37	18.667	2614	2617	2620	rBV4	2243	3303	0.22%	0.025%
38	19.114	2690	2693	2695	rBV2	1295	1741	0.12%	0.013%
39	19.390	2737	2740	2744	rBV5	1962	2665	0.18%	0.020%
40	19.425	2744	2746	2748	rBV3	1822	2151	0.14%	0.016%
41	19.554	2763	2768	2773	rBV5	2295	5277	0.35%	0.039%
42	19.607	2773	2777	2783	rBV2	13693	20824	1.38%	0.155%
43	19.678	2783	2789	2794	rVV2	9959	16062	1.07%	0.120%
44	19.777	2803	2806	2808	rBV4	1802	2120	0.14%	0.016%
45	19.871	2819	2822	2825	rBV3	1526	2337	0.16%	0.017%
46	19.924	2829	2831	2834	rVB	2712	1761	0.12%	0.013%
47	20.042	2842	2851	2859	rBV	1076984	1505662	100.00%	11.235%
48	20.101	2859	2861	2863	rVB3	2342	1776	0.12%	0.013%
49	20.153	2868	2870	2872	rVB2	2797	1902	0.13%	0.014%
50	20.183	2872	2875	2877	rVB3	2179	2510	0.17%	0.019%
51	20.206	2877	2879	2881	rBV3	2237	2261	0.15%	0.017%
52	20.247	2883	2886	2887	rBV2	2828	2631	0.17%	0.020%
53	20.347	2902	2903	2906	rBV3	3121	3428	0.23%	0.026%
54	20.494	2926	2928	2929	rBV2	2823	2238	0.15%	0.017%
55	20.700	2960	2963	2964	rBV3	2800	3084	0.20%	0.023%
56	20.953	3005	3006	3008	rBV2	4730	3630	0.24%	0.027%
57	21.975	3173	3180	3189	rVB2	500932	875690	58.16%	6.534%
58	22.133	3203	3207	3209	rBV4	5068	6299	0.42%	0.047%
59	23.156	3373	3381	3383	rBV6	21443	44678	2.97%	0.333%
60	24.284	3571	3573	3575	rVB3	5568	3938	0.26%	0.029%
61	24.390	3589	3591	3597	rVB6	15809	22358	1.48%	0.167%
62	25.189	3717	3727	3739	rVB2	493138	1467761	97.48%	10.952%
63	25.430	3757	3768	3779	rBV2	288516	898751	59.69%	6.706%
64	26.129	3886	3887	3889	rBV2	4412	3779	0.25%	0.028%
65	26.270	3909	3911	3914	rVB4	5277	4298	0.29%	0.032%
66	26.640	3967	3974	3981	rVB6	18062	46476	3.09%	0.347%
67	27.674	4148	4150	4153	rBV4	4250	3910	0.26%	0.029%
68	31.240	4755	4757	4758	rBV2	4159	3264	0.22%	0.024%
69	31.587	4814	4816	4818	rBV3	4116	3516	0.23%	0.026%
70	32.322	4939	4941	4944	rBV4	4330	4539	0.30%	0.034%


Sum of corrected areas: 13401412

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010623\
Data File : BG056219.D
Acq On : 6 Jan 2023 10:14
Operator : CG/JU
Sample : PB149983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

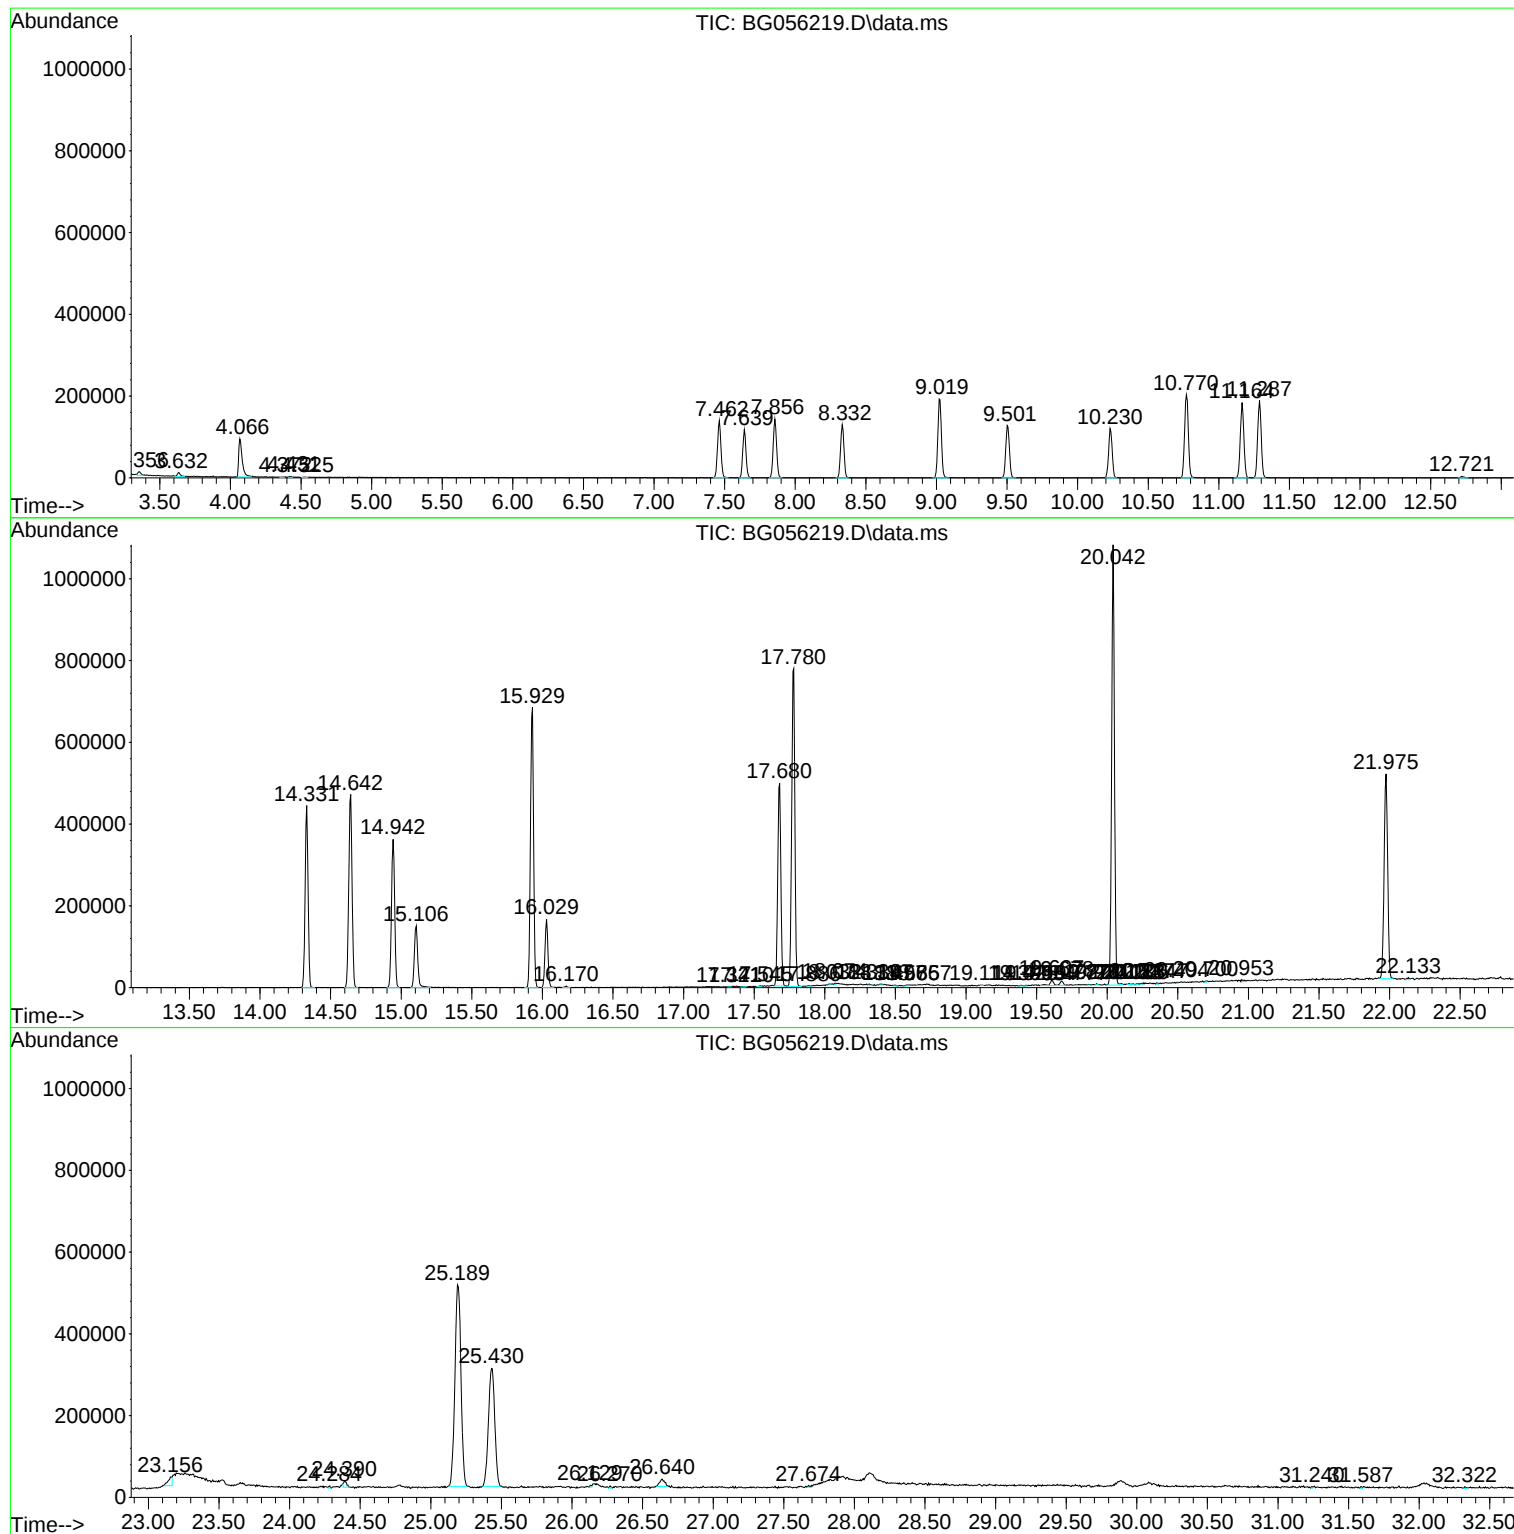

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010623\
Data File : BG056219.D
Acq On : 6 Jan 2023 10:14
Operator : CG/JU
Sample : PB149983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010623\
Data File : BG056219.D
Acq On : 6 Jan 2023 10:14
Operator : CG/JU
Sample : PB149983BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK983

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------