


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010819\
 Data File : BG038995.D
 Acq On : 8 Jan 2019 15:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

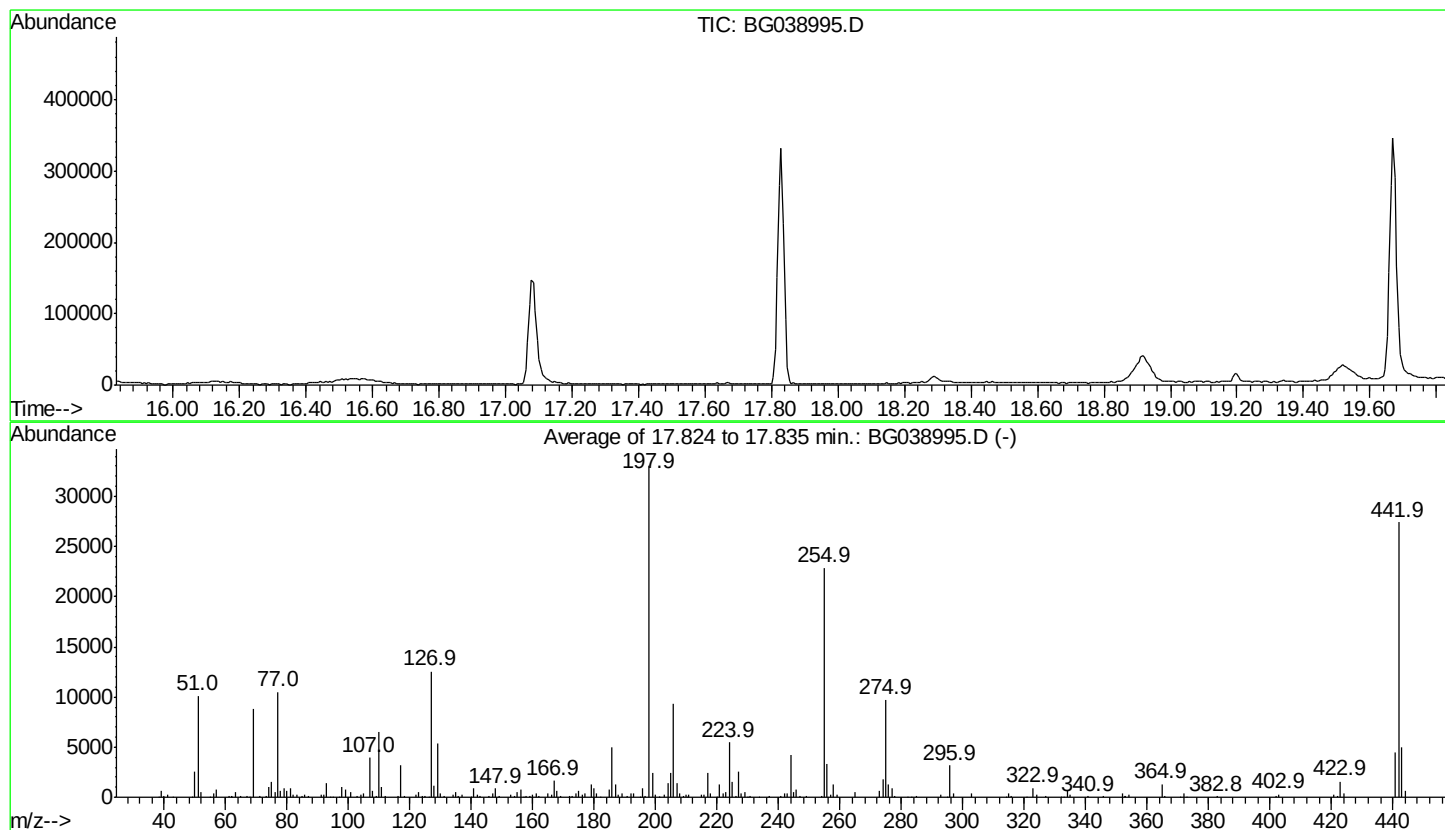

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	10108	PASS
68	69	0.00	2	0.8	67	PASS
69	198	0.00	100	26.5	8752	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.0	12552	PASS
197	198	0.00	2	0.3	97	PASS
198	198	100	100	100.0	33064	PASS
199	198	5	9	7.4	2444	PASS
275	198	10	60	29.5	9740	PASS
365	198	1	100	4.0	1321	PASS
441	198	0.01	100	13.5	4465	PASS
442	198	50	100	82.9	27421	PASS
443	442	15	24	18.2	5004	PASS