
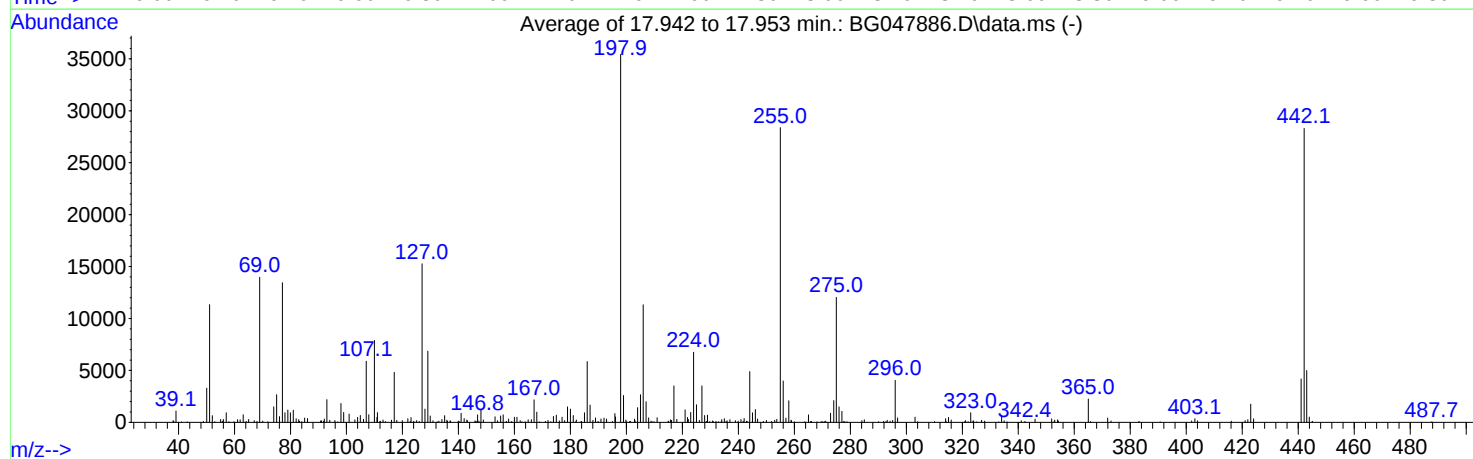


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010821\
 Data File : BG047886.D
 Acq On : 8 Jan 2021 14:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 08 11:19:41 2021

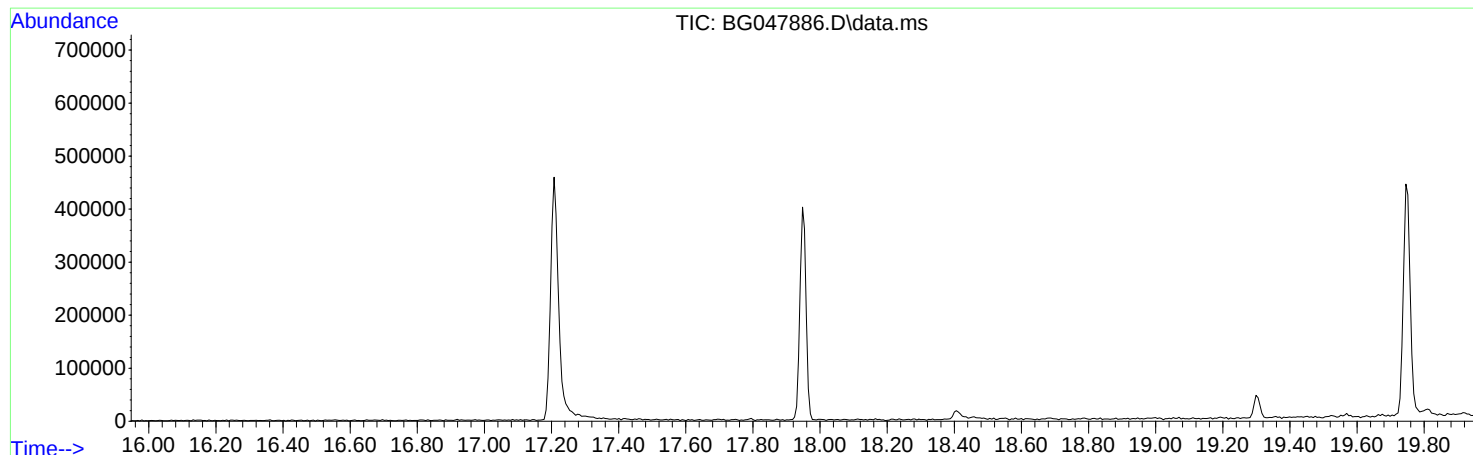

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	11338	PASS
68	69	0.00	2	0.6	86	PASS
69	198	0.00	100	39.4	13968	PASS
70	69	0.00	2	0.9	129	PASS
127	198	10	80	43.1	15267	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35421	PASS
199	198	5	9	7.3	2589	PASS
275	198	10	60	34.0	12040	PASS
365	198	1	100	6.4	2254	PASS
441	198	0.01	100	11.8	4177	PASS
442	198	50	100	79.9	28309	PASS
443	442	15	24	17.6	4992	PASS