
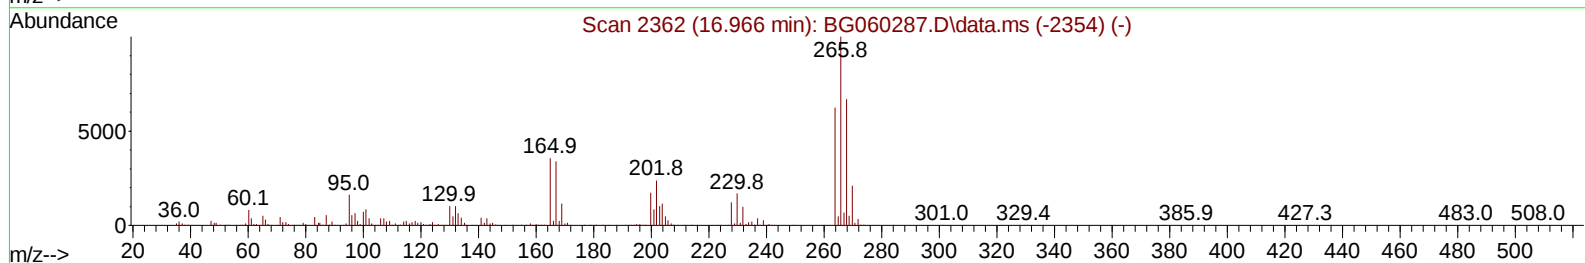
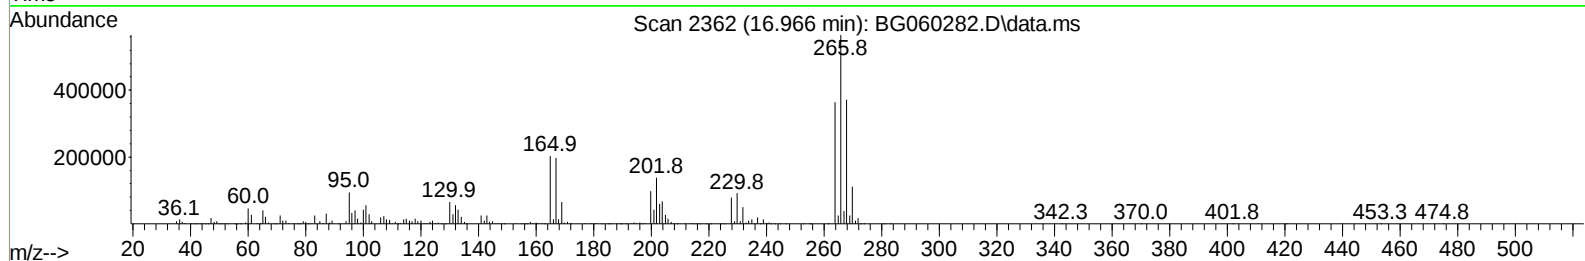


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010824\
Data File : BG060282.D
Acq On : 8 Jan 2024 15:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 04:13:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

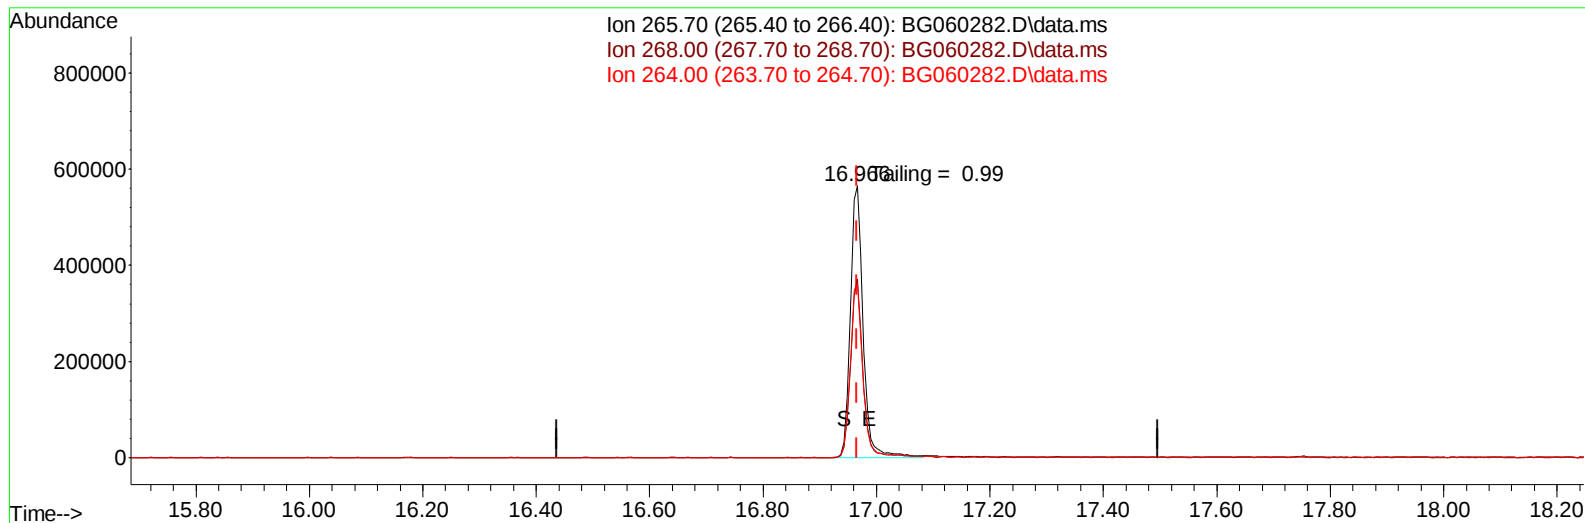

TIC: BG060282.D\data.ms

(70) Pentachlorophenol (C)




16.966min (+ 0.000) 122815.05 ng

response 885145

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	65.73
264.00	62.30	64.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010824\
Data File : BG060282.D
Acq On : 8 Jan 2024 15:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 04:13:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

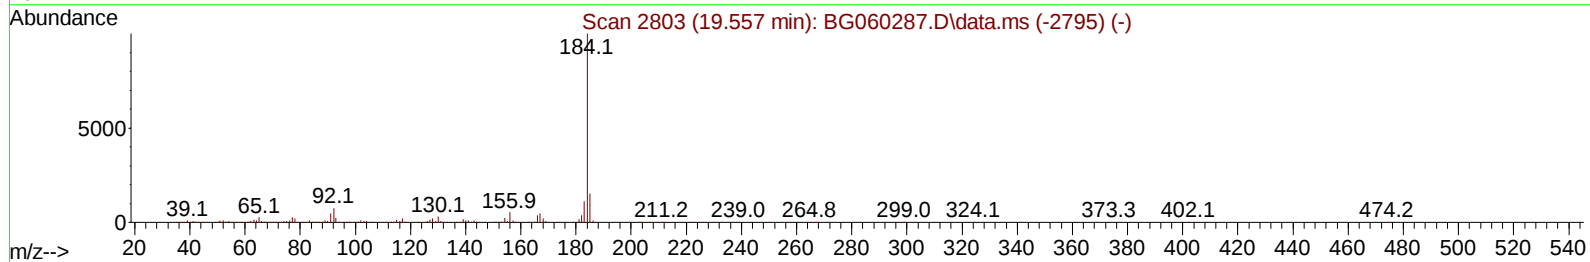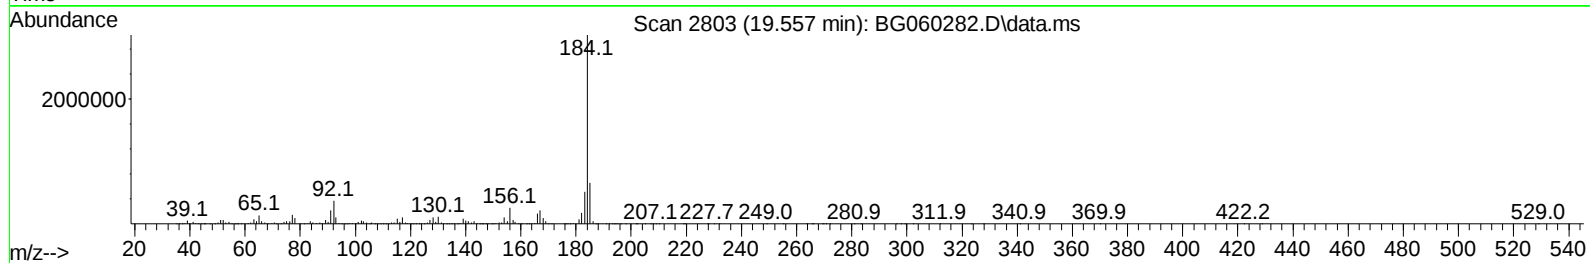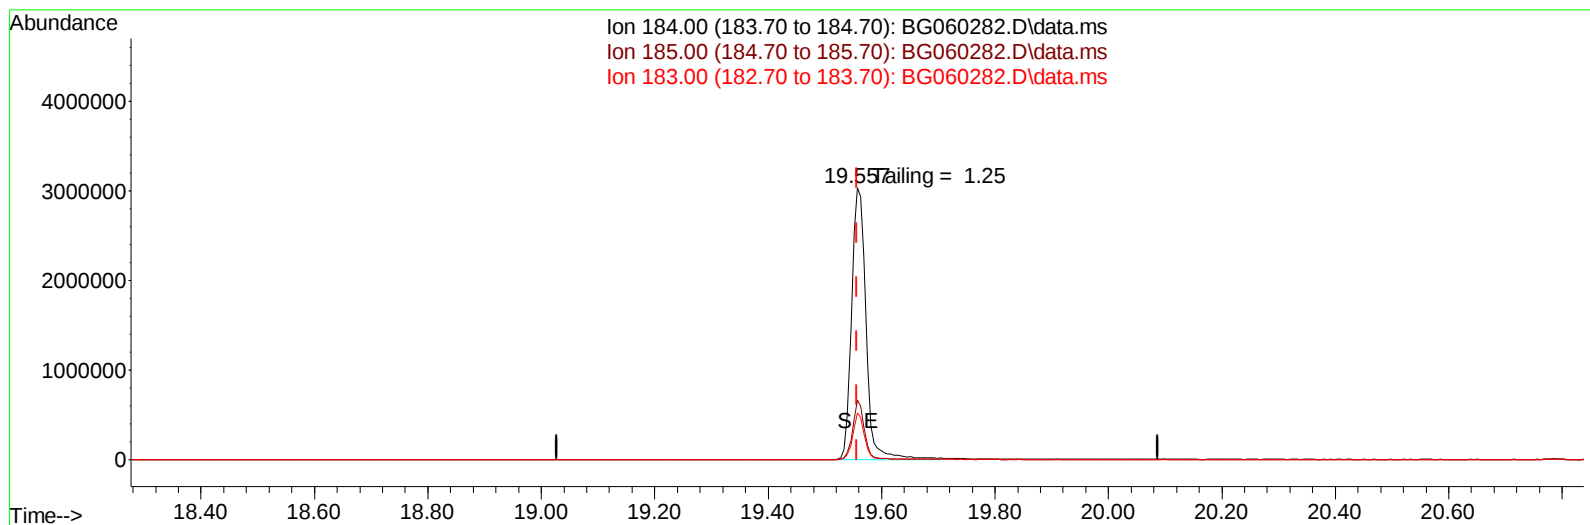

TIC: BG060282.D\data.ms

(77) Benzidine**19.557min (+ 0.000) 188944.20 ng****response 5389670**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	21.77#
183.00	11.20	17.10#
0.00	0.00	0.00