
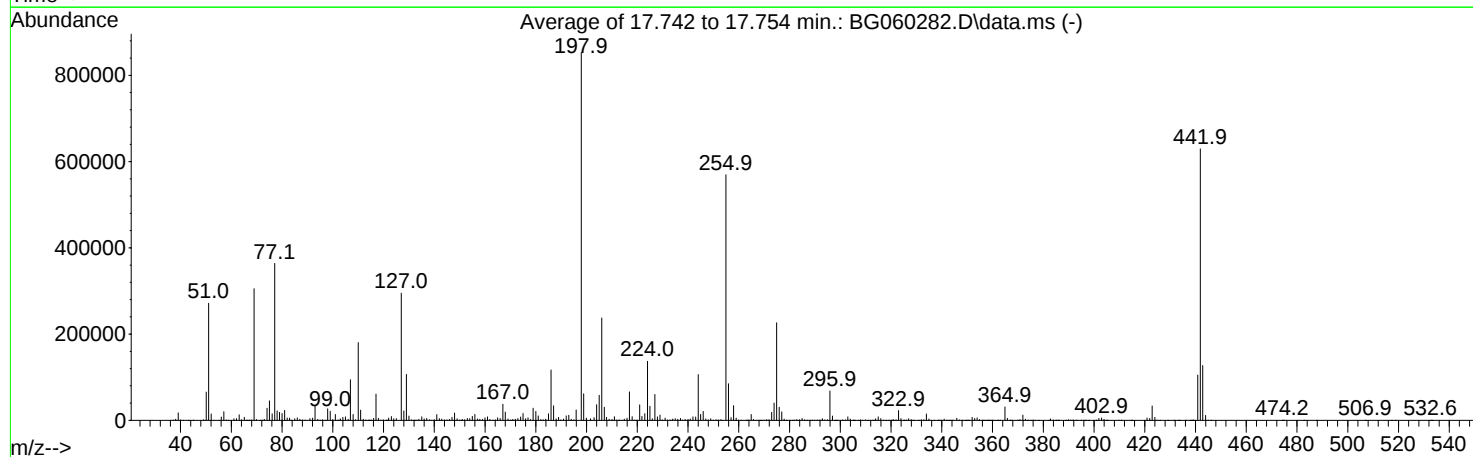


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010824\
Data File : BG060282.D
Acq On : 8 Jan 2024 15:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

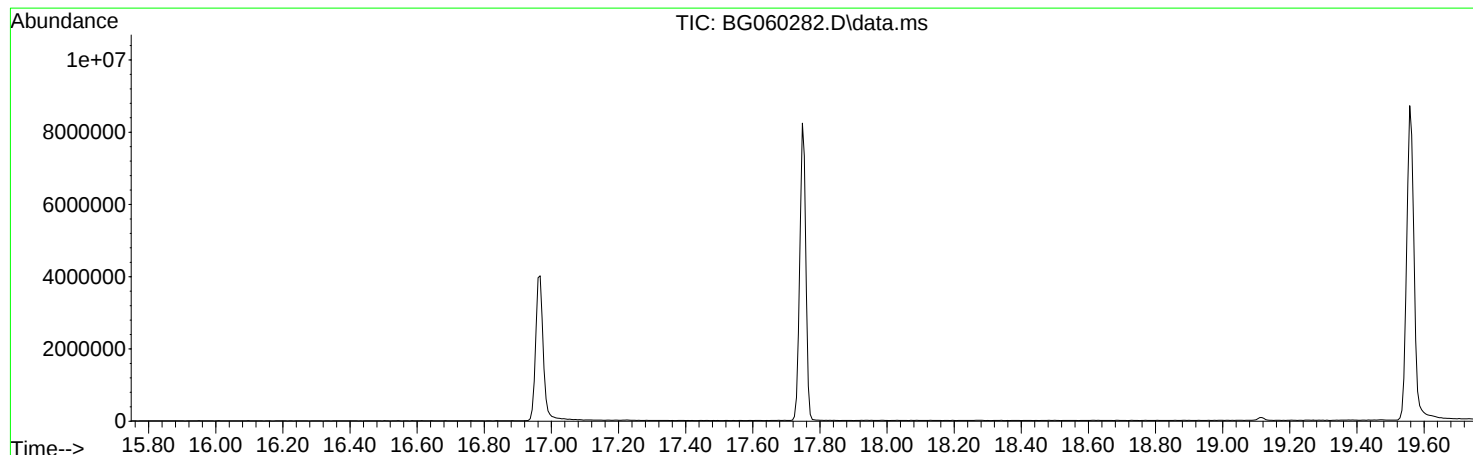




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	271703	PASS
68	69	0.00	2	0.4	1112	PASS
69	198	0.00	100	35.8	305294	PASS
70	69	0.00	2	0.6	1967	PASS
127	198	10	80	34.6	294784	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	852928	PASS
199	198	5	9	7.2	61733	PASS
275	198	10	60	26.5	226432	PASS
365	198	1	100	3.6	31011	PASS
441	198	0.01	100	12.3	104883	PASS
442	442	50	100	100.0	629611	PASS
443	442	15	24	20.2	127209	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010824\
Data File : BG060282.D
Acq On : 8 Jan 2024 15:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 09 04:13:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

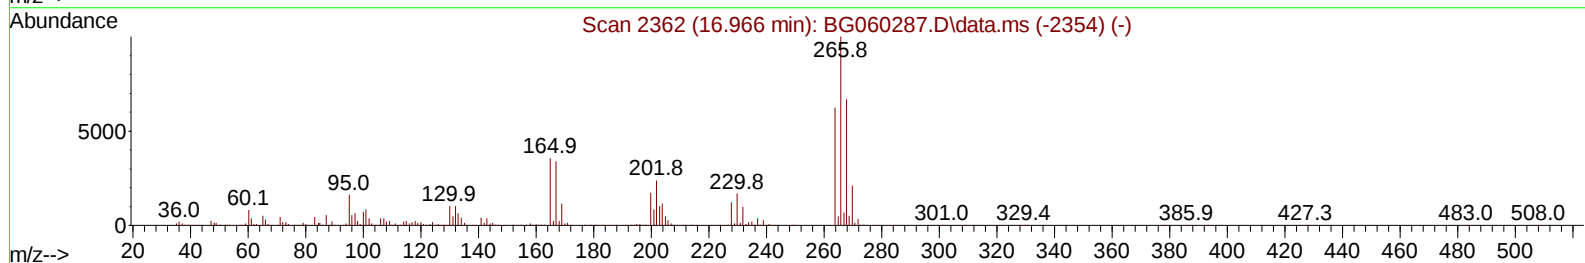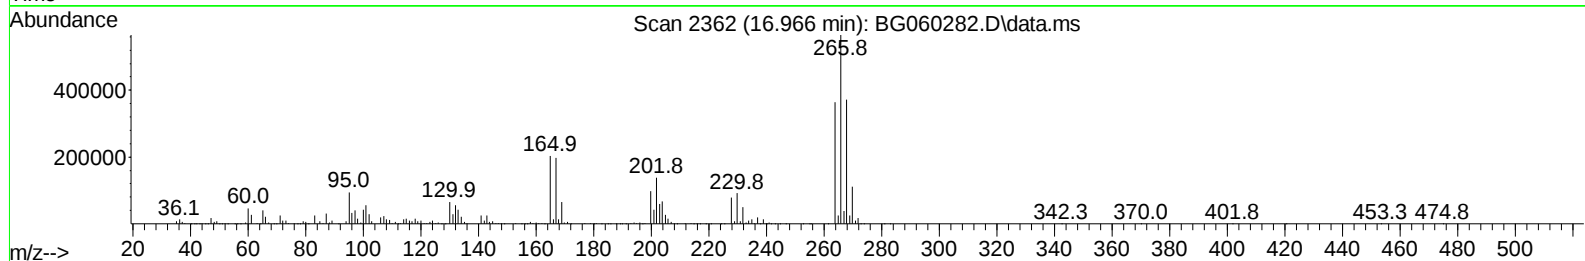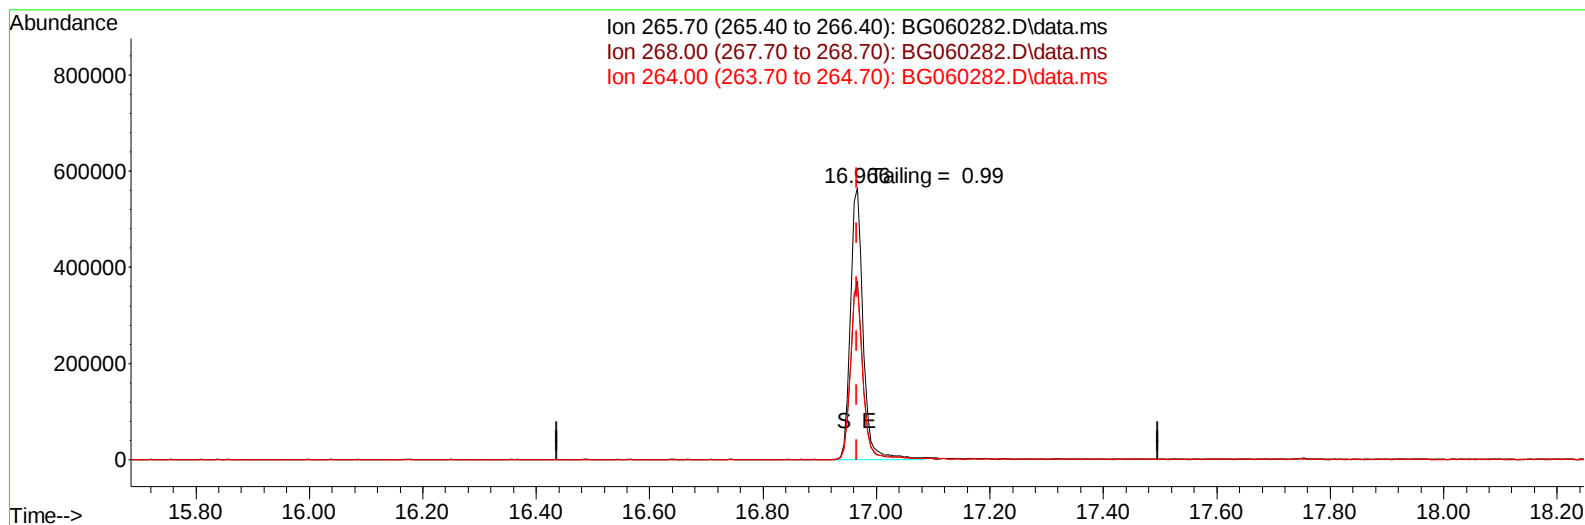

TIC: BG060282.D\data.ms

(70) Pentachlorophenol (C)

16.966min (+ 0.000) 122815.05 ng




response 885145

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	65.73
264.00	62.30	64.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010824\
Data File : BG060282.D
Acq On : 8 Jan 2024 15:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 09 04:13:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

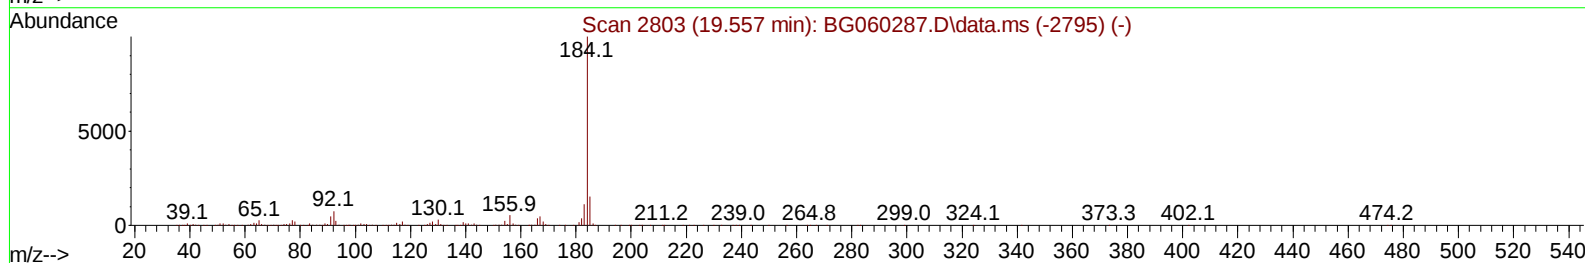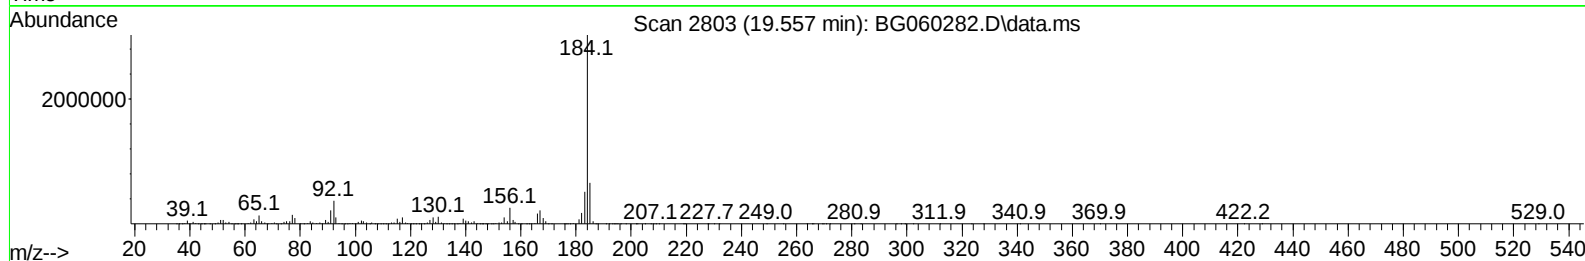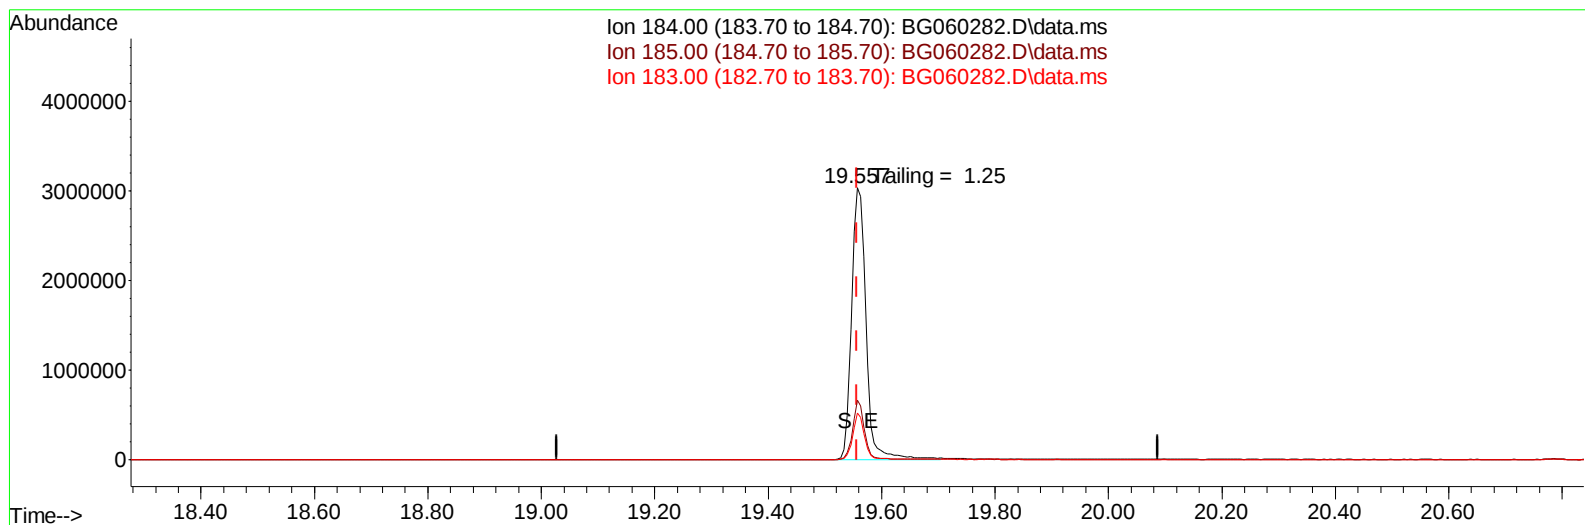

TIC: BG060282.D\data.ms

(77) Benzidine

19.557min (+ 0.000) 188944.20 ng

response 5389670

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	21.77#
183.00	11.20	17.10#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/8/2024	BNA_G	<u>BG060282.D</u>
Compound Name	Response	Retention Time
DDT	2730237	20.785
DDD	27787	20.398
DDE	0	19.843
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27787	2758024	1.01

Instrument :
BNA_G
ClientSampleId :
DFTPP