



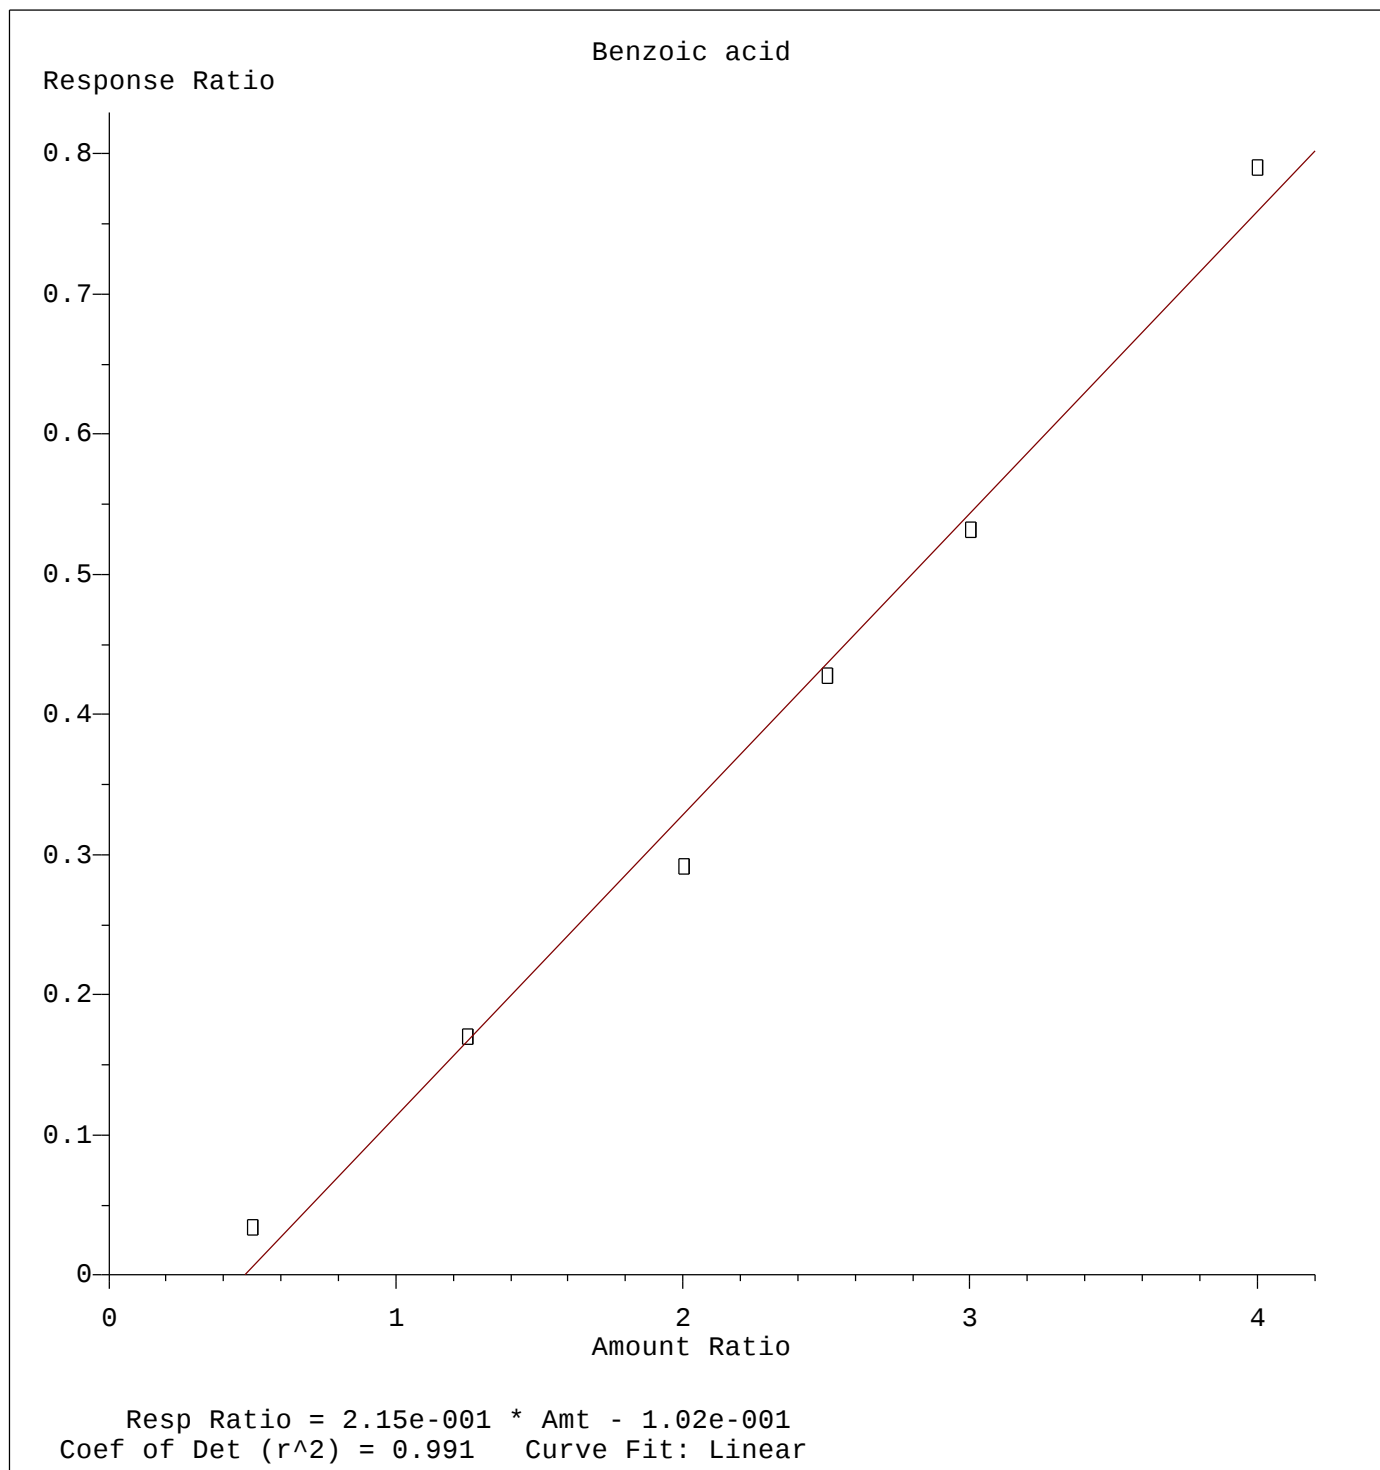

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Calibration Table Last Updated: Wed Jan 09 14:23:53 2019

Hexachlorocyclopentadiene

Response Ratio

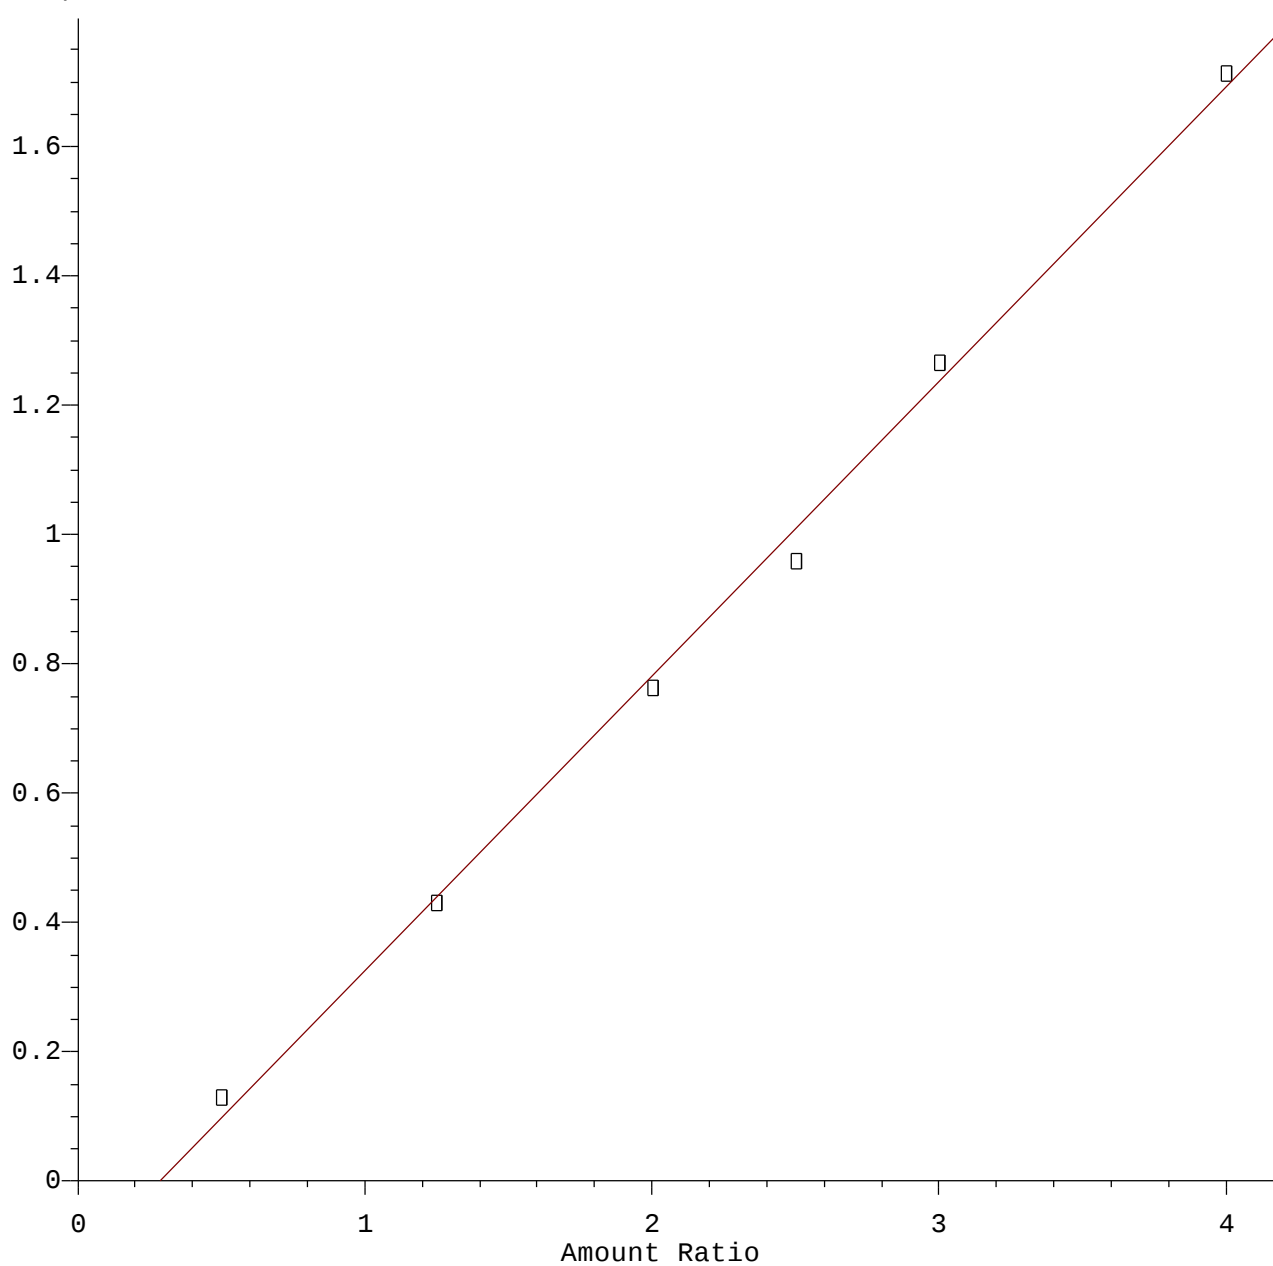


Resp Ratio = $4.56 \times 10^{-1} \times \text{Amt} - 1.31 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Calibration Table Last Updated: Wed Jan 09 14:23:53 2019


2,4-Dinitrophenol

Response Ratio

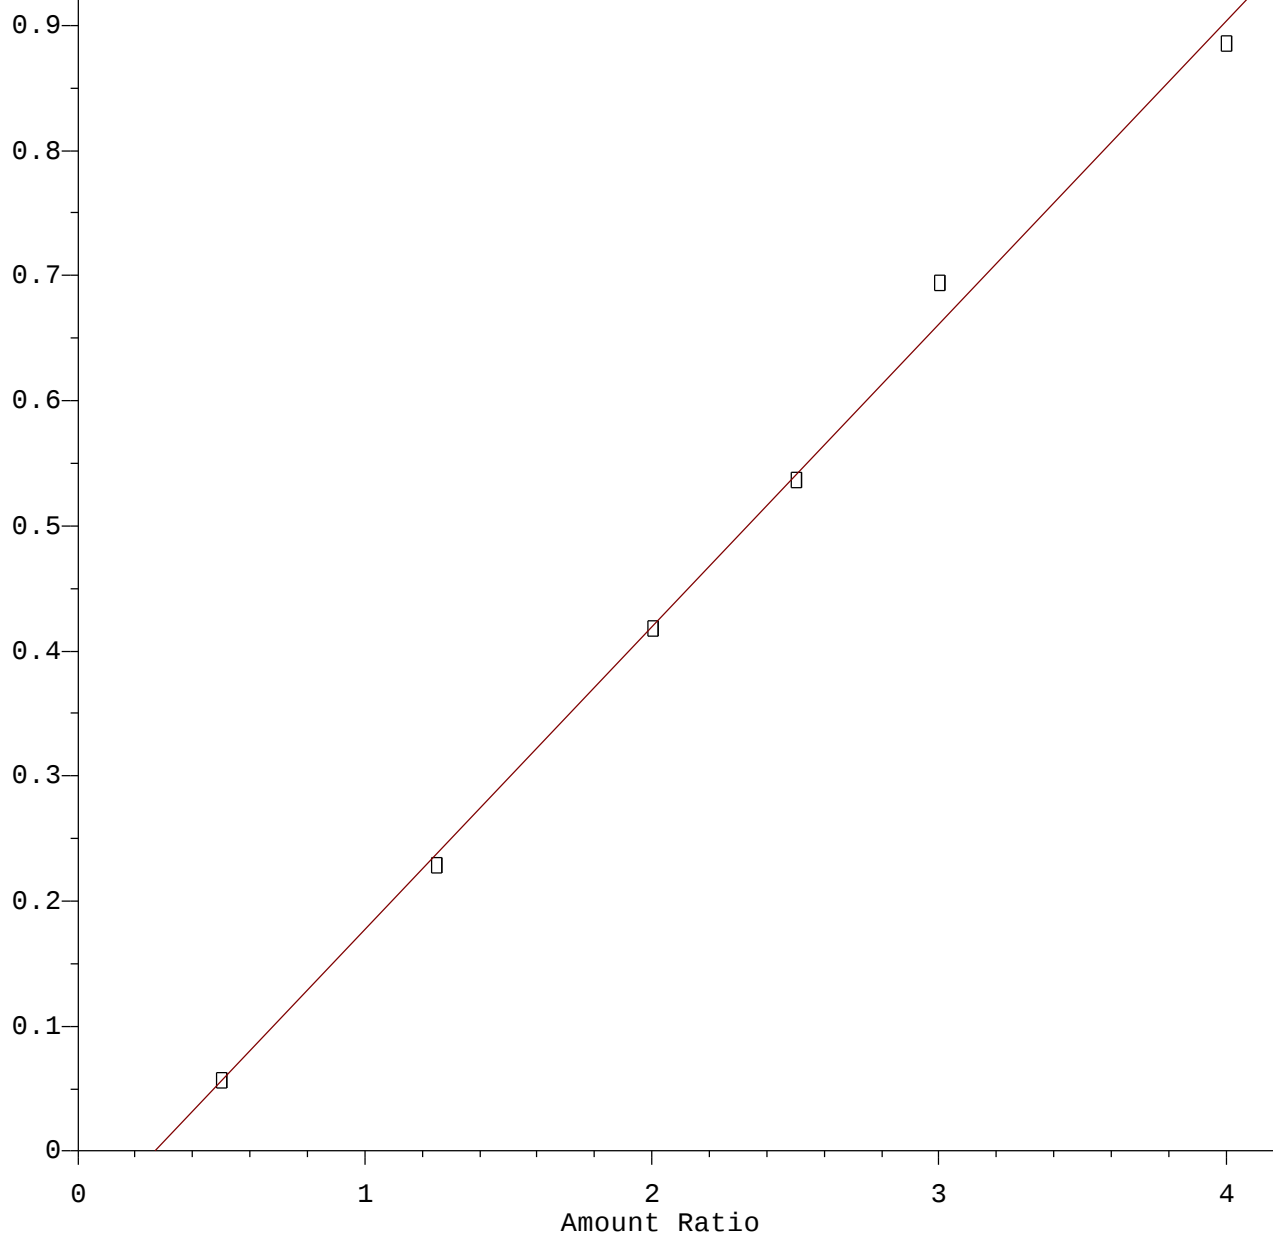

Resp Ratio = $2.42 \times 10^{-1} \times \text{Amt} - 6.52 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Calibration Table Last Updated: Wed Jan 09 14:23:53 2019

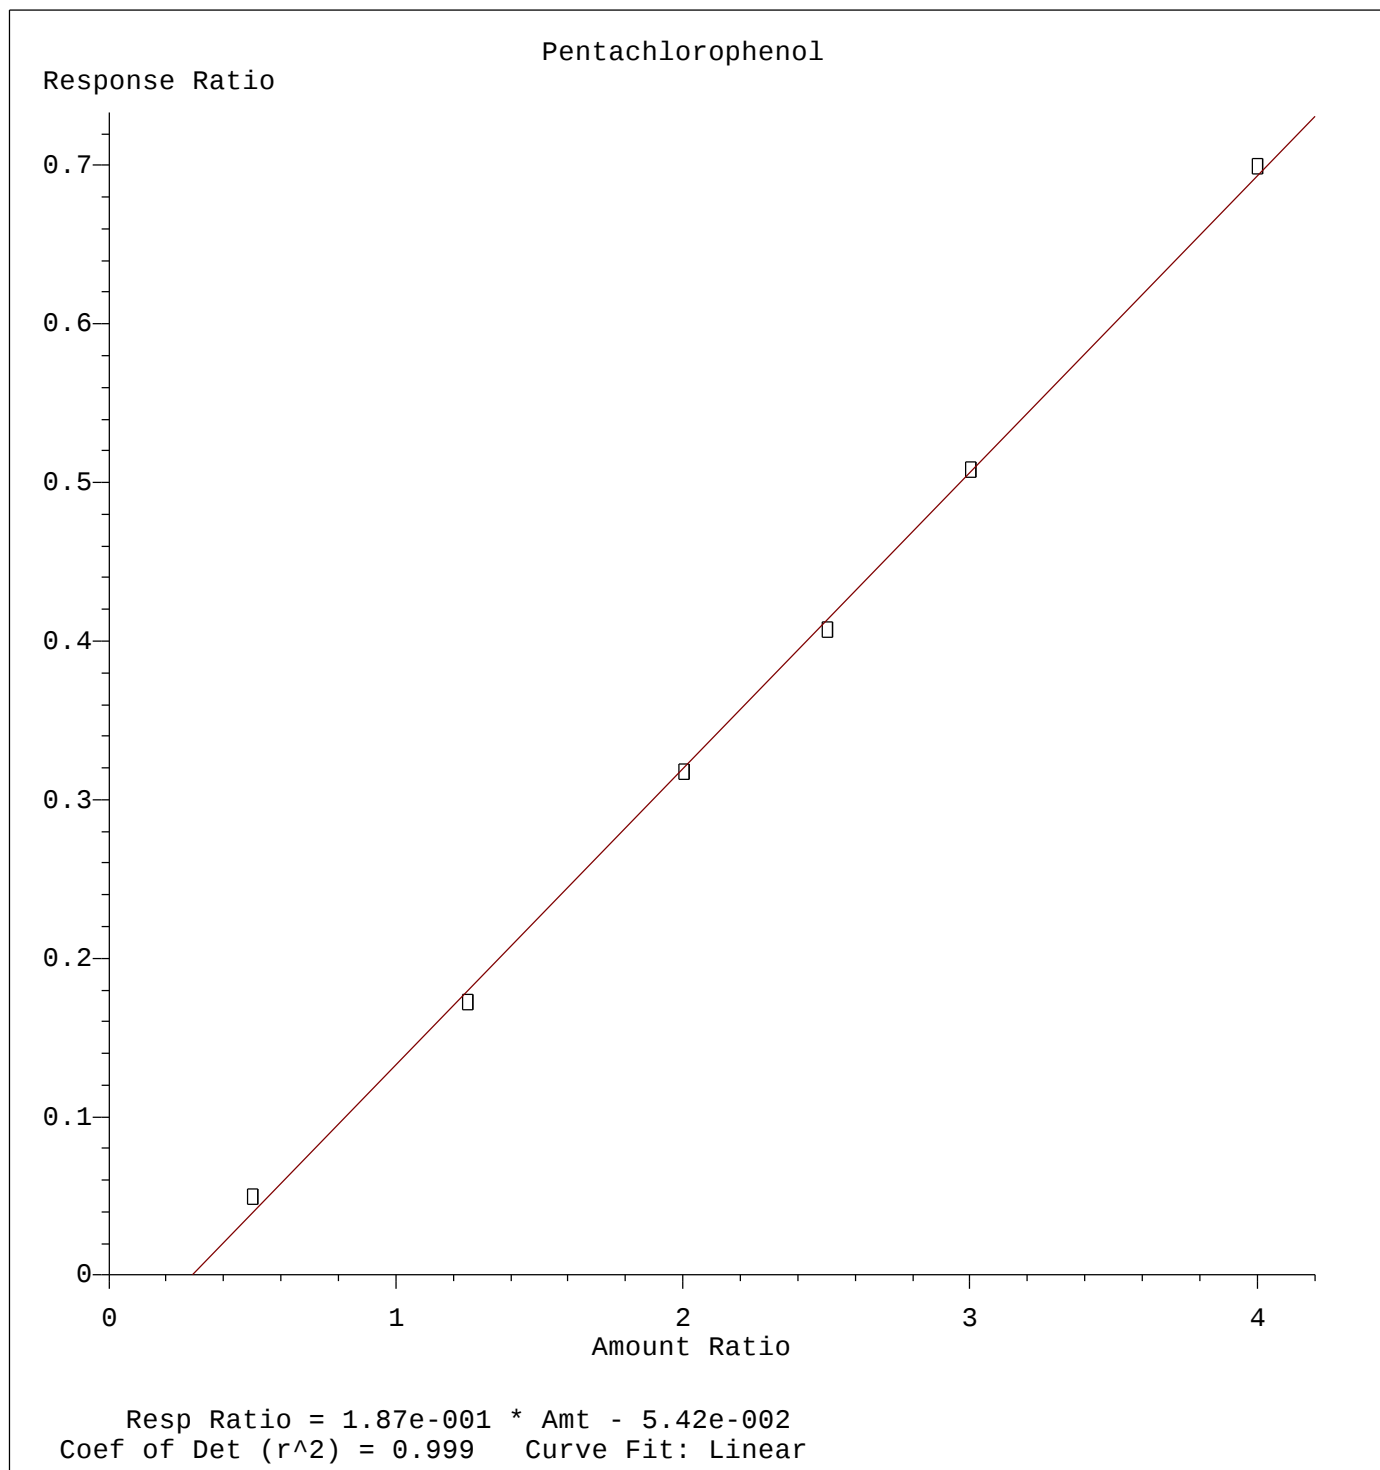

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Calibration Table Last Updated: Wed Jan 09 14:23:53 2019