
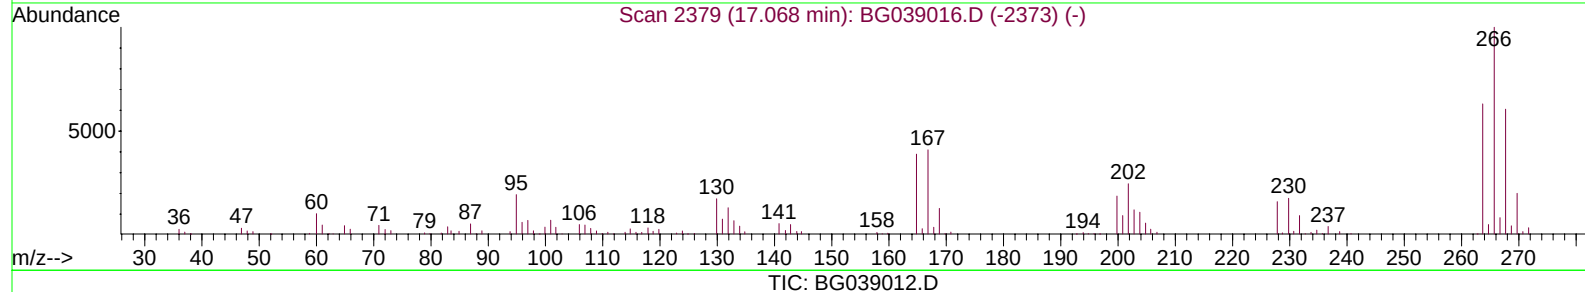
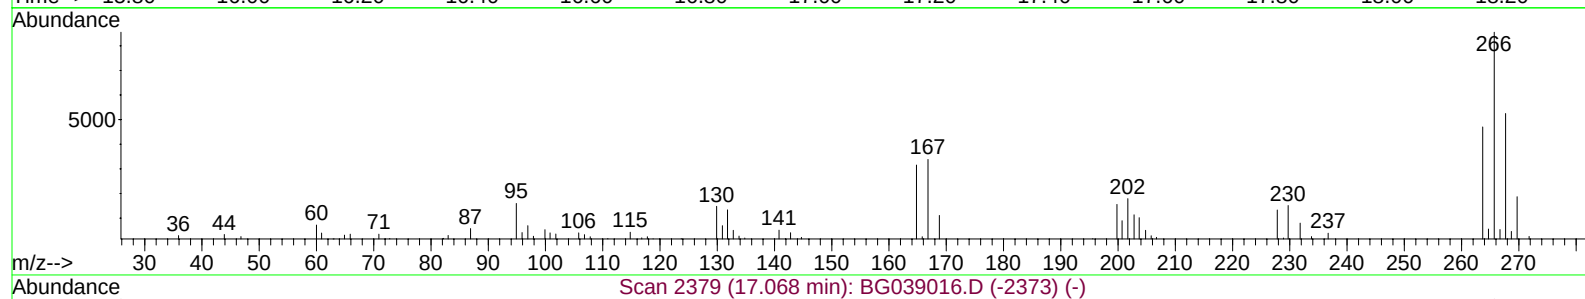


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010919\  
Data File : BG039012.D  
Acq On : 9 Jan 2019 9:03  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 16:06:47 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 09 14:23:53 2019  
Response via : Initial Calibration

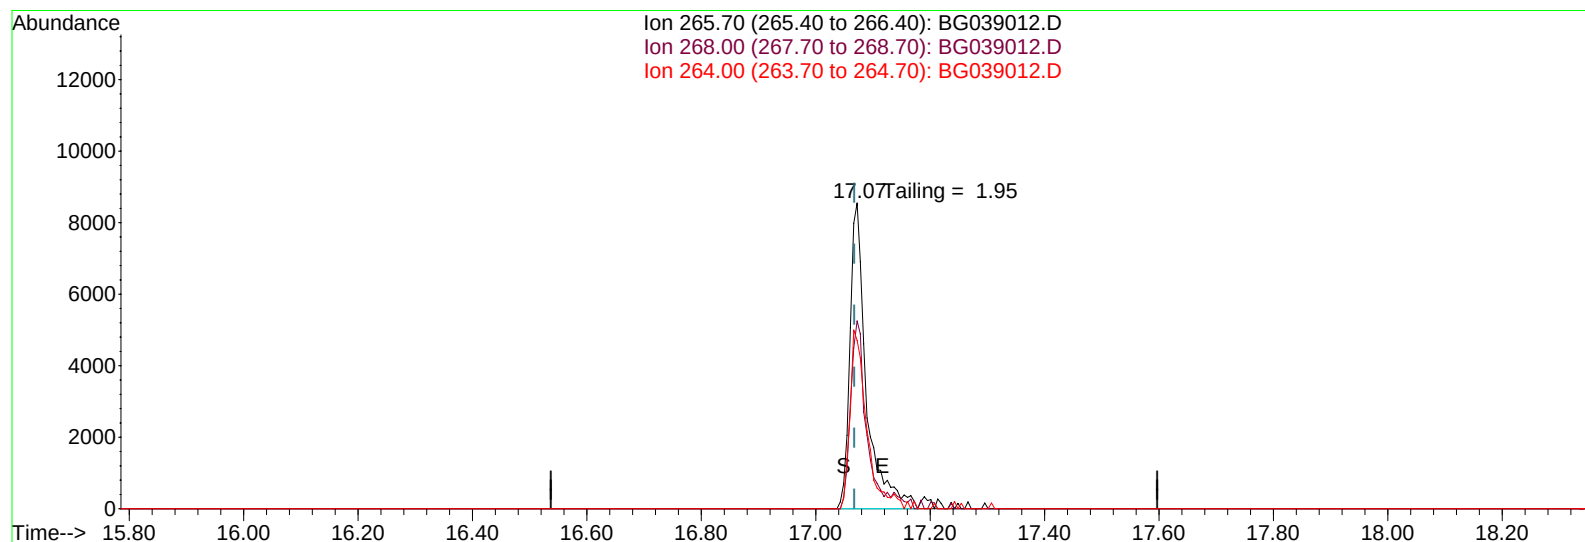

(70) Pentachlorophenol (C)




17.072min (+0.005) 32028.08ng

response 17354

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 66.78 |
| 264.00 | 68.20 | 61.53 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010919\  
 Data File : BG039012.D  
 Acq On : 9 Jan 2019 9:03  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 16:06:47 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jan 09 14:23:53 2019  
 Response via : Initial Calibration

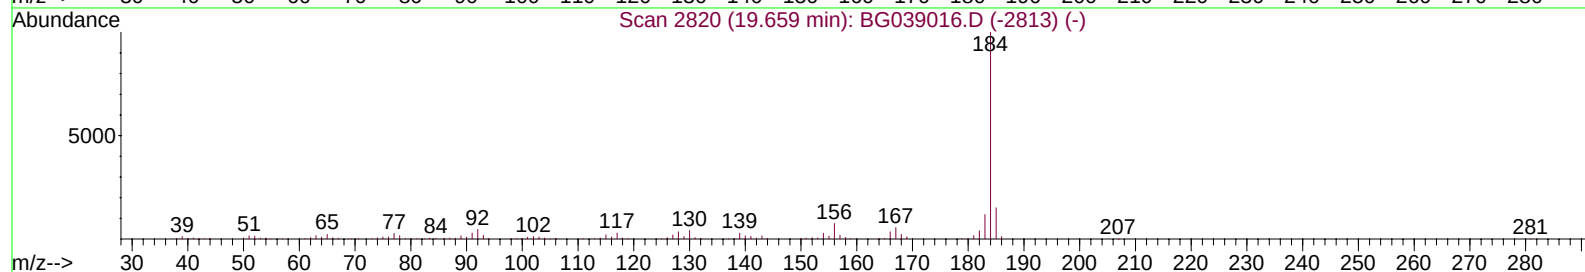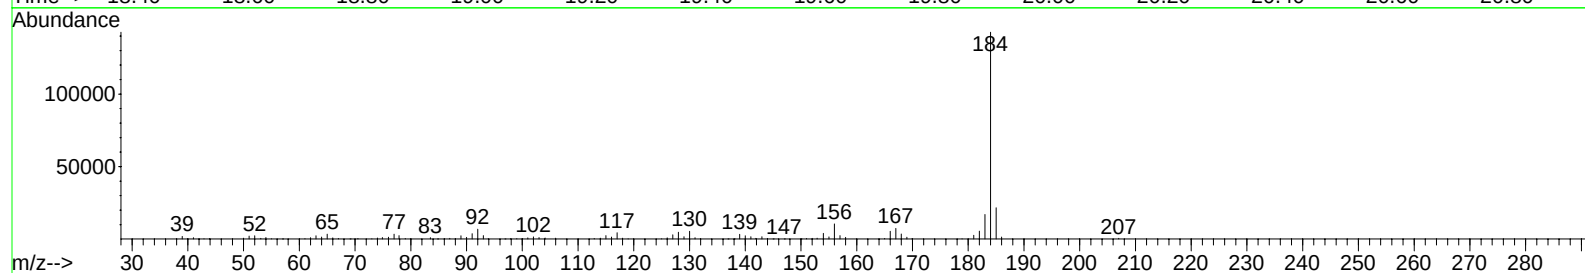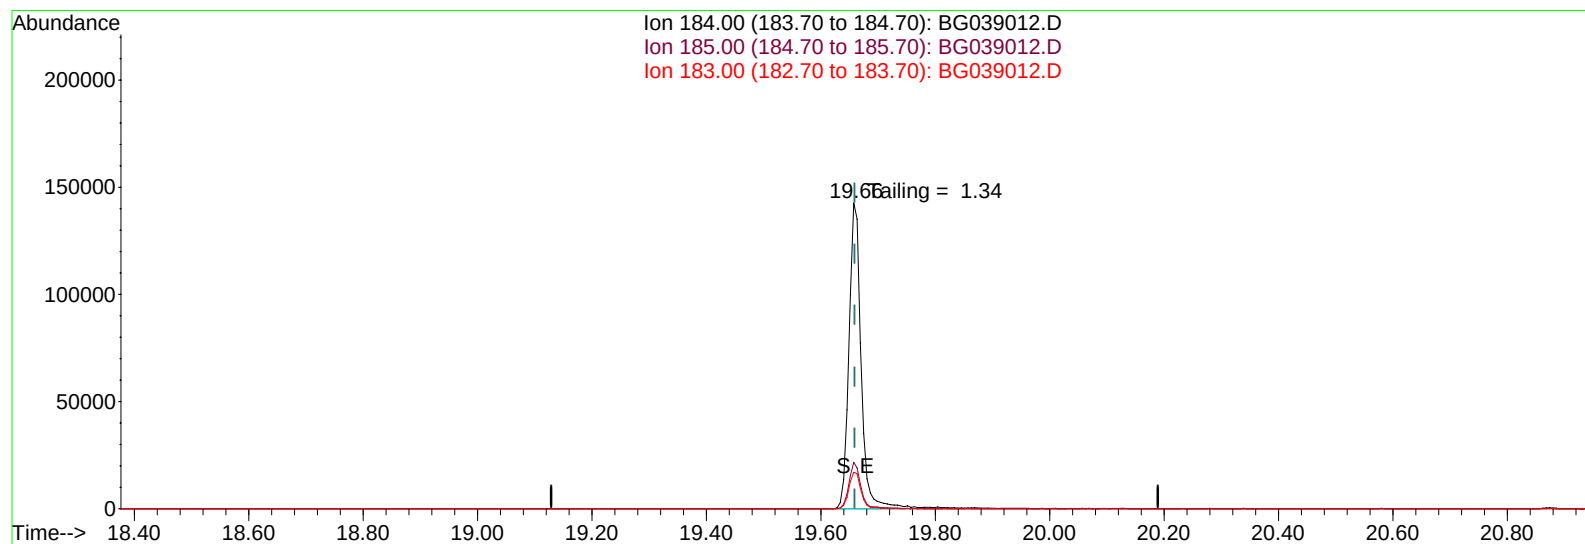

TIC: BG039012.D

(77) Benzidine

19.657min (-0.002) 0.00ng

response 212277

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.10 | 15.20 |
| 183.00 | 11.90 | 11.92 |
| 0.00   | 0.00  | 0.00  |