
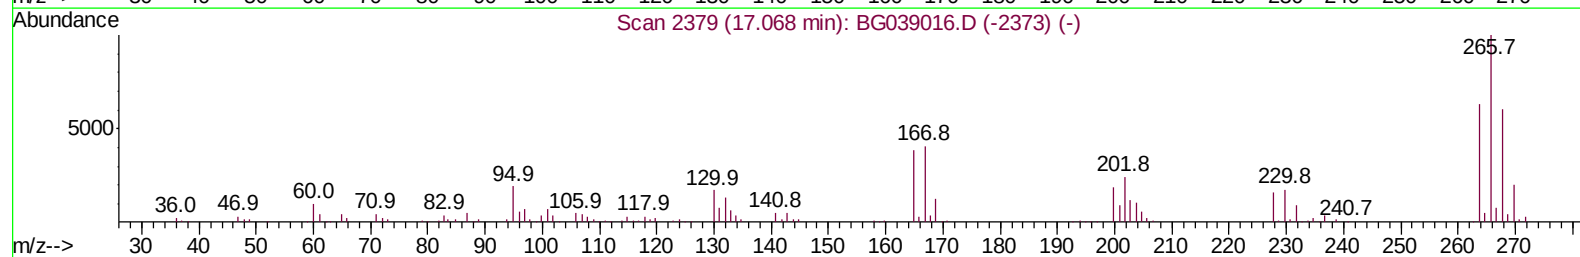
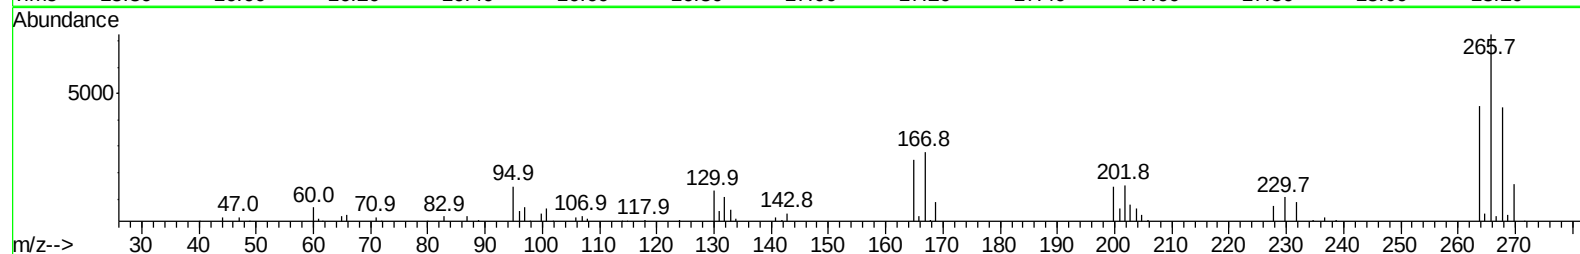


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010919\
Data File : BG039040.D
Acq On : 10 Jan 2019 4:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 08:16:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

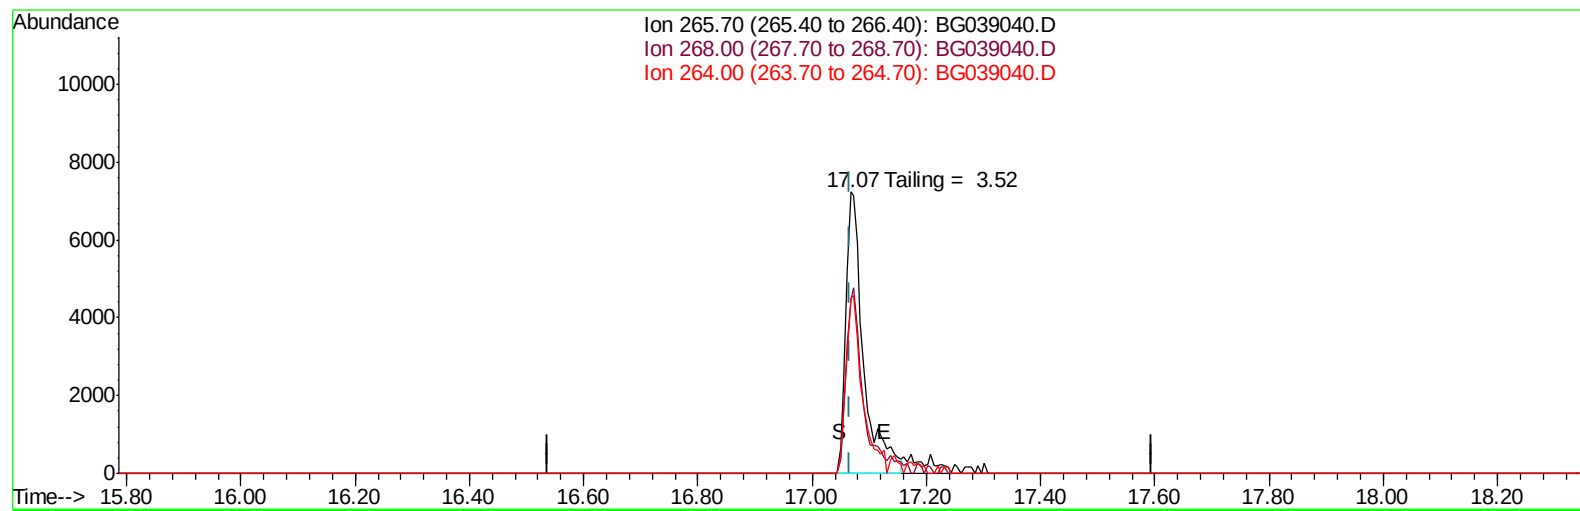

TIC: BG039040.D

(70) Pentachlorophenol (C)




17.067min (-0.000) 27340.04ng

response 15835

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	67.30
264.00	68.20	68.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010919\
Data File : BG039040.D
Acq On : 10 Jan 2019 4:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 08:16:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

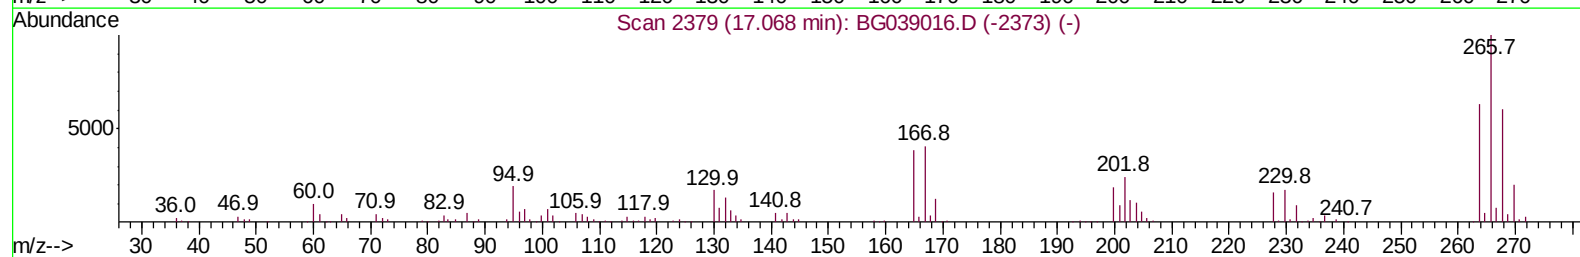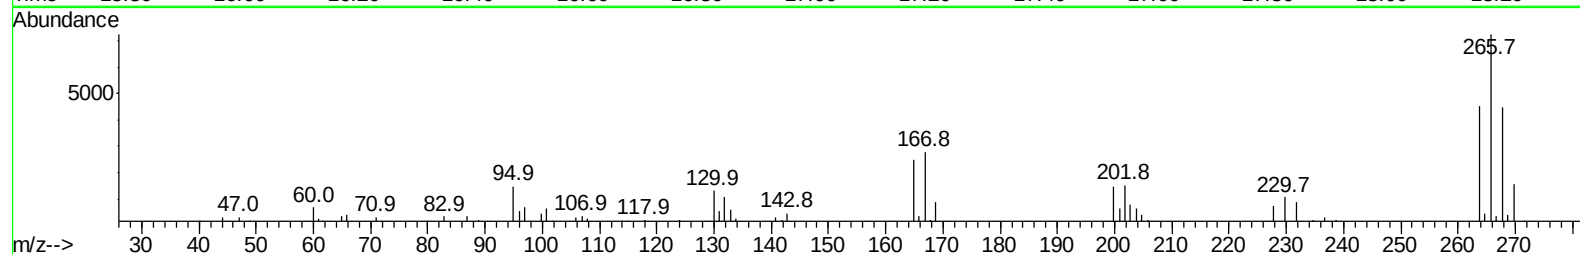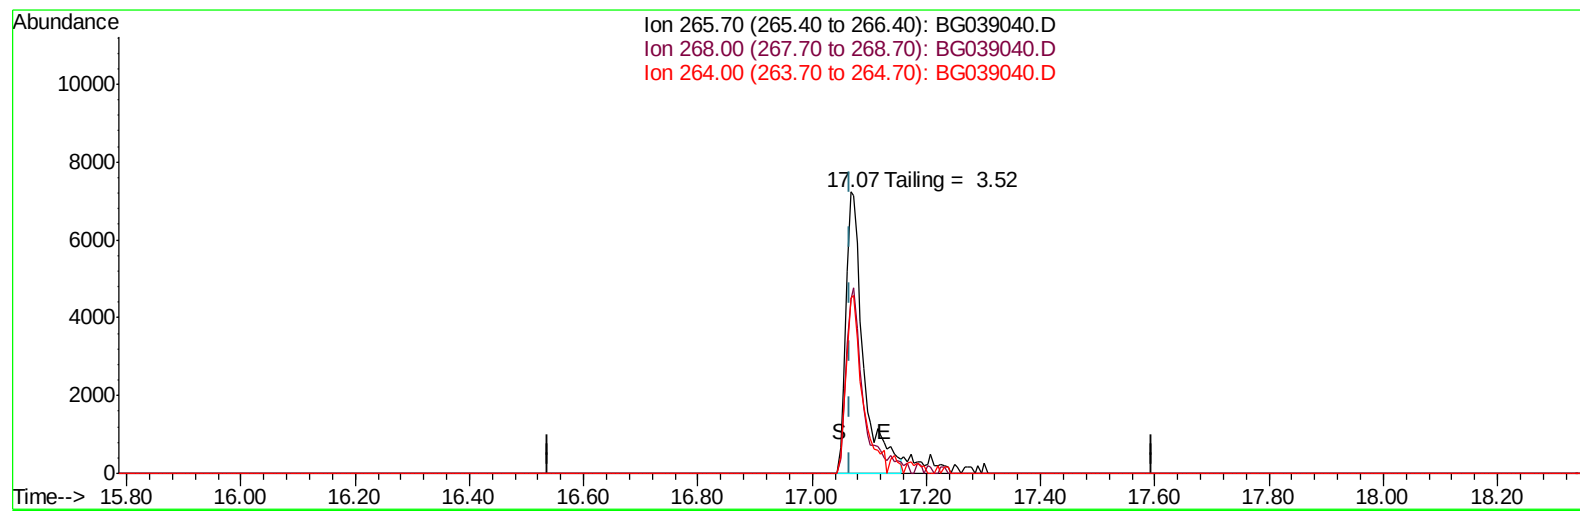

TIC: BG039040.D

(70) Pentachlorophenol (C)

17.067min (-0.000) 27340.04ng

response 15835

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	67.30
264.00	68.20	68.67
0.00	0.00	0.00