

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010919\
 Data File : BG039047.D
 Acq On : 10 Jan 2019 9:32
 Operator : JU/SJ
 Sample : K1006-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JC-03-010819-C

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.161	8	12	19	rVB	26839	38044	1.72%	0.416%
2	3.460	59	63	73	rVB	31218	44449	2.01%	0.486%
3	4.612	254	259	265	rBV	17104	23382	1.06%	0.256%
4	5.111	340	344	355	rVB	38592	61369	2.77%	0.671%
5	5.581	416	424	434	rBV	290877	481717	21.75%	5.264%
6	7.185	691	697	707	rBV	270181	476000	21.49%	5.202%
7	7.555	753	760	771	rVB	317582	575501	25.99%	6.289%
8	8.025	834	840	849	rBV	67820	112382	5.07%	1.228%
9	8.349	887	895	906	rVB	257015	464243	20.96%	5.073%
10	9.206	1033	1041	1054	rBV	217306	401534	18.13%	4.388%
11	10.846	1312	1320	1333	rBV	84741	162045	7.32%	1.771%
12	13.290	1729	1736	1747	rBV	667900	1083584	48.93%	11.841%
13	14.671	1965	1971	1979	rBV2	154407	253508	11.45%	2.770%
14	16.163	2218	2225	2239	rBV3	591351	945856	42.71%	10.336%
15	17.420	2431	2439	2449	rBV2	242690	378578	17.09%	4.137%
16	19.124	2724	2729	2744	rBV	264883	364400	16.45%	3.982%
17	19.894	2853	2860	2866	rBV2	28890	38895	1.76%	0.425%
18	20.023	2876	2882	2892	rBV	1670743	2214696	100.00%	24.201%
19	20.440	2949	2953	2958	rVB2	37742	43315	1.96%	0.473%
20	20.957	3037	3041	3046	rVB	17530	22517	1.02%	0.246%
21	21.504	3129	3134	3139	rBV3	15722	23499	1.06%	0.257%
22	21.698	3160	3167	3175	rVB2	282086	467945	21.13%	5.114%
23	24.976	3715	3725	3742	rVB	162387	473671	21.39%	5.176%


Sum of corrected areas: 9151130

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010919\
Data File : BG039047.D
Acq On : 10 Jan 2019 9:32
Operator : JU/SJ
Sample : K1006-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JC-03-010819-C

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

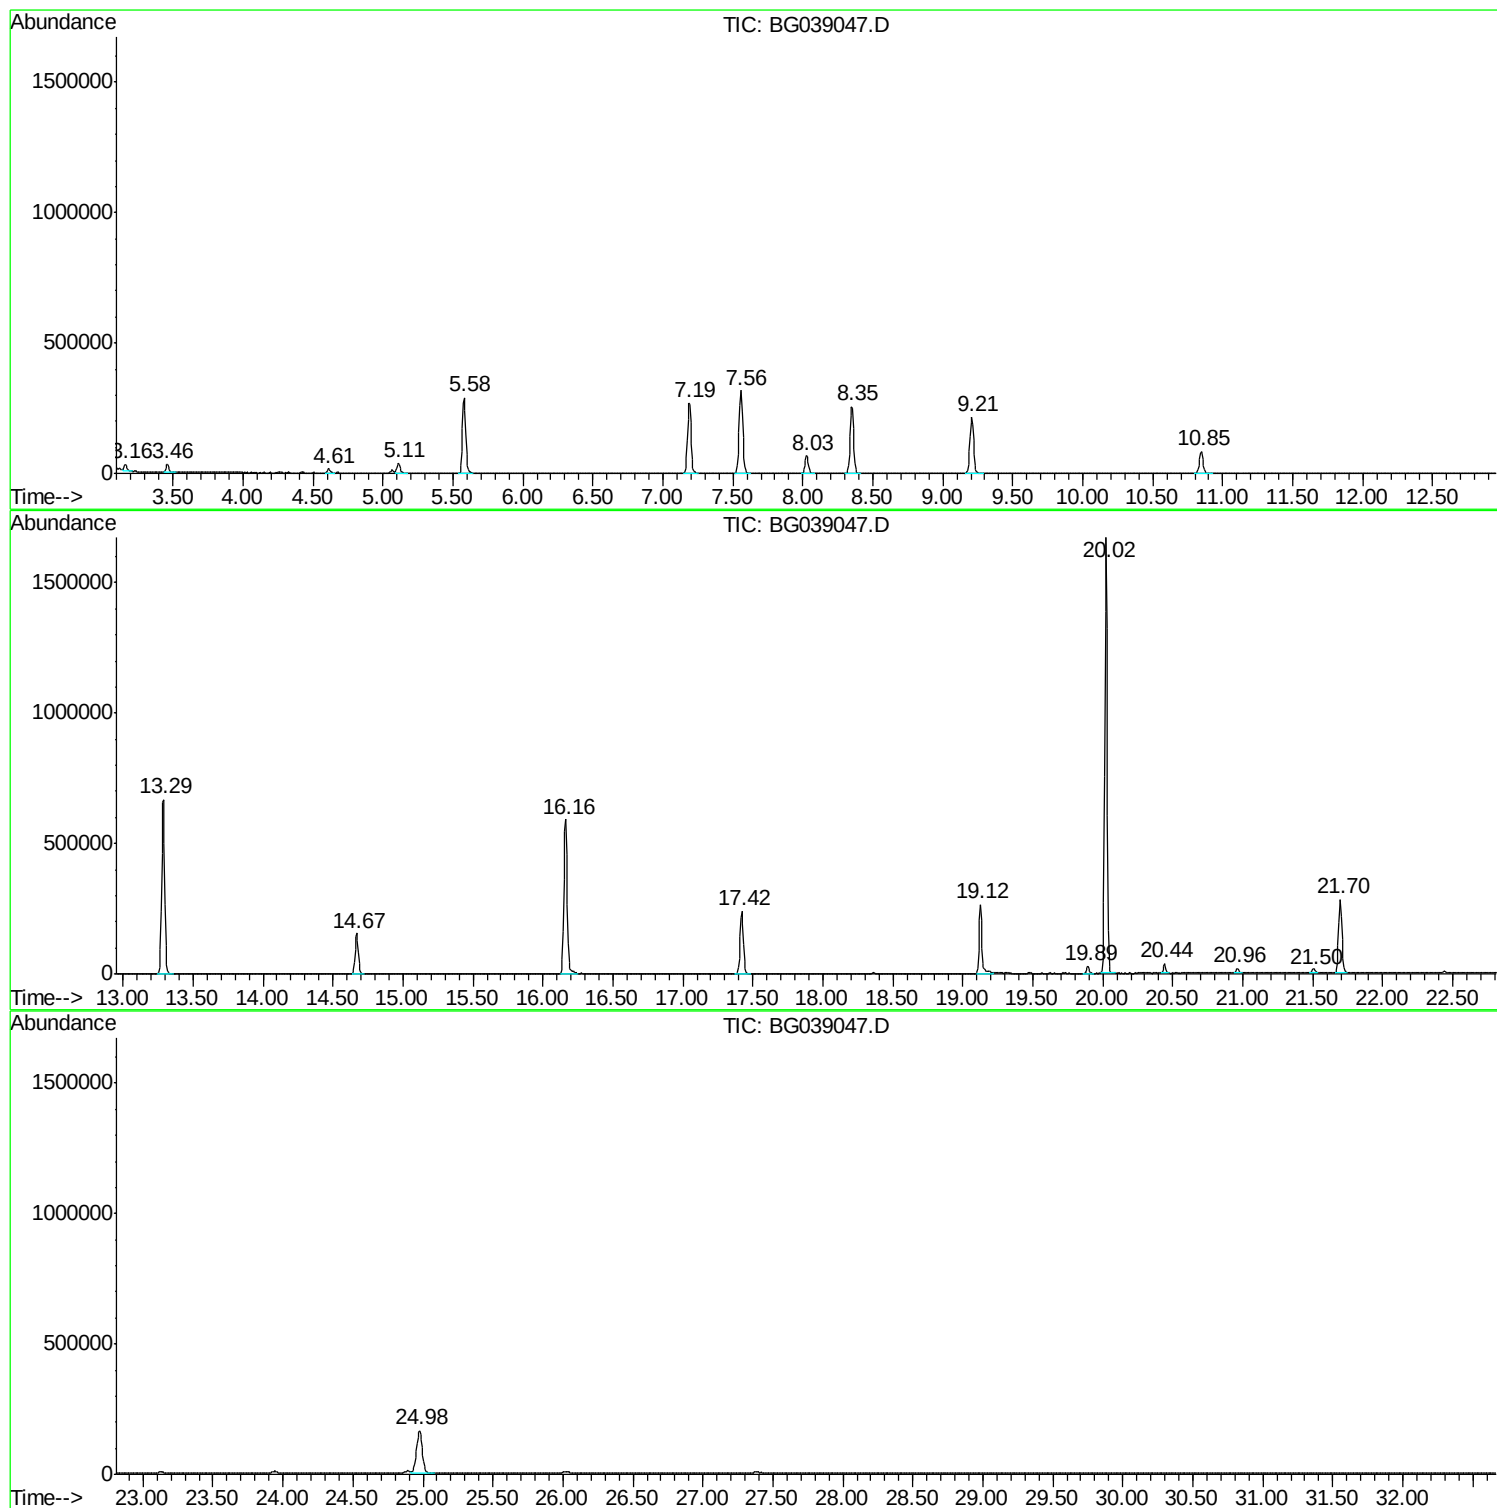

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010919\
Data_File : BG039047.D
Acq_On : 10 Jan 2019 9:322
Operator : JU/SJJ
Sample : K1006-066
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
JC-03-010819-C

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
