

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010919\
 Data File : BG039048.D
 Acq On : 10 Jan 2019 10:11
 Operator : JU/SJ
 Sample : K1006-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JC-03-010819-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.161	7	12	22	rVB	32368	53597	2.12%	0.584%
2	3.461	58	63	69	rVB	25406	34782	1.37%	0.379%
3	5.112	339	344	353	rVB	45633	71751	2.83%	0.782%
4	5.582	417	424	436	rBV	310683	524373	20.71%	5.713%
5	7.186	690	697	709	rBV	304248	545717	21.56%	5.946%
6	7.556	751	760	769	rBV	351902	612444	24.19%	6.673%
7	8.026	832	840	846	rBV	62109	106539	4.21%	1.161%
8	8.349	888	895	904	rVB	242252	423147	16.71%	4.610%
9	9.207	1034	1041	1050	rBV	219998	403149	15.92%	4.392%
10	10.847	1313	1320	1329	rBV	81976	152647	6.03%	1.663%
11	13.291	1728	1736	1746	rBV	642709	1044366	41.25%	11.379%
12	14.671	1963	1971	1979	rBV2	147600	253703	10.02%	2.764%
13	16.164	2218	2225	2238	rBV	672037	1074898	42.46%	11.711%
14	17.421	2432	2439	2447	rBV2	241990	381702	15.08%	4.159%
15	20.024	2875	2882	2892	rBV	1917574	2531674	100.00%	27.583%
16	21.693	3159	3166	3176	rBV	293469	490646	19.38%	5.346%
17	24.971	3714	3724	3735	rVB2	162417	473110	18.69%	5.155%


Sum of corrected areas: 9178245

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010919\
Data File : BG039048.D
Acq On : 10 Jan 2019 10:11
Operator : JU/SJ
Sample : K1006-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JC-03-010819-D

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

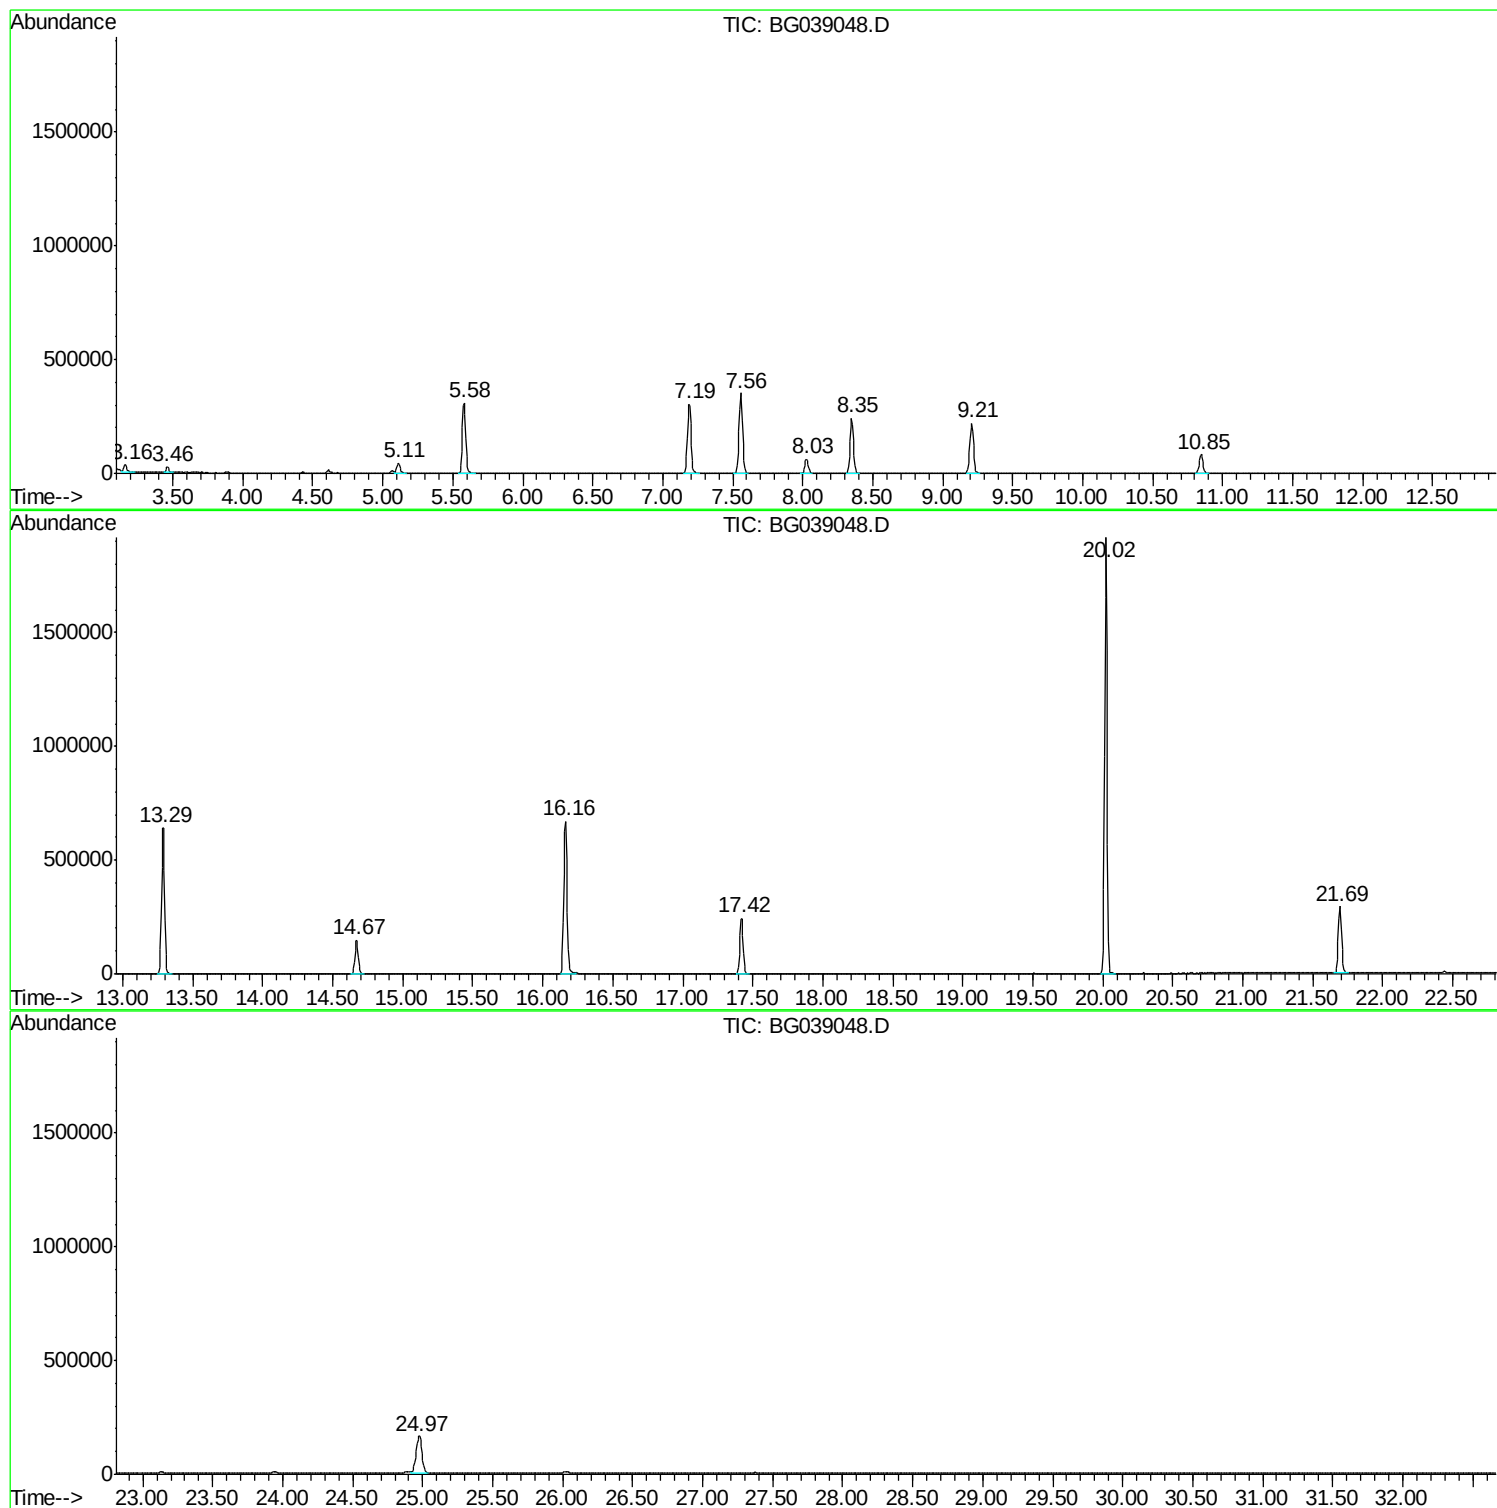

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010919\
Data_File : BG039048.D
Acq_On : 10 Jan 2019 10:111
Operator : JU/SJJ
Sample : K1006-088
Misc :
ALS_Vial : 26 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
JC-03-010819-D

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
