


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010919\
 Data File : BG039021.D
 Acq On : 9 Jan 2019 15:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 09 14:23:53 2019

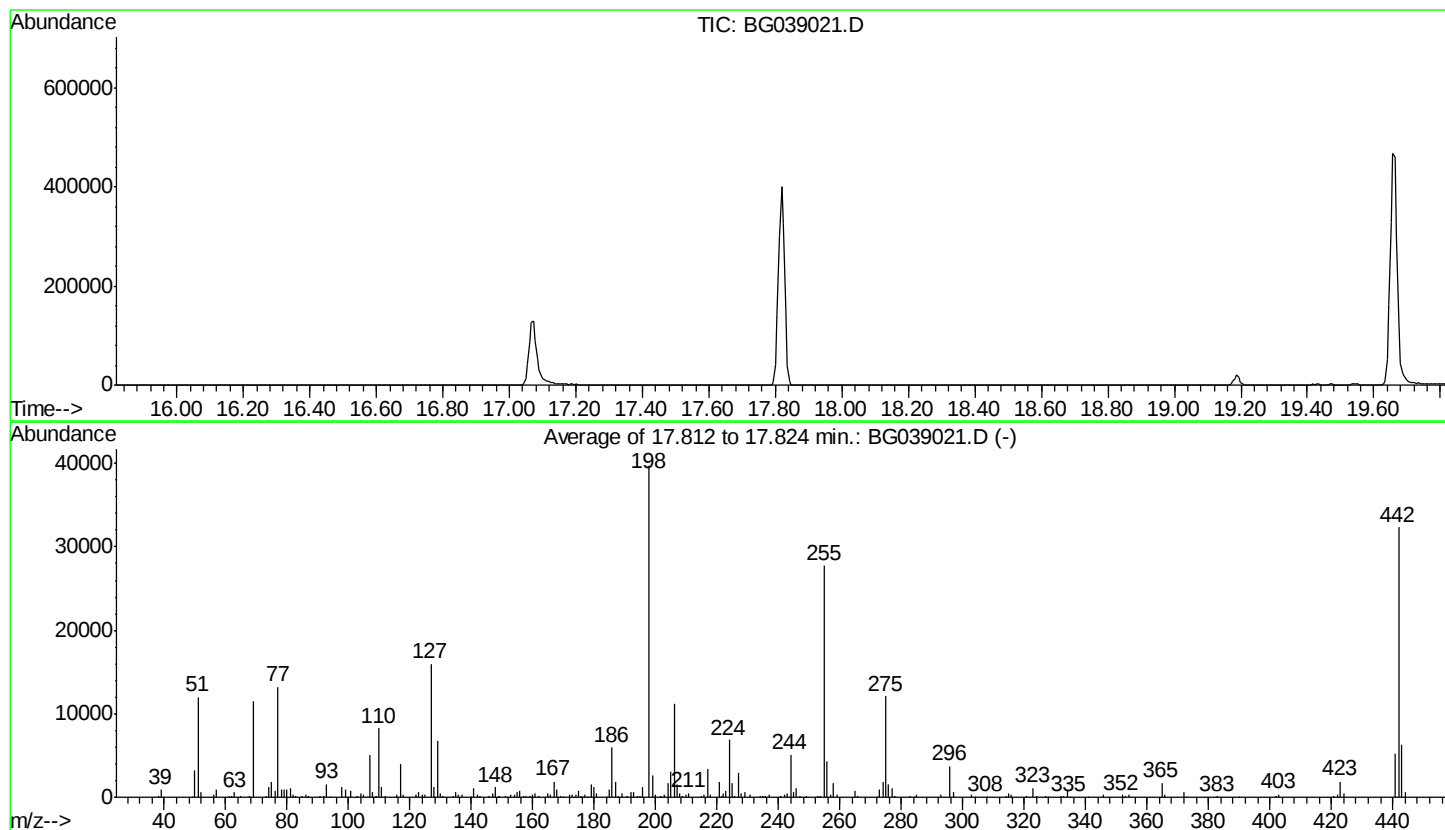

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	12015	PASS
68	69	0.00	2	0.9	108	PASS
69	198	0.00	100	29.0	11506	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.3	16006	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39736	PASS
199	198	5	9	6.7	2678	PASS
275	198	10	60	30.3	12052	PASS
365	198	1	100	4.3	1691	PASS
441	198	0.01	100	13.2	5246	PASS
442	198	50	100	81.4	32352	PASS
443	442	15	24	19.5	6317	PASS