

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011019\
 Data File : BG039067.D
 Acq On : 11 Jan 2019 00:33
 Operator : JU/SJ
 Sample : K1005-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jan 11 05:12:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 09 14:23:53 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	21918	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	91312	20.00	ng	0.00
39) Acenaphthene-d10	14.67	164	67569	20.00	ng	0.00
64) Phenanthrene-d10	17.42	188	177517	20.00	ng	0.00
76) Chrysene-d12	21.69	240	183573	20.00	ng	-0.01
87) Perylene-d12	24.98	264	194078	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.58	112	149568	129.45	ng	0.00
7) Phenol-d6	7.19	99	187364	112.68	ng	0.00
23) Nitrobenzene-d5	9.21	82	144193	86.41	ng	0.00
42) 2,4,6-Tribromophenol	16.16	330	152357	134.51	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	422660	85.61	ng	0.00
79) Terphenyl-d14	20.02	244	823295	82.96	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.21	70	19115	17.506	ng	# 67
51) 2,6-Dinitrotoluene	14.67	165	8262	6.472	ng	# 24
57) 2,4-Dinitrotoluene	14.67	165	8262	4.511	ng	# 26
67) 4-Bromophenyl-phenylether	16.16	248	10086	4.420	ng	# 1
77) Benzidine	20.02	184	12498	2.226	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011019\
Data File : BG039067.D
Acq On : 11 Jan 2019 00:33
Operator : JU/SJ
Sample : K1005-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jan 11 05:12:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

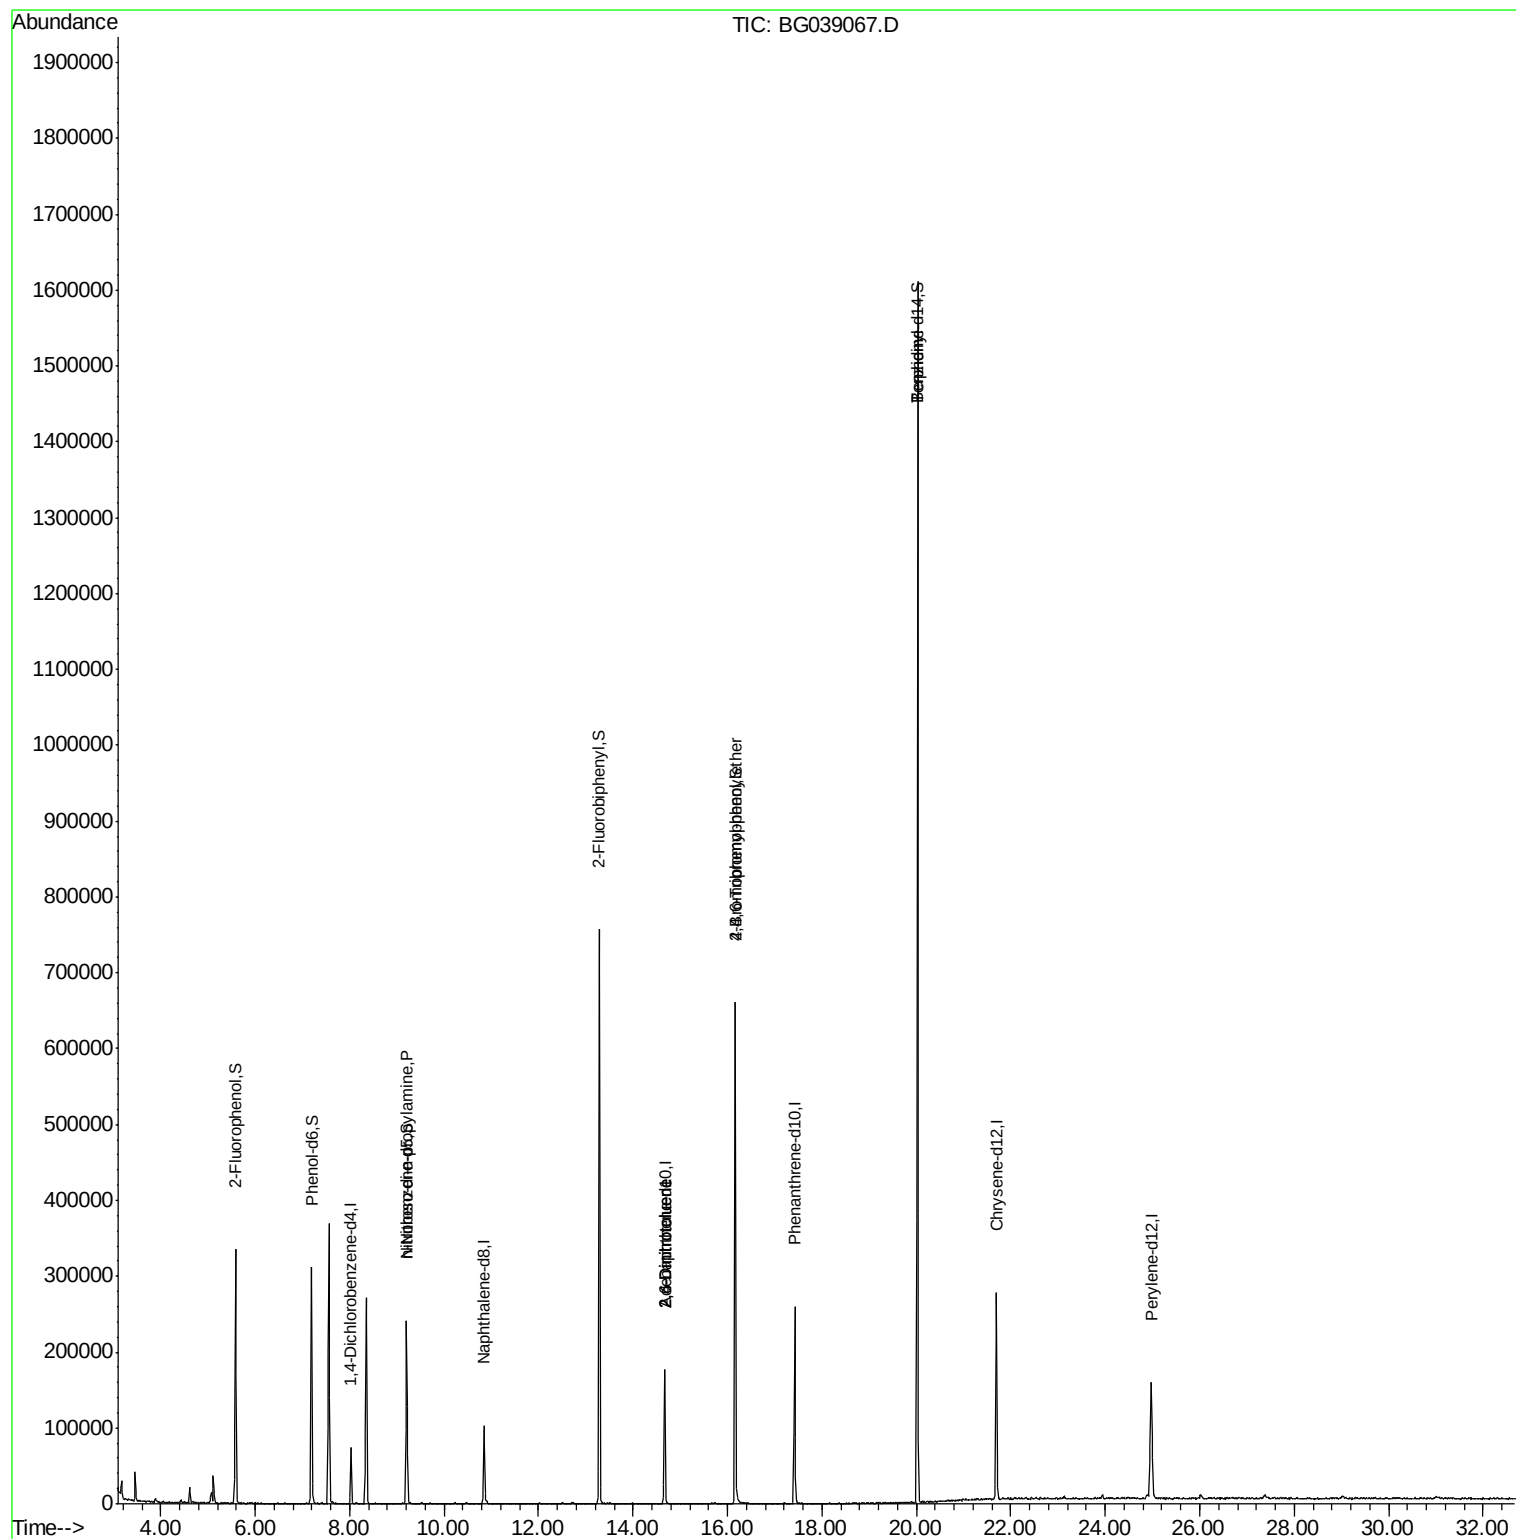




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.03 min Scan# 840
Delta R.T. -0.01 min
Lab File: BG039067.D
Acq: 11 Jan 2019 00:33

Instrument :
BNA_G
ClientSampled :

Tot Ion:152 Resp: 21918
Ion Ratio Lower Upper
152 100
150 154.2 124.7 187.1
115 53.8 46.5 69.7

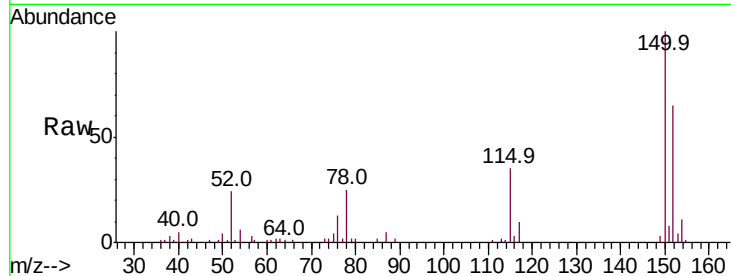


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

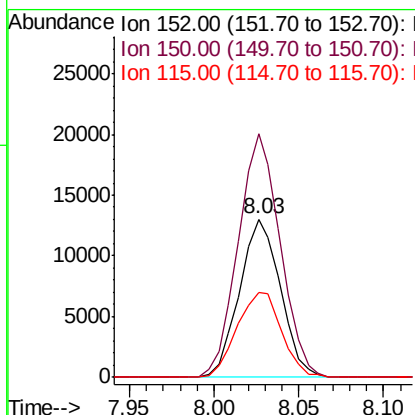



#5


2-Fluorophenol
Concen: 129.450 ng
RT: 5.58 min Scan# 424
Delta R.T. 0.00 min
Lab File: BG039067.D
Acq: 11 Jan 2019 00:33

Tgt Ion:112 Resp: 149568
Ion Ratio Lower Upper
112 100
64 60.9 47.0 70.6
63 36.0 28.0 42.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

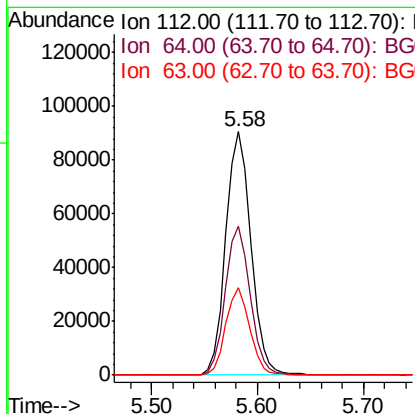

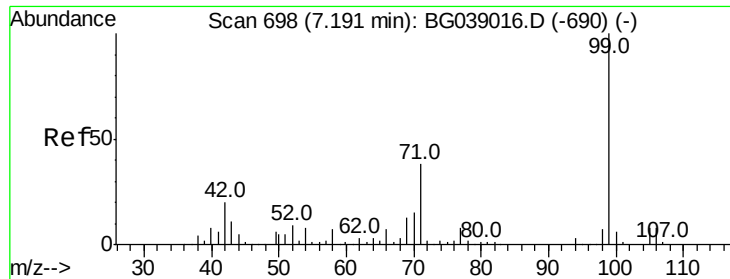

#7

Phenol-d6

Concen: 112.680 ng

RT: 7.19 min Scan# 698

Delta R.T. 0.00 min

Lab File: BG039067.D

Acq: 11 Jan 2019 00:33

Instrument :

BNA_G

ClientSampled :


Tot Ion: 99 Resp: 187364

Ion Ratio Lower Upper




99 100

42 20.0 15.8 23.6

71 36.5 30.2 45.4

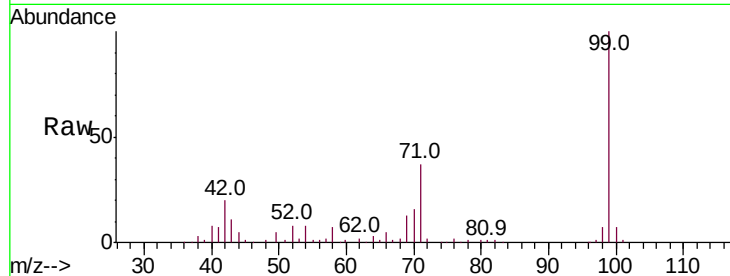

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

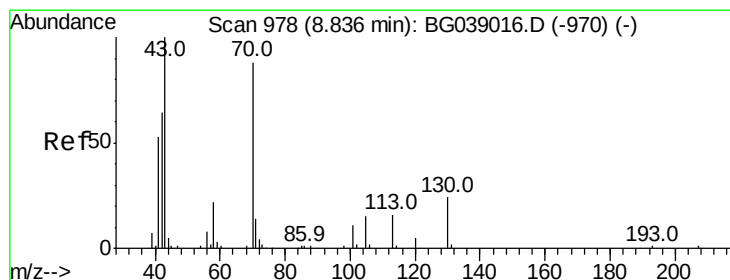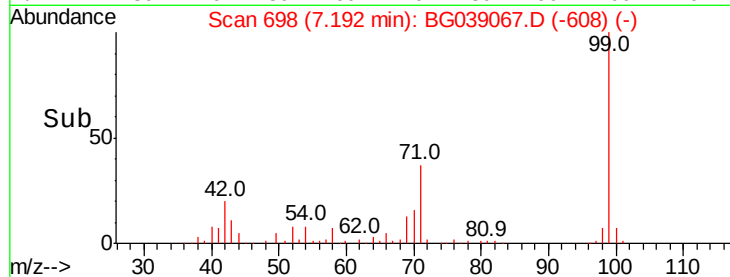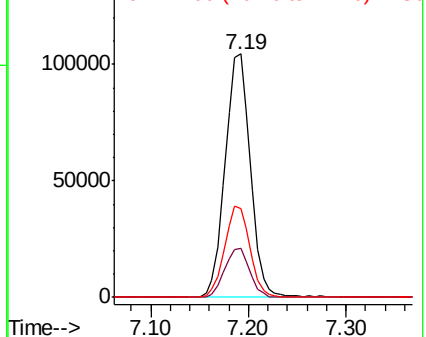

#19

n-Nitroso-di-n-propylamine

Concen: 17.506 ng

RT: 9.21 min Scan# 1041

Delta R.T. 0.37 min

Lab File: BG039067.D

Acq: 11 Jan 2019 00:33

Tgt Ion: 70 Resp: 19115


Ion Ratio Lower Upper

70 100



42 50.4 59.0 88.4#


101 0.0 10.4 15.6#

130 2.3 21.6 32.4#

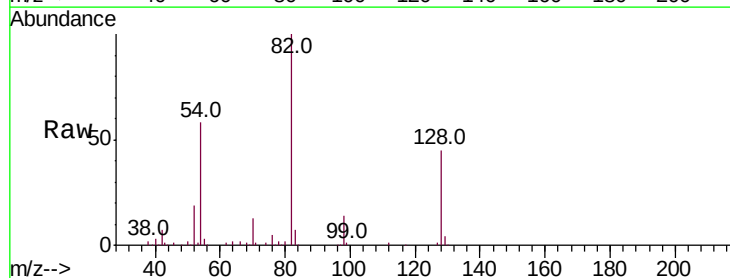

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

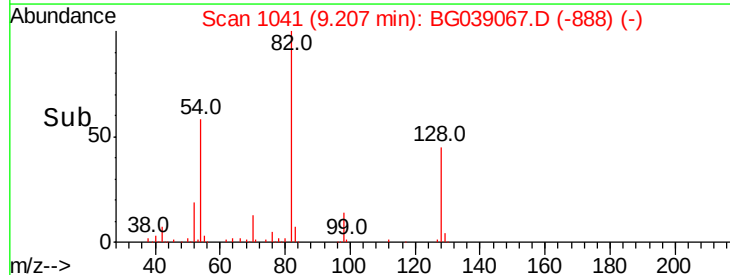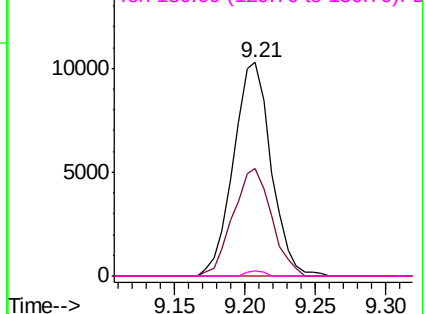







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.85 min Scan# 1320
Delta R.T. 0.00 min
Lab File: BG039067.D
Acq: 11 Jan 2019 00:33

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	91312
Ion Ratio	Lower	Upper
136	100	
137	12.3	9.4 14.2
54	9.9	7.2 10.8
68	3.8	3.5 5.3

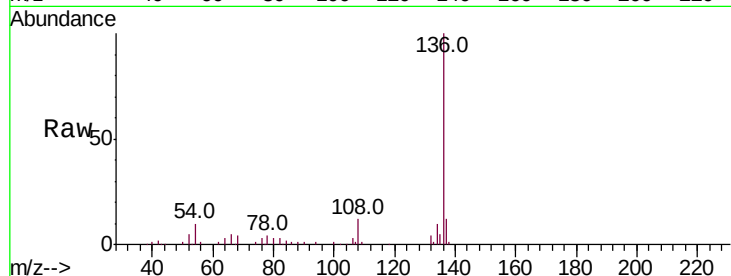


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


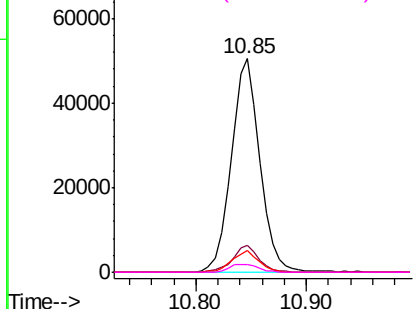



#23
Nitrobenzene-d5
Concen: 86.409 ng
RT: 9.21 min Scan# 1041
Delta R.T. -0.01 min
Lab File: BG039067.D
Acq: 11 Jan 2019 00:33

Tgt Ion: 82	Resp:	144193
Ion Ratio	Lower	Upper
82	100	
128	45.4	37.3 55.9
54	57.6	46.4 69.6



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

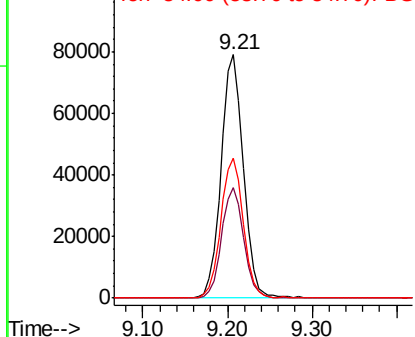

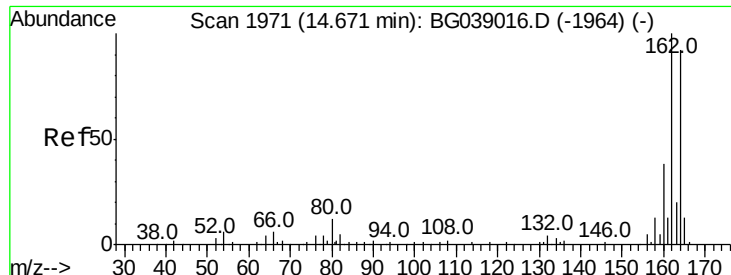

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1970

Delta R.T. -0.01 min

Lab File: BG039067.D

Acq: 11 Jan 2019 00:33

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 67569

Ion Ratio Lower Upper

164 100

162 104.2 87.2 130.8




160 45.5 33.3 49.9

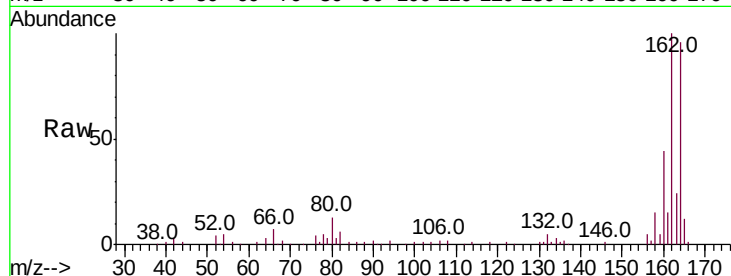

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

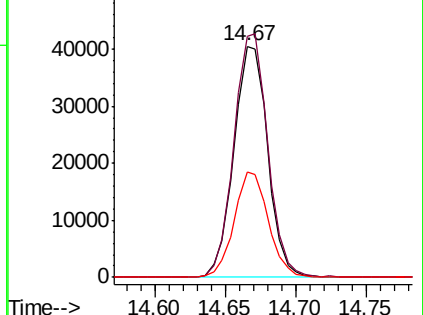

#42

2,4,6-Tribromophenol

Concen: 134.515 ng

RT: 16.16 min Scan# 2225

Delta R.T. -0.01 min

Lab File: BG039067.D

Acq: 11 Jan 2019 00:33


Tgt Ion:330 Resp: 152357

Ion Ratio Lower Upper

330 100

332 96.8 75.7 113.5



141 30.3 24.9 37.3




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

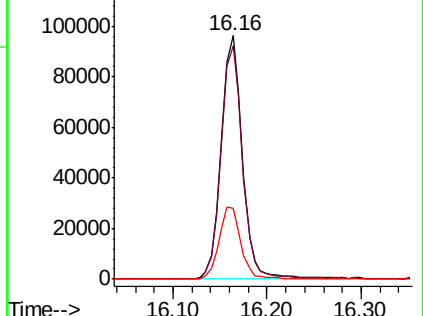


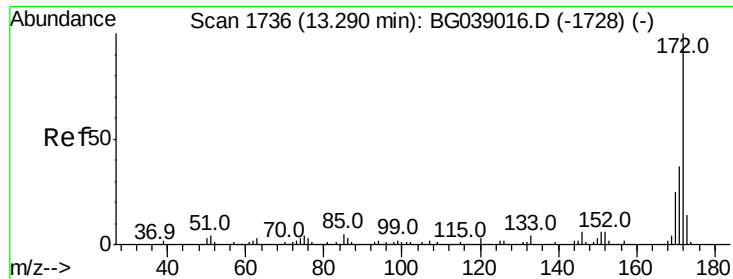




#45
 2-Fluorobiphenyl
 Concen: 85.607 ng
 RT: 13.28 min Scan# 1735
 Delta R.T. -0.01 min
 Lab File: BG039067.D
 Acq: 11 Jan 2019 00:33

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:172 Resp: 422660
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.4 44.0
 170 23.5 20.1 30.1

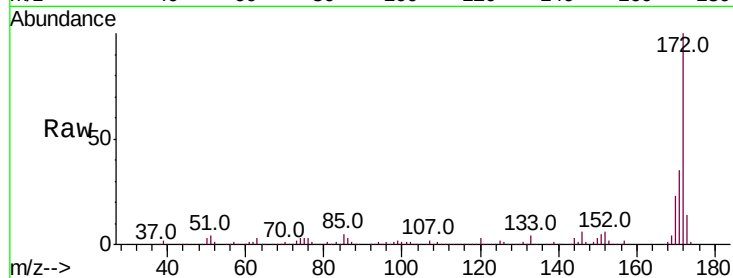


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

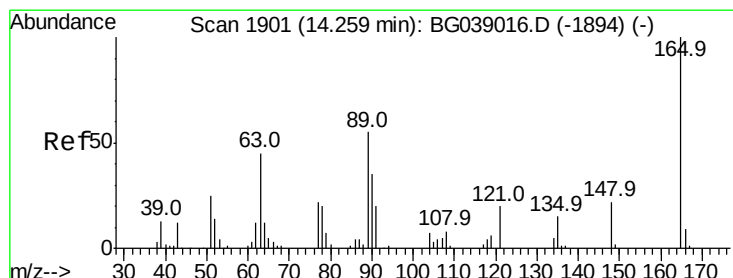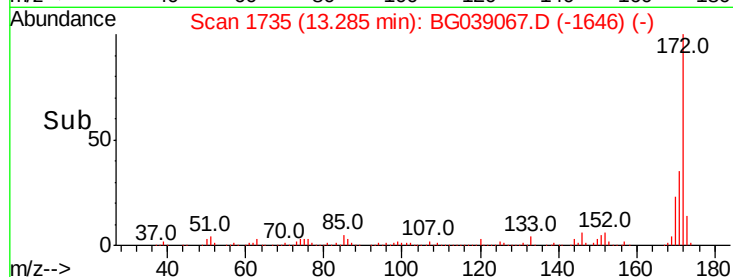
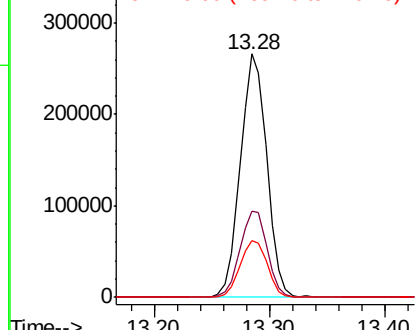



#51
 2,6-Dinitrotoluene
 Concen: 6.472 ng
 RT: 14.67 min Scan# 1970
 Delta R.T. 0.41 min
 Lab File: BG039067.D
 Acq: 11 Jan 2019 00:33

Tgt Ion:165 Resp: 8262
 Ion Ratio Lower Upper
 165 100
 63 0.0 43.6 65.4#
 89 0.0 43.7 65.5#

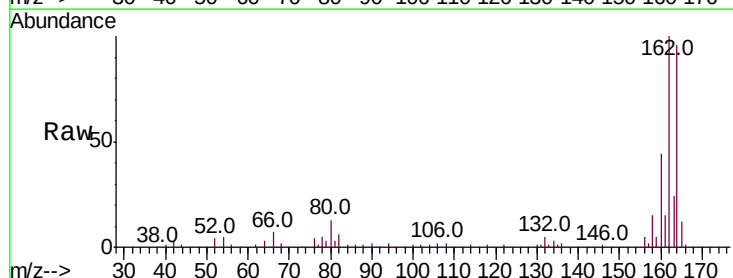

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC

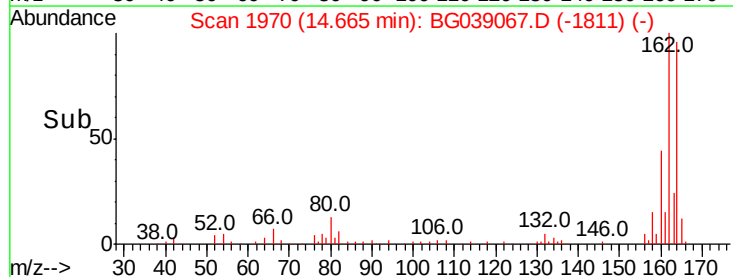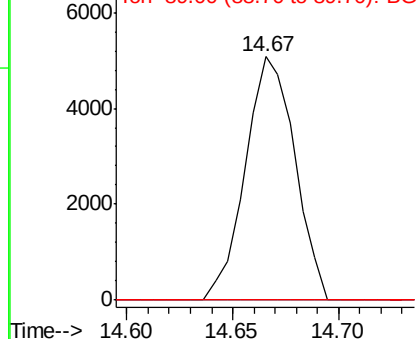







#57
 2,4-Dinitrotoluene
 Concen: 4.511 ng
 RT: 14.67 min Scan# 1970
 Delta R.T. -0.38 min
 Lab File: BG039067.D
 Acq: 11 Jan 2019 00:33

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:165 Resp: 8262
 Ion Ratio Lower Upper
 165 100
 63 0.0 30.2 45.4#
 89 0.0 53.2 79.8#
 182 0.0 2.7 4.1#

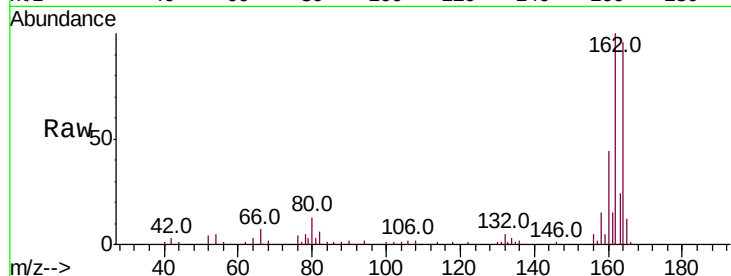


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

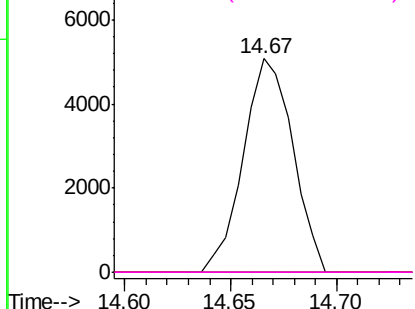




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.42 min Scan# 2439
 Delta R.T. 0.00 min
 Lab File: BG039067.D
 Acq: 11 Jan 2019 00:33

Tgt Ion:188 Resp: 177517
 Ion Ratio Lower Upper
 188 100
 94 5.9 5.0 7.4
 80 6.5 4.7 7.1



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

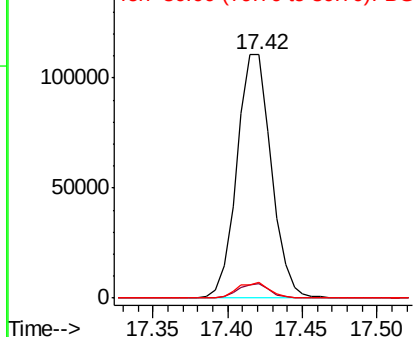


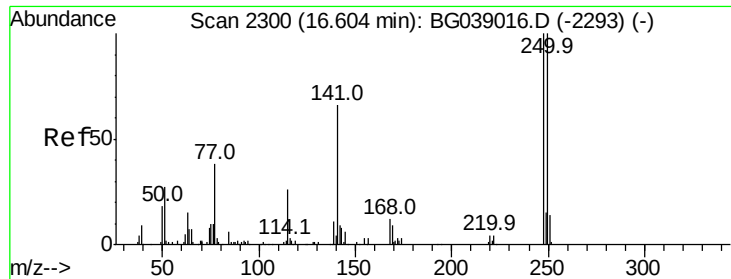




#67
 4-Bromophenyl-phenylether
 Concen: 4.420 ng
 RT: 16.16 min Scan# 2224
 Delta R.T. -0.45 min
 Lab File: BG039067.D
 Acq: 11 Jan 2019 00:33

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:248 Resp: 10086
 Ion Ratio Lower Upper
 248 100
 250 176.1 79.9 119.9#
 141 341.7 52.7 79.1#

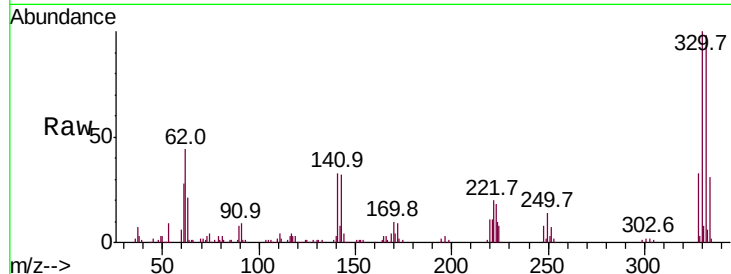


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E


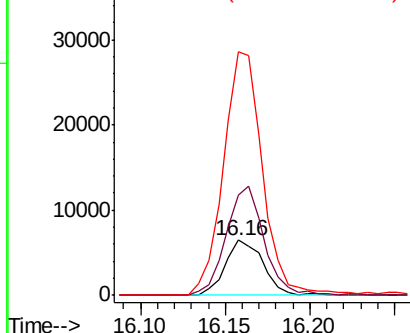



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.69 min Scan# 3166
 Delta R.T. -0.01 min
 Lab File: BG039067.D
 Acq: 11 Jan 2019 00:33

Tgt Ion:240 Resp: 183573
 Ion Ratio Lower Upper
 240 100
 120 5.6 4.3 6.5
 236 25.5 20.1 30.1



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

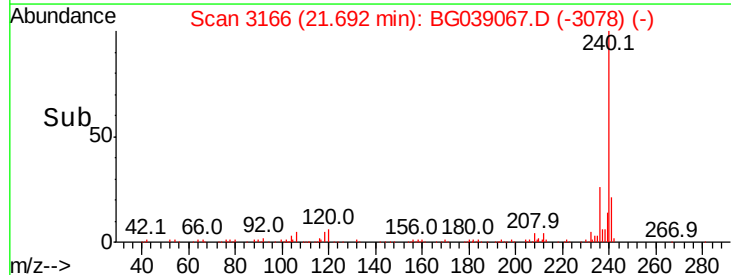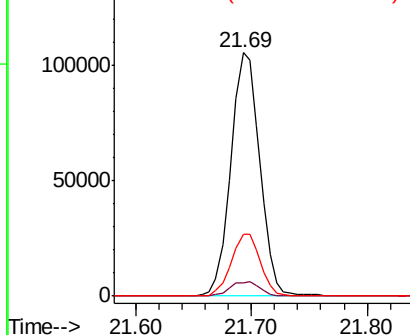

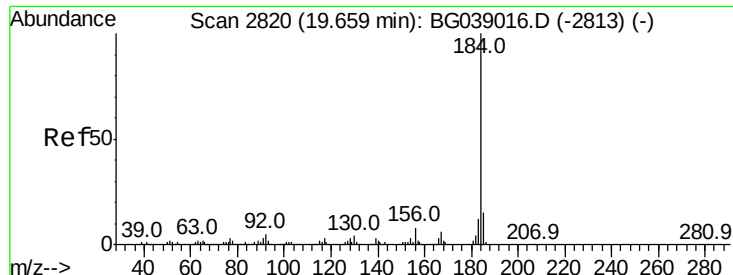

#77

Benzidine

Concen: 2.226 ng

RT: 20.02 min Scan# 2882

Delta R.T. 0.36 min

Lab File: BG039067.D

Acq: 11 Jan 2019 00:33

Instrument :

BNA_G

ClientSampleId :


Tot Ion:184 Resp: 12498

Ion Ratio Lower Upper

184 100

185 18.6 12.1 18.1#




183 11.3 9.5 14.3

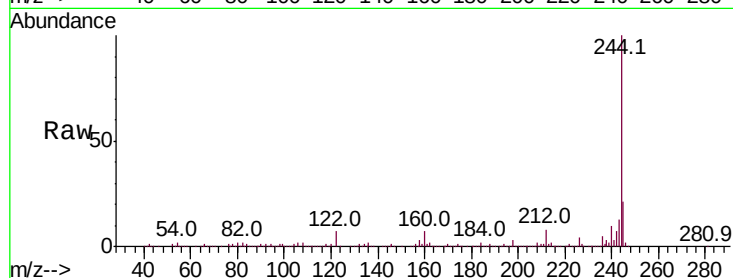

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

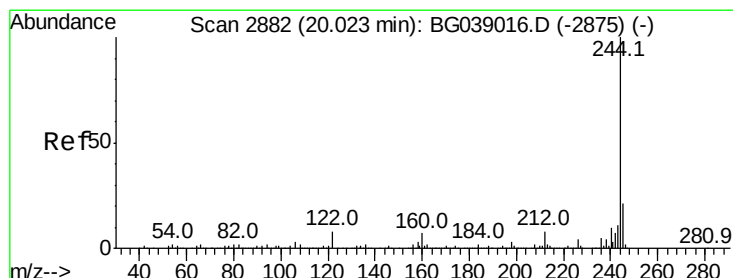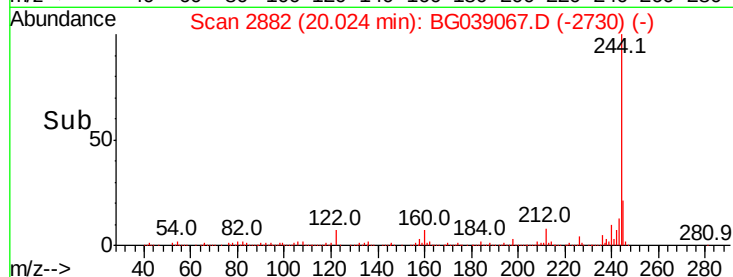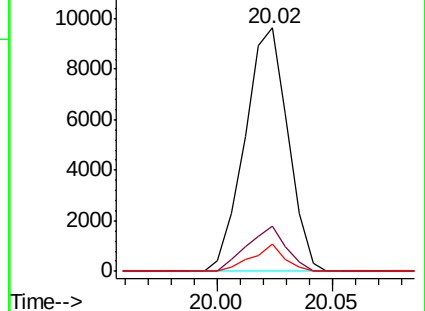

#79

Terphenyl-d14

Concen: 82.965 ng

RT: 20.02 min Scan# 2882

Delta R.T. 0.00 min

Lab File: BG039067.D

Acq: 11 Jan 2019 00:33


Tgt Ion:244 Resp: 823295

Ion Ratio Lower Upper

244 100

212 7.7 6.1 9.1



122 6.8 6.1 9.1

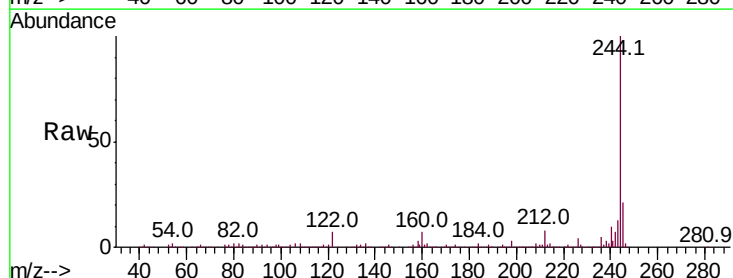


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

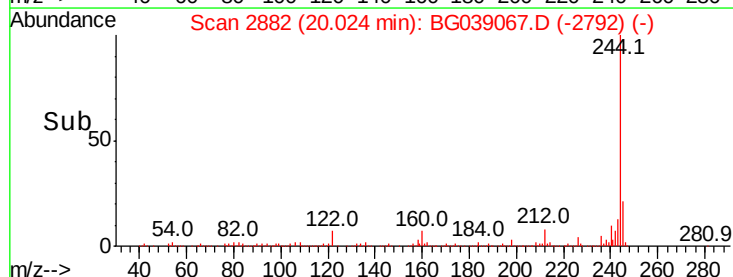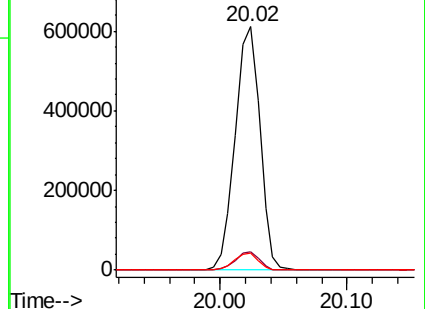


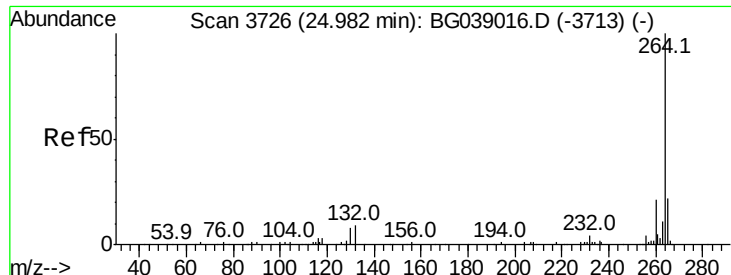

#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.98 min Scan# 3725
Delta R.T. -0.01 min
Lab File: BG039067.D
Acq: 11 Jan 2019 00:33

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.8	17.0	25.6
265	21.3	17.2	25.8



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

