

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011019\
 Data File : BG039075.D
 Acq On : 11 Jan 2019 5:48
 Operator : JU/SJ
 Sample : K1015-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SU-03-010918-B

Quant Time: Jan 11 06:55:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 09 14:23:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	22049	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	82778	20.00	ng	0.00
39) Acenaphthene-d10	14.67	164	56839	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	154616	20.00	ng	0.00
76) Chrysene-d12	21.69	240	177020	20.00	ng	-0.01
87) Perylene-d12	24.97	264	187761	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.58	112	164299	141.35	ng	0.00
7) Phenol-d6	7.19	99	196574	117.52	ng	0.00
23) Nitrobenzene-d5	9.21	82	148874	98.41	ng	0.00
42) 2,4,6-Tribromophenol	16.16	330	145152	152.35	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	404543	97.41	ng	0.00
79) Terphenyl-d14	20.02	244	883933	92.37	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011019\
Data File : BG039075.D
Acq On : 11 Jan 2019 5:48
Operator : JU/SJ
Sample : K1015-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SU-03-010918-B

Quant Time: Jan 11 06:55:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

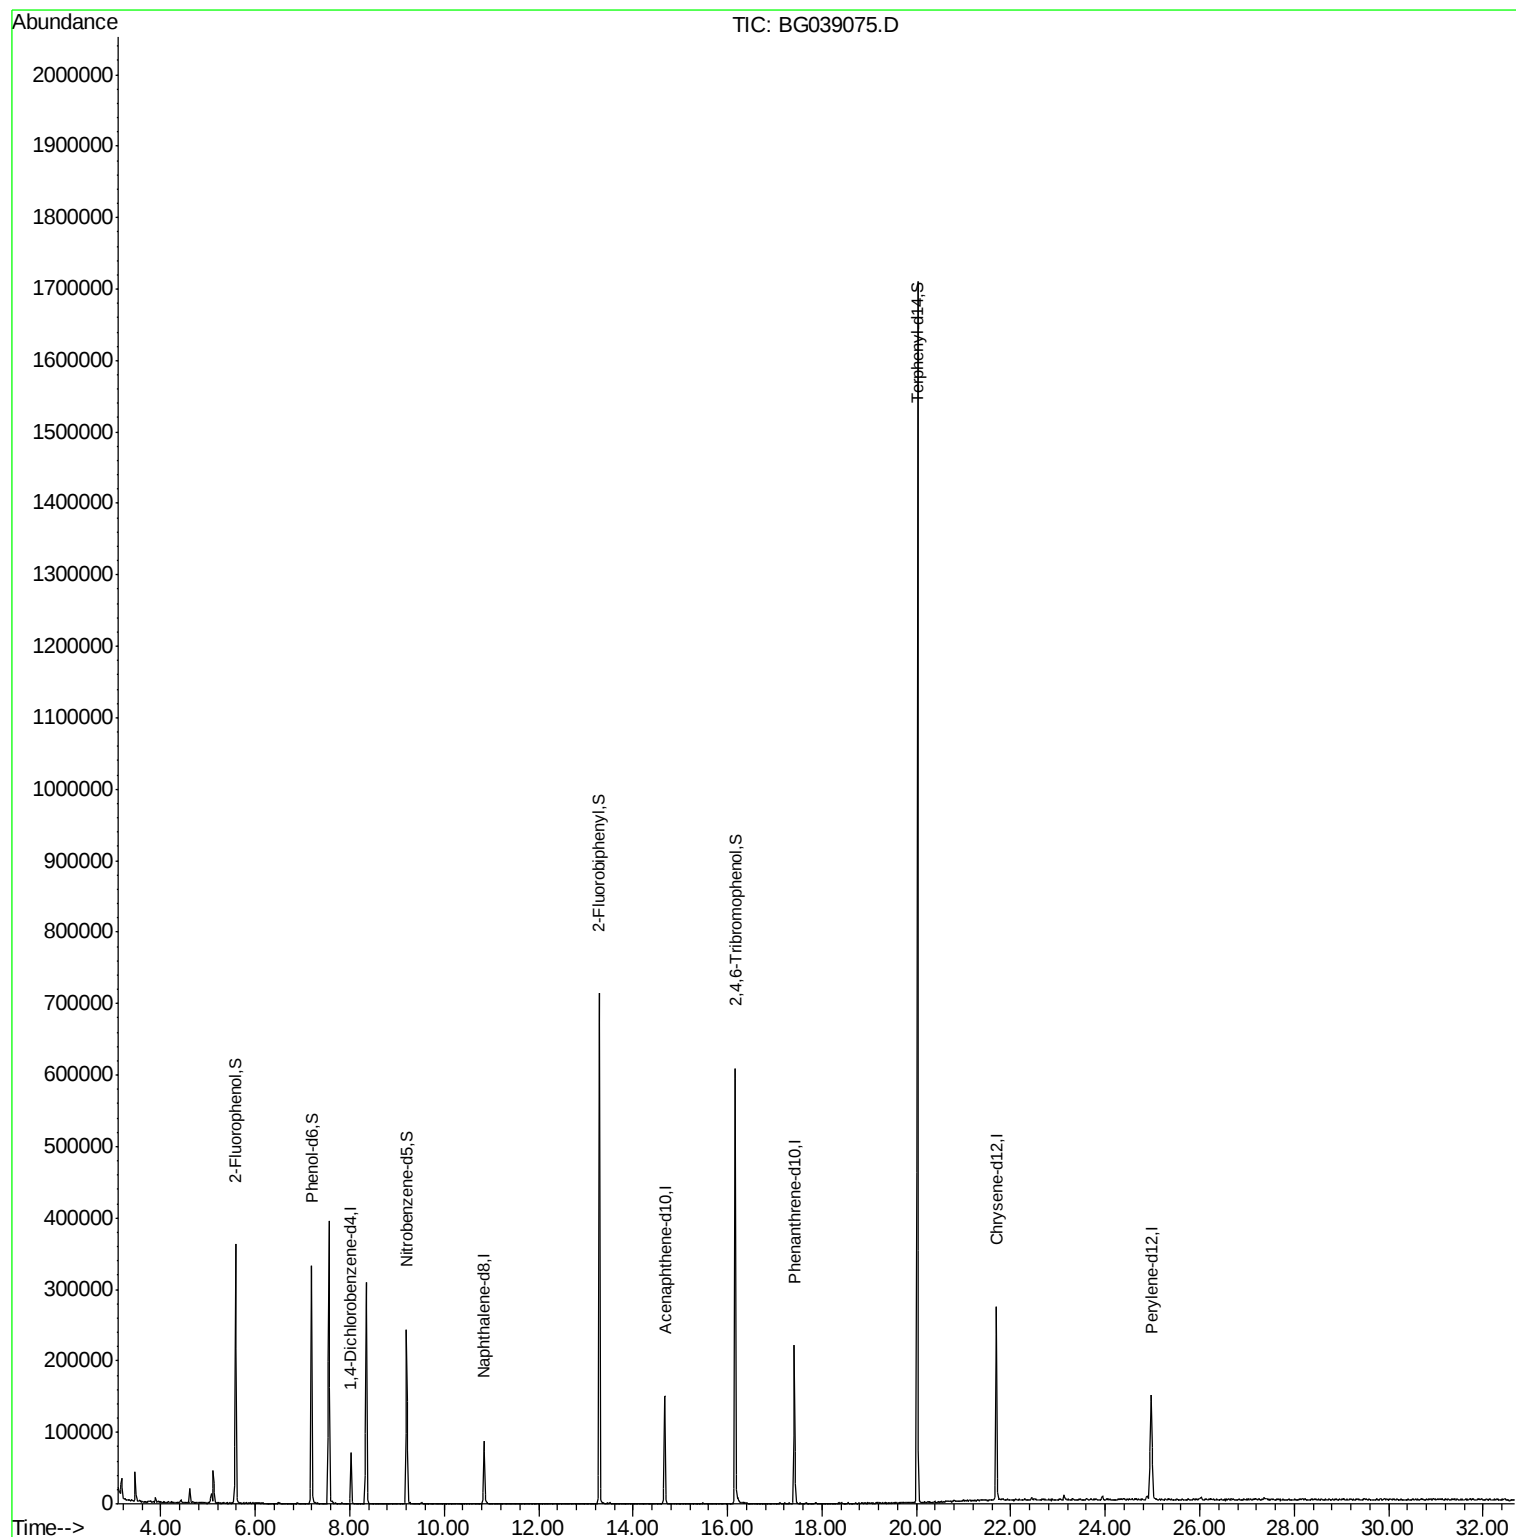

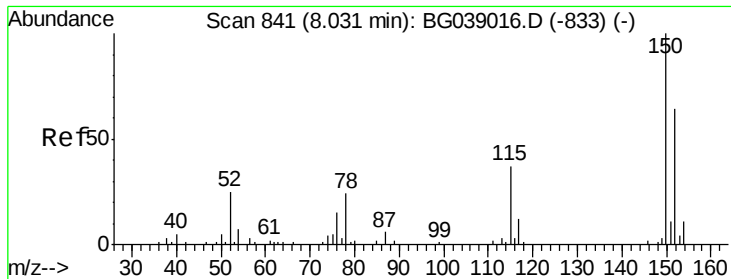


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.03 min Scan# 840
Delta R.T. -0.01 min
Lab File: BG039075.D
Acq: 11 Jan 2019 5:48

Instrument :
BNA_G
ClientSampleId :
SU-03-010918-B

Tot Ion:152 Resp: 22049
Ion Ratio Lower Upper
152 100
150 151.2 124.7 187.1
115 55.9 46.5 69.7

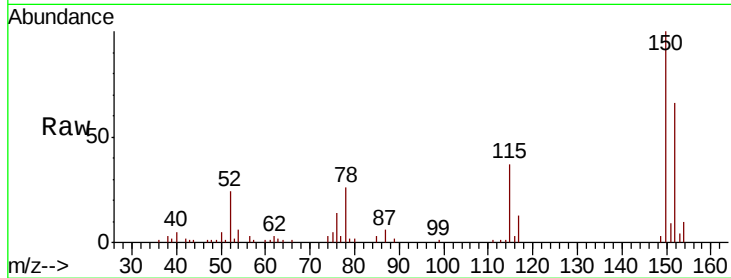


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

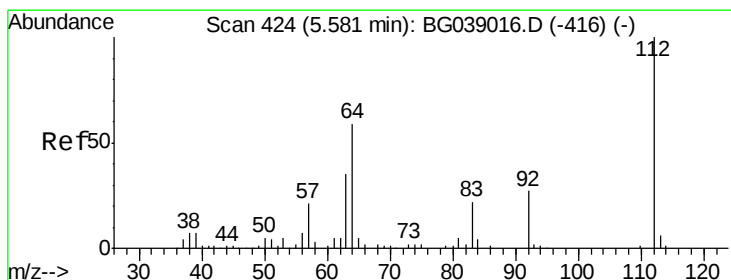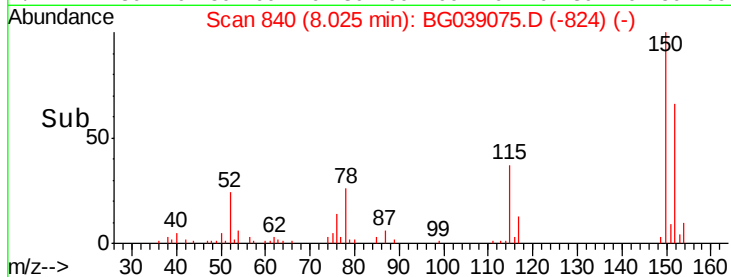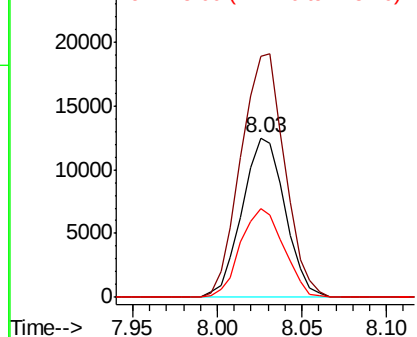



#5


2-Fluorophenol
Concen: 141.354 ng
RT: 5.58 min Scan# 424
Delta R.T. -0.00 min
Lab File: BG039075.D
Acq: 11 Jan 2019 5:48

Tgt Ion:112 Resp: 164299
Ion Ratio Lower Upper
112 100
64 59.2 47.0 70.6
63 32.8 28.0 42.0

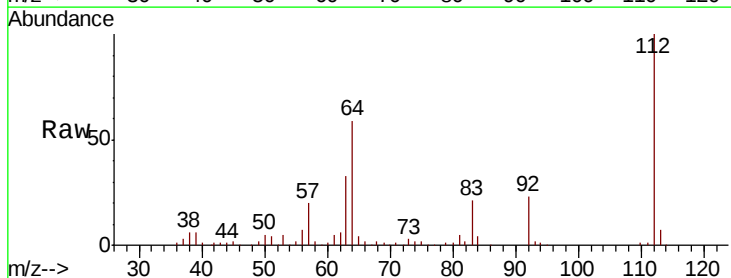

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

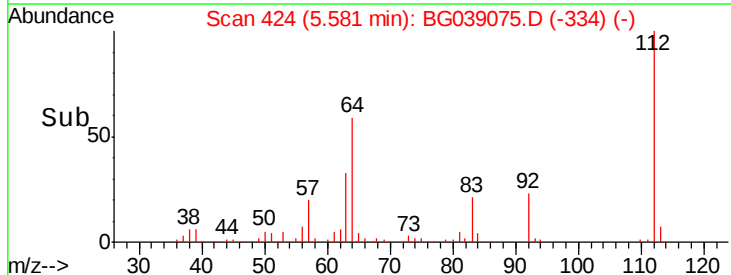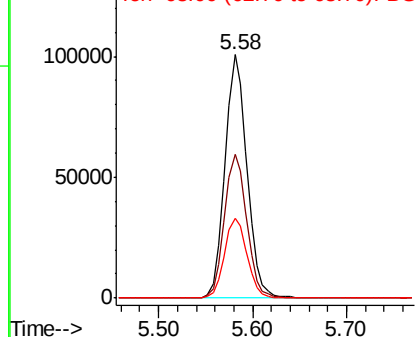

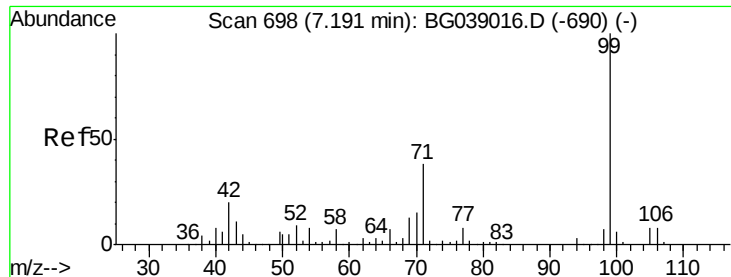

#7

Phenol-d6

Concen: 117.517 ng

RT: 7.19 min Scan# 698

Delta R.T. -0.00 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48

Instrument :

BNA_G

ClientSampleId :

SU-03-010918-B


Tot Ion: 99 Resp: 196574

Ion Ratio Lower Upper




99 100

42 19.6 15.8 23.6

71 39.4 30.2 45.4

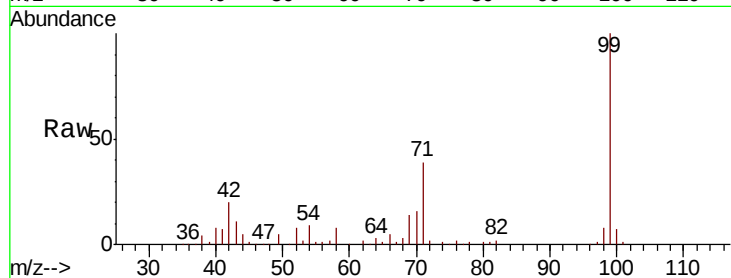

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

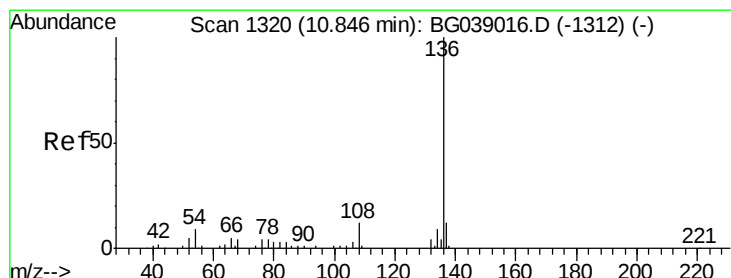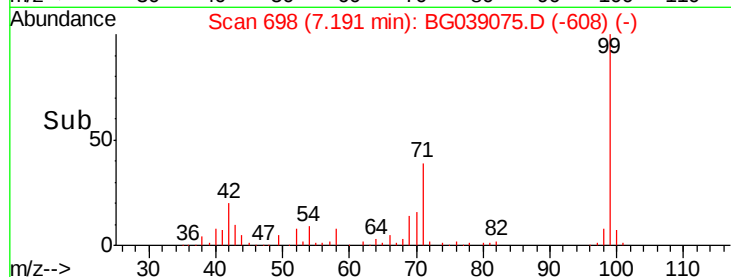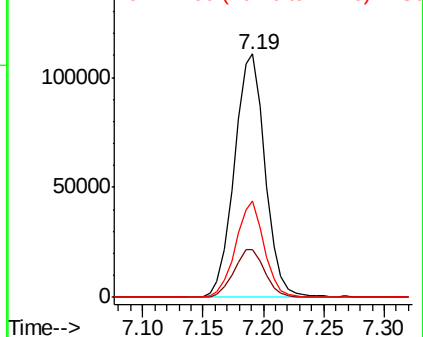

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1320

Delta R.T. -0.00 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48

Tgt Ion: 136 Resp: 82778


Ion Ratio Lower Upper

136 100



137 11.4 9.4 14.2


54 8.6 7.2 10.8

68 3.9 3.5 5.3

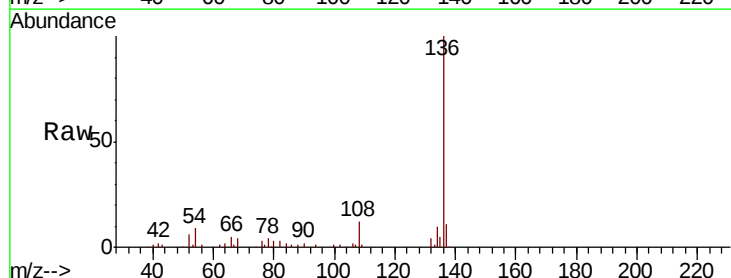

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



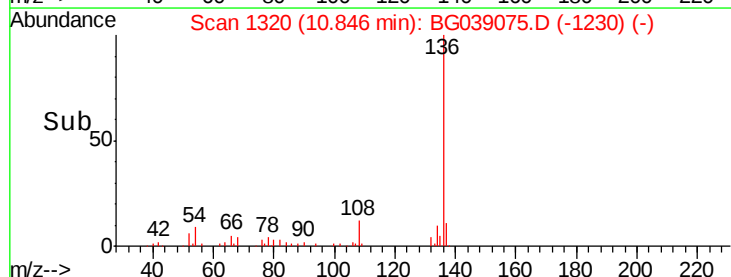
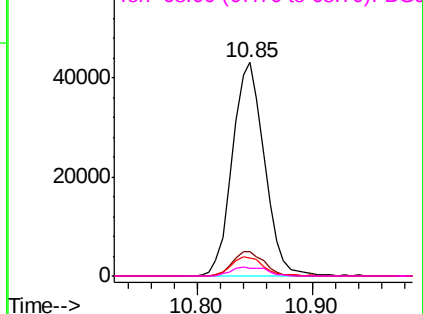


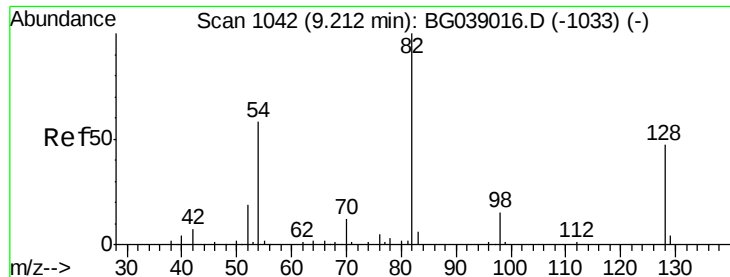

#23
Nitrobenzene-d5
Concen: 98.411 ng
RT: 9.21 min Scan# 1041
Delta R.T. -0.01 min
Lab File: BG039075.D
Acq: 11 Jan 2019 5:48




Instrument :
BNA_G
ClientSampleId :
SU-03-010918-B


Tot Ion: 82 Resp: 148874
Ion Ratio Lower Upper
82 100
128 46.0 37.3 55.9
54 57.3 46.4 69.6

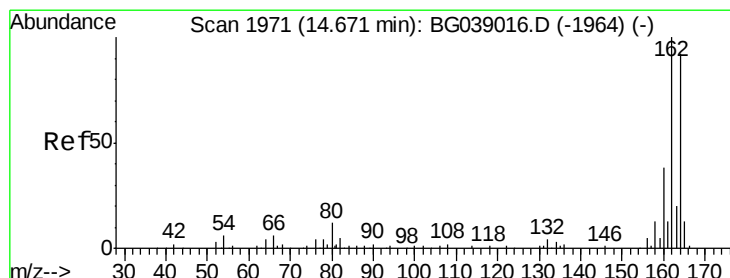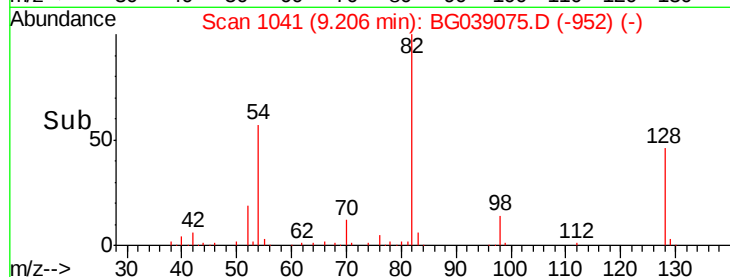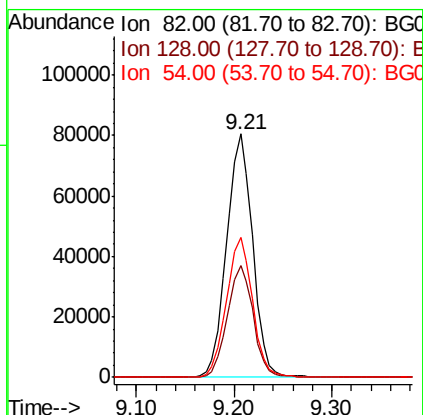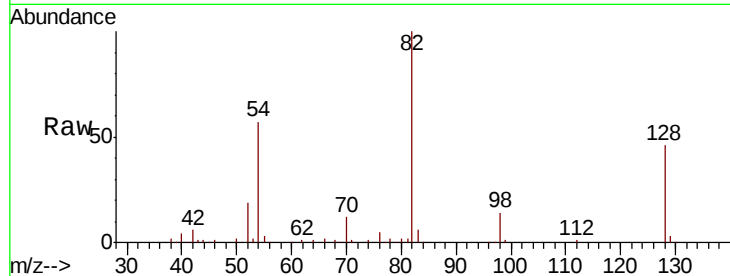

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1971
Delta R.T. -0.00 min
Lab File: BG039075.D
Acq: 11 Jan 2019 5:48

Tgt Ion: 164 Resp: 56839
Ion Ratio Lower Upper
164 100
162 102.6 87.2 130.8
160 44.8 33.3 49.9

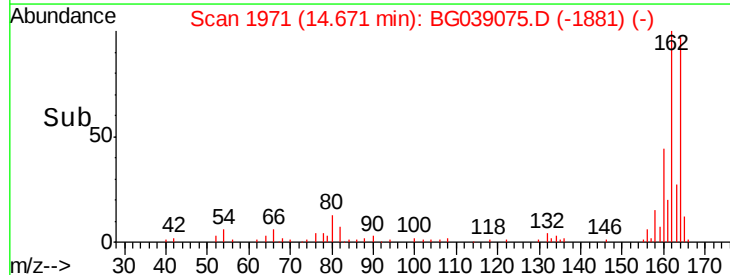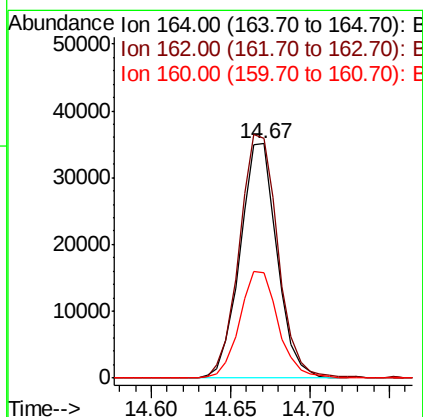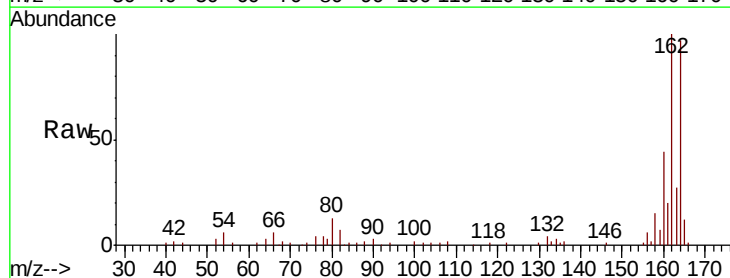

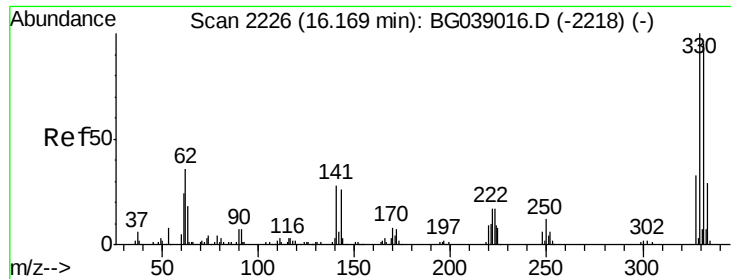

#42

2,4,6-Tribromophenol

Concen: 152.346 ng

RT: 16.16 min Scan# 2225

Delta R.T. -0.01 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48

Instrument :

BNA_G

ClientSampleId :

SU-03-010918-B


Tot Ion:330 Resp: 145152

Ion Ratio Lower Upper

330 100

332 96.2 75.7 113.5




141 30.2 24.9 37.3

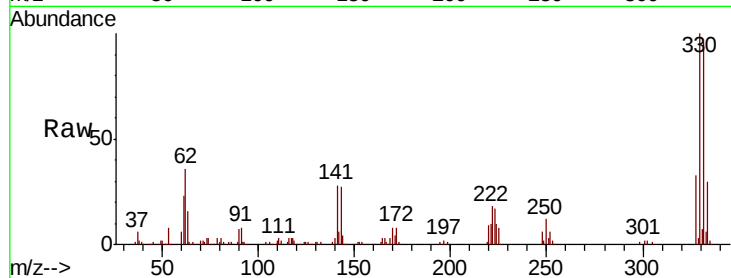

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

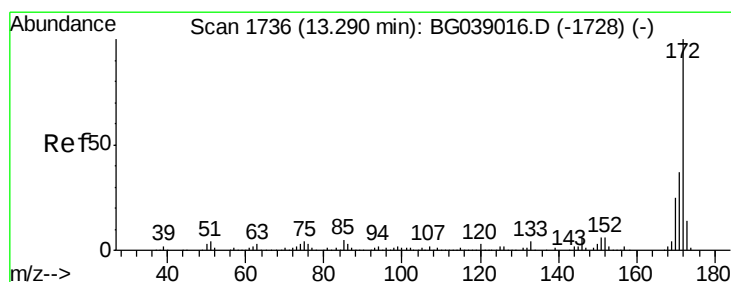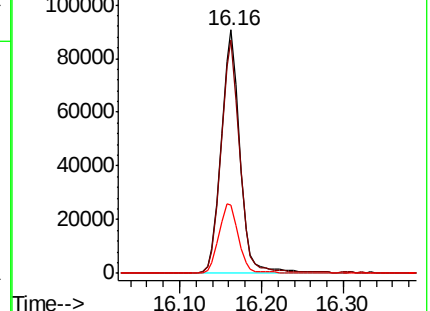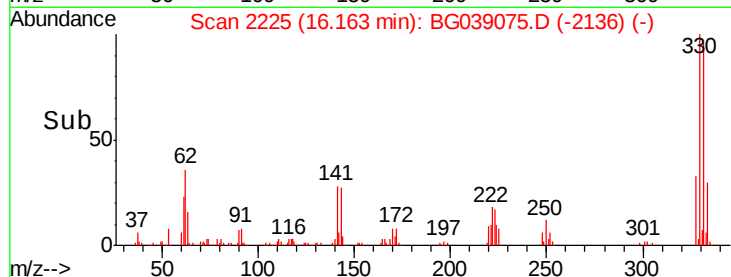

#45

2-Fluorobiphenyl

Concen: 97.405 ng

RT: 13.28 min Scan# 1735

Delta R.T. -0.01 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48


Tgt Ion:172 Resp: 404543

Ion Ratio Lower Upper

172 100

171 37.6 29.4 44.0



170 24.3 20.1 30.1

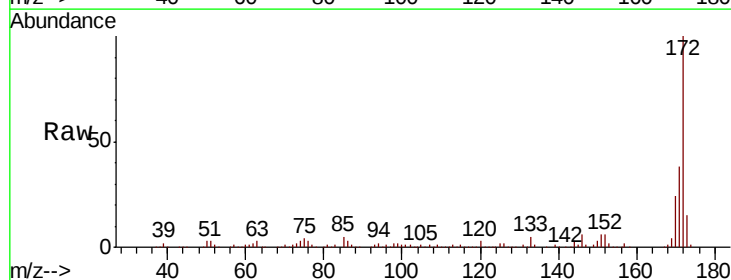

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

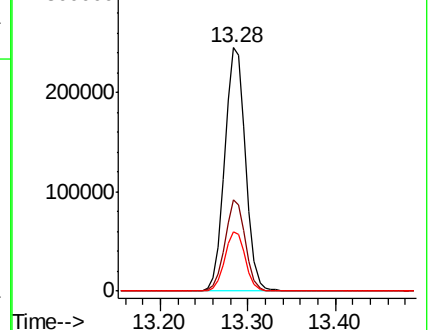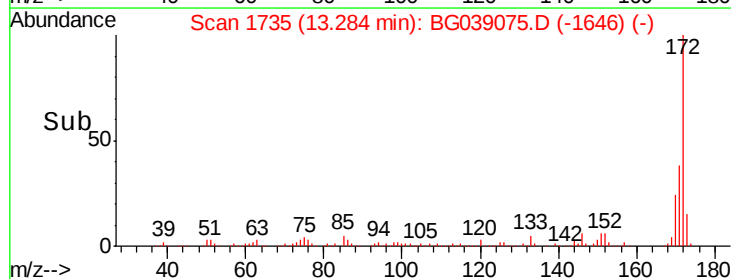



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.41 min Scan# 2438

Delta R.T. -0.01 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48

Instrument :

BNA_G

ClientSampleId :

SU-03-010918-B


Tot Ion:188 Resp: 154616

Ion Ratio Lower Upper

188 100

94 5.7 5.0 7.4




80 6.5 4.7 7.1

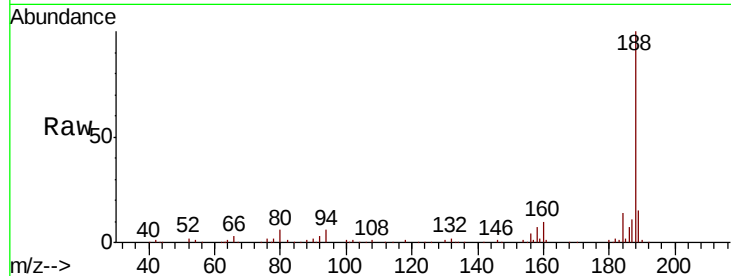

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

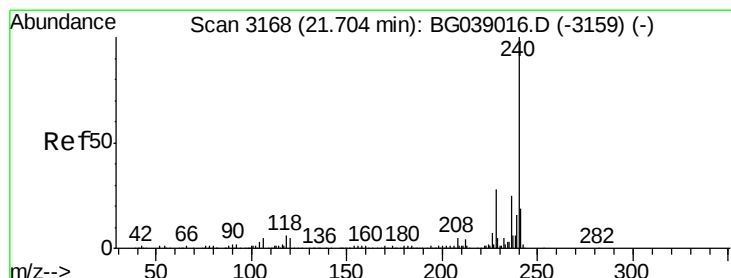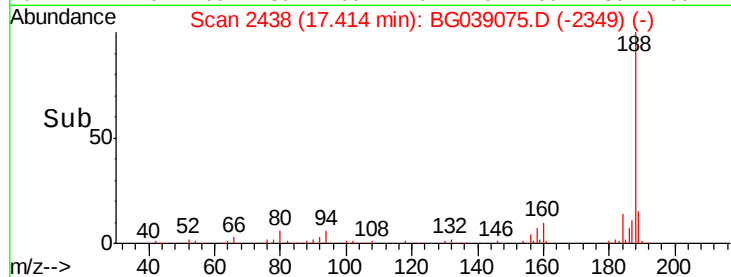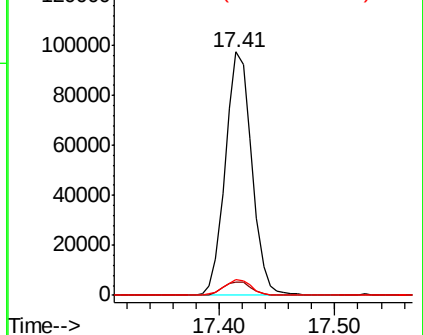

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3166

Delta R.T. -0.01 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48


Tgt Ion:240 Resp: 177020

Ion Ratio Lower Upper

240 100

120 6.4 4.3 6.5



236 26.0 20.1 30.1

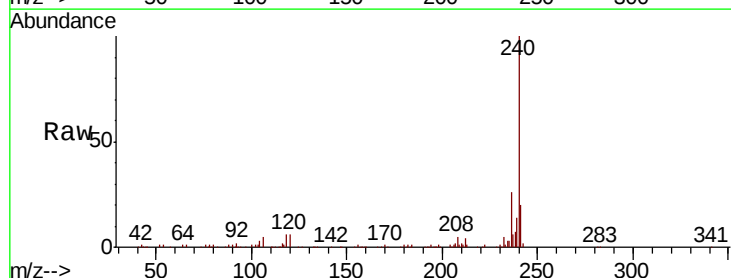


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

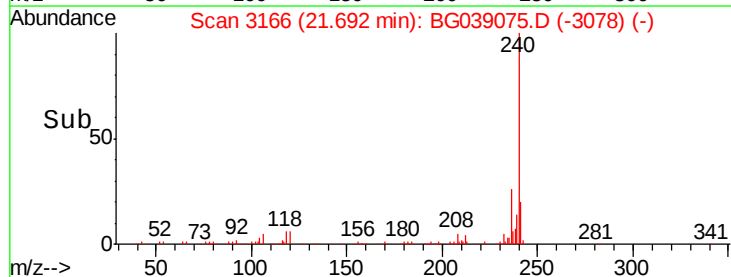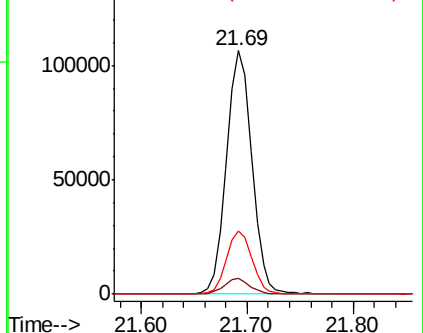

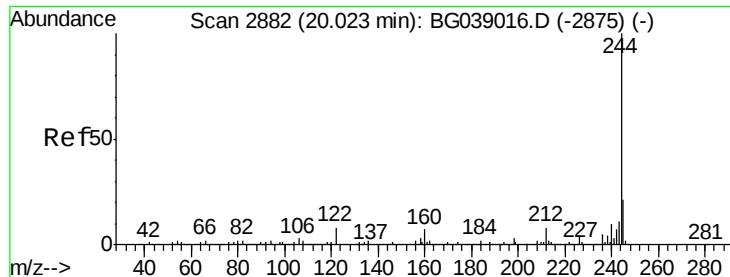

#79

Terphenyl-d14

Concen: 92.373 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.00 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48

Instrument :

BNA_G

ClientSampleId :

SU-03-010918-B


Tot Ion:244 Resp: 883933

Ion Ratio Lower Upper

244 100

212 7.5 6.1 9.1


122 7.0 6.1 9.1

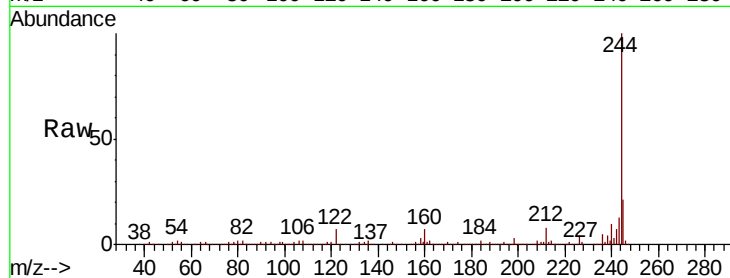



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

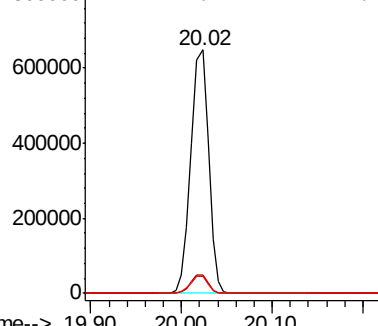

Time--> 19.90 20.00 20.10

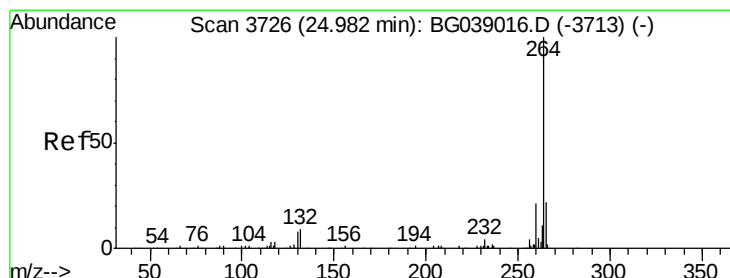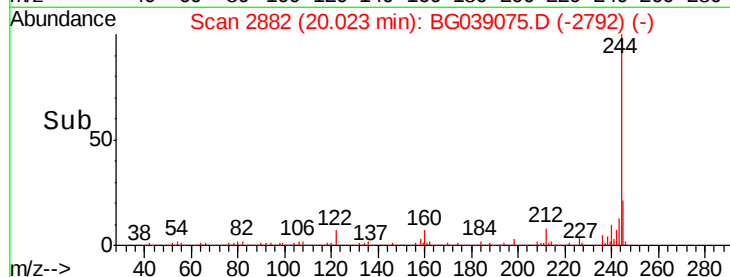

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.97 min Scan# 3724

Delta R.T. -0.01 min

Lab File: BG039075.D

Acq: 11 Jan 2019 5:48


Tgt Ion:264 Resp: 187761

Ion Ratio Lower Upper

264 100

260 23.2 17.0 25.6


265 21.1 17.2 25.8

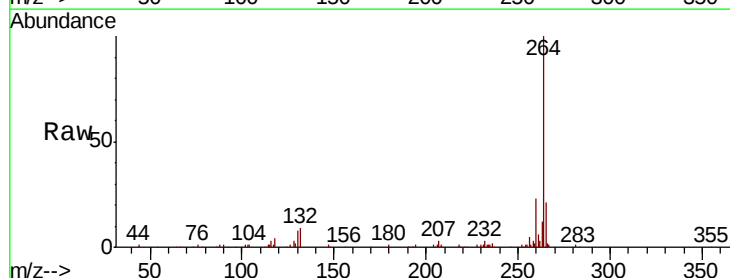

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

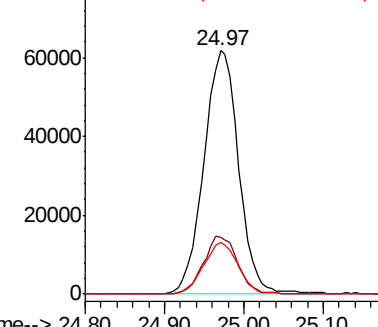

Time--> 24.80 24.90 25.00 25.10

